

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
 Data File : VV038102.D
 Acq On : 14 Nov 2024 22:08
 Operator : SY/MD
 Sample : P4761-15 2X
 Misc : 26mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 15 00:35:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 00:15:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	3552	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	3576	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	1807	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	2337	0.635	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	= 126.000%	
4) 1,2-Dichloroethane-d4	4.969	65	1621	0.728	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	= 146.000%#	
7) 1,2-Dichloropropane-d6	5.995	67	1645	0.568	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	= 114.000%	
8) Toluene-d8	7.253	98	3945	0.532	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	= 106.000%	
10) 1,1,2,2-Tetrachloroeth...	10.146	84	2026	0.875	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	= 174.000%#	
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.339	75	12	0.038	ug/L	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
Data File : VV038102.D
Acq On : 14 Nov 2024 22:08
Operator : SY/MD
Sample : P4761-15 2X
Misc : 26mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Nov 15 00:35:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

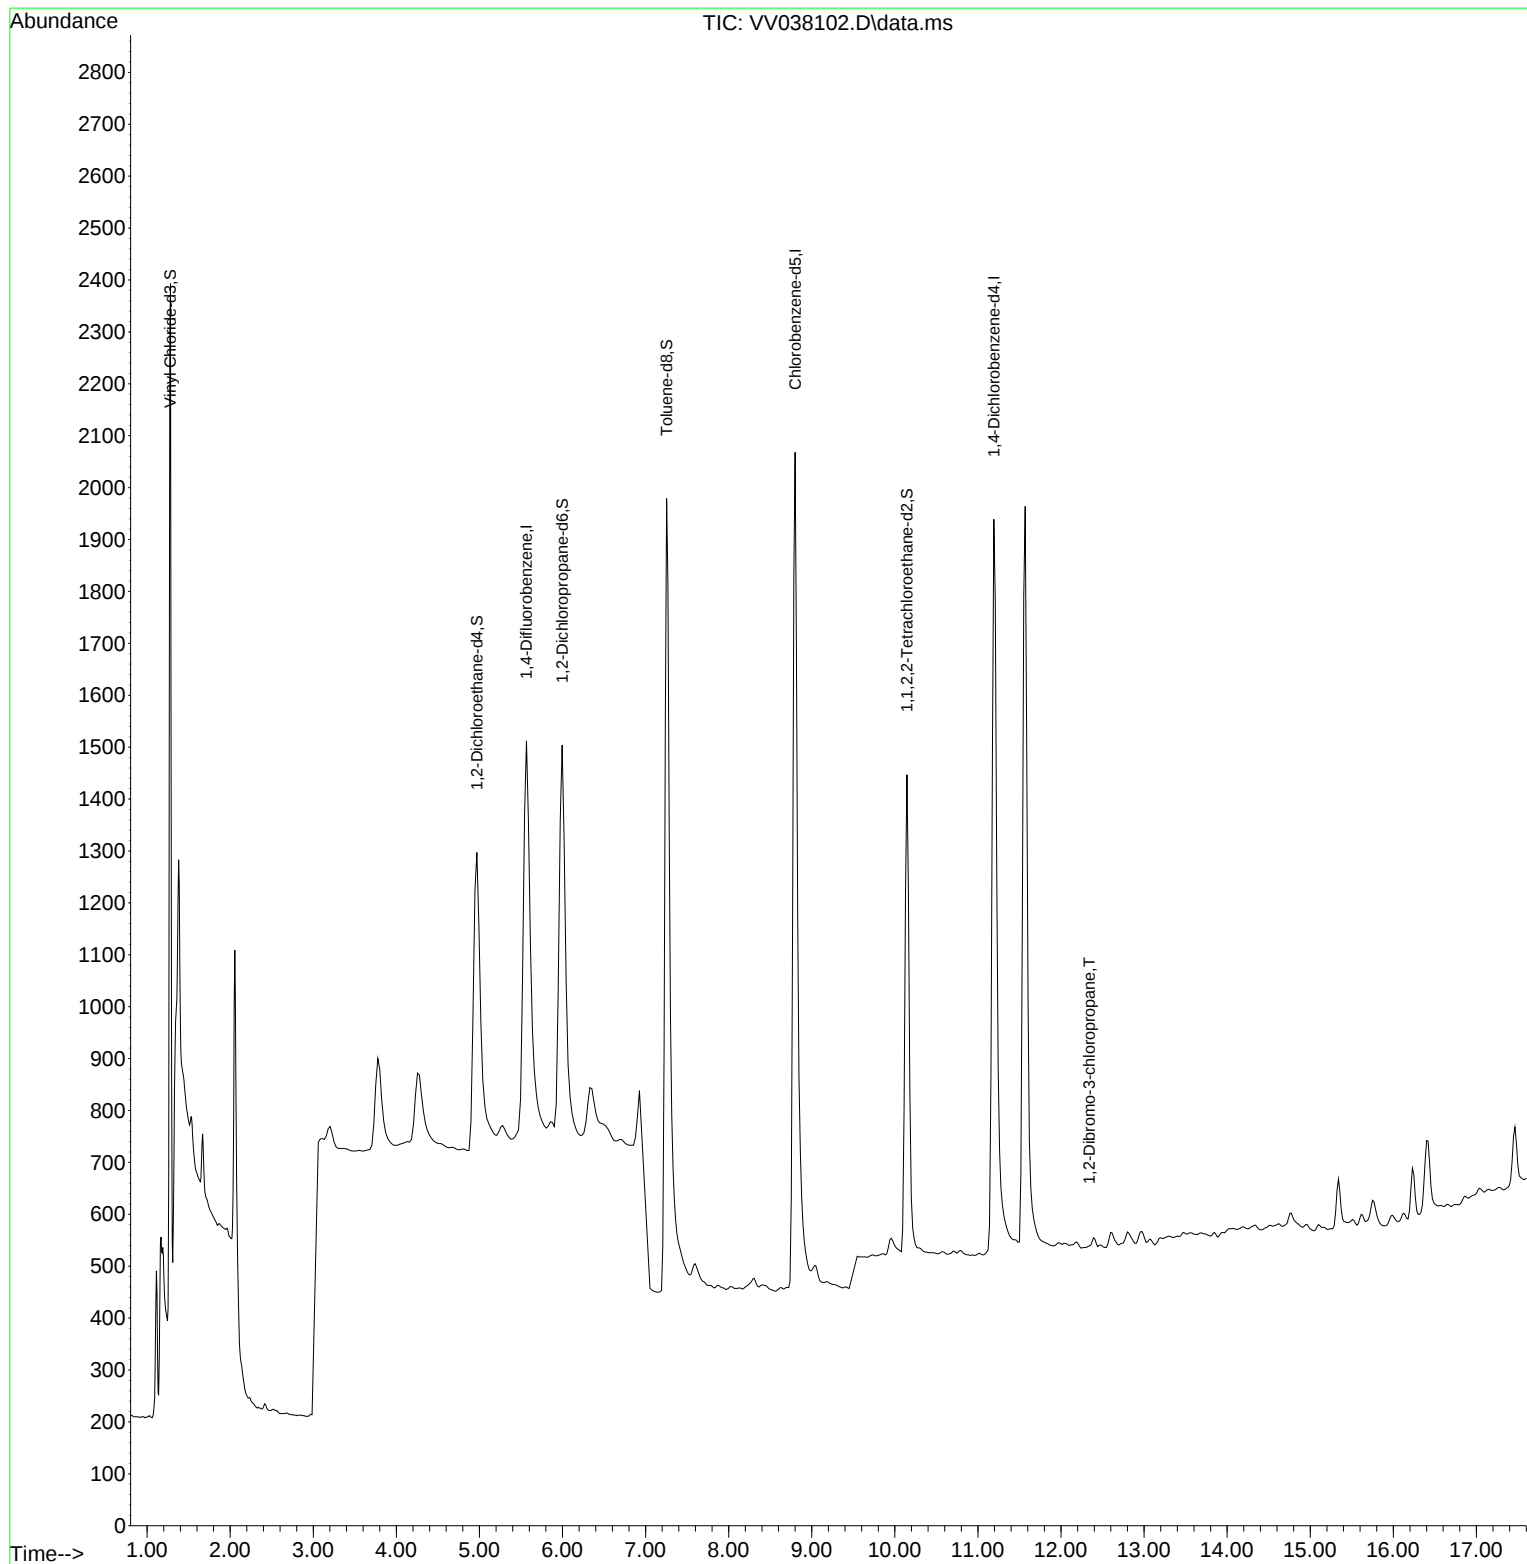

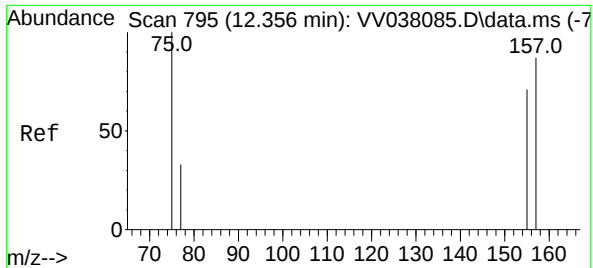

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.038 ug/L
 RT: 12.339 min Scan# 794
 Delta R.T. -0.017 min
 Lab File: VV038102.D
 Acq: 14 Nov 2024 22:08

Instrument :
 MSVOA_V
 ClientSampleId :

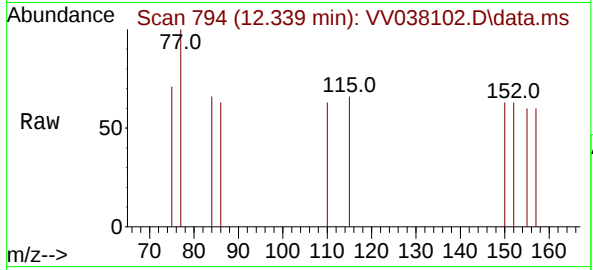

Tgt Ion: 75 Resp: 12

Ion	Ratio	Lower	Upper
75	100		
157	84.2	69.4	104.0
155	84.2	61.3	91.9

