

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
 Data File : VV038103.D
 Acq On : 14 Nov 2024 22:32
 Operator : SY/MD
 Sample : P4761-17 2X
 Misc : 26mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 15 00:35:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 00:15:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	9492	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.785	117	9765	0.500	ug/L	#-0.02
11) 1,4-Dichlorobenzene-d4	11.191	152	4901	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.273	65	5976	0.607	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	122.000%
4) 1,2-Dichloroethane-d4	4.969	65	3483	0.585	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	116.000%
7) 1,2-Dichloropropane-d6	5.995	67	4405	0.557	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	112.000%
8) Toluene-d8	7.253	98	11055	0.546	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	110.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	3483	0.551	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	110.000%
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.305	75	26	0.031	ug/L	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
Data File : VV038103.D
Acq On : 14 Nov 2024 22:32
Operator : SY/MD
Sample : P4761-17 2X
Misc : 26mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Nov 15 00:35:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

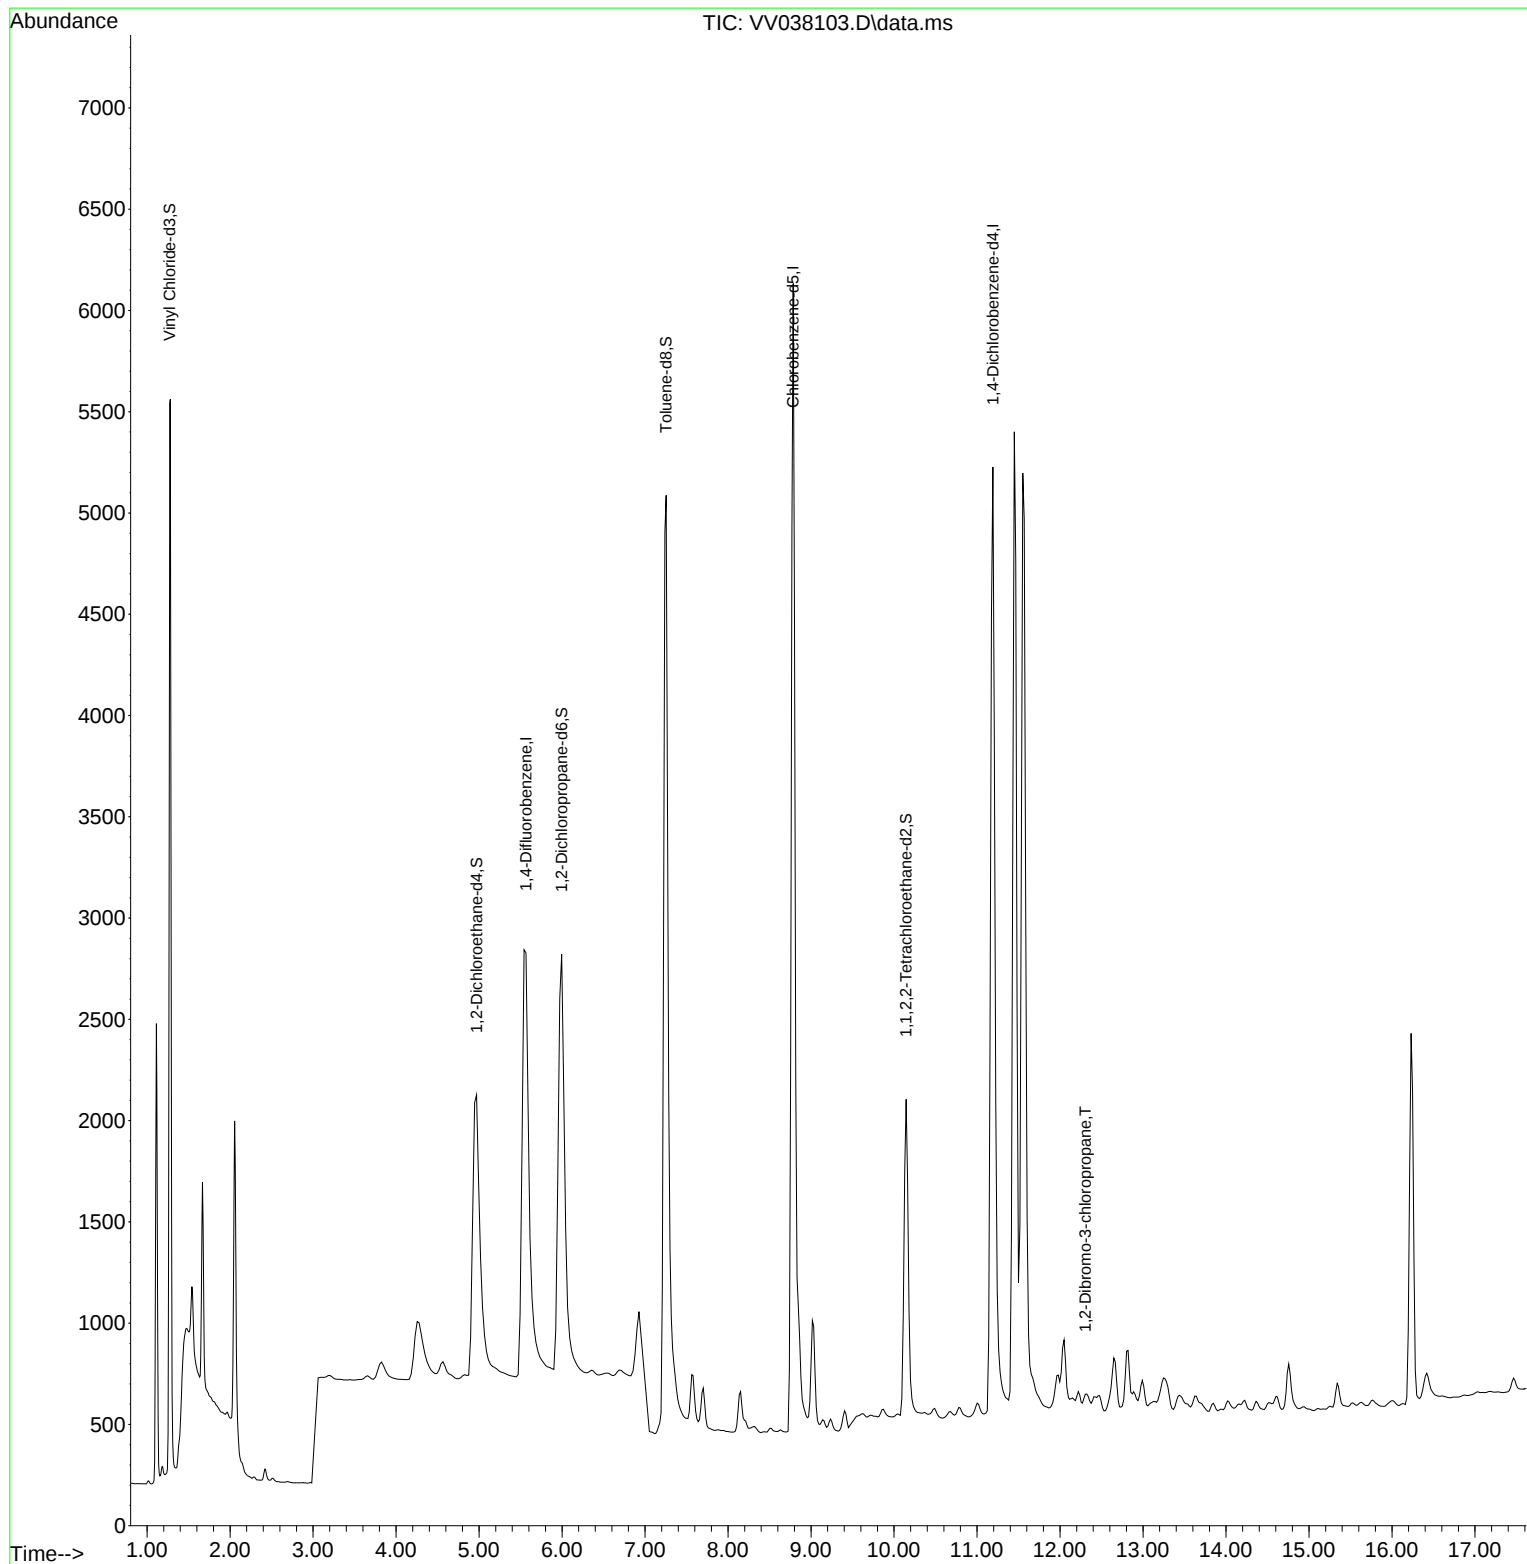

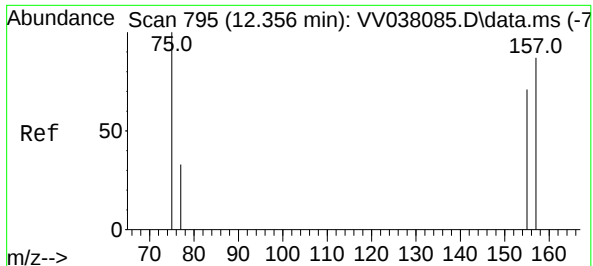

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.031 ug/L
 RT: 12.305 min Scan# 792
 Delta R.T. -0.051 min
 Lab File: VV038103.D
 Acq: 14 Nov 2024 22:32

Instrument :
 MSVOA_V
 ClientSampleId :

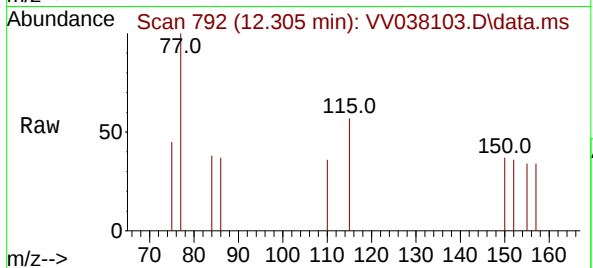

Tgt Ion: 75 Resp: 26
 Ion Ratio Lower Upper
 75 100
 157 73.8 69.4 104.0
 155 73.8 61.3 91.9

