

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
 Data File : VV038105.D
 Acq On : 14 Nov 2024 23:20
 Operator : SY/MD
 Sample : P4761-20 5X
 Misc : 26mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 15 00:35:43 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 00:15:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	9969	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.785	117	10687	0.500	ug/L	-0.02
11) 1,4-Dichlorobenzene-d4	11.191	152	5340	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	5826	0.564	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	112.000%
4) 1,2-Dichloroethane-d4	4.945	65	3523	0.563	ug/L	-0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	112.000%
7) 1,2-Dichloropropane-d6	5.995	67	4516	0.522	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	104.000%
8) Toluene-d8	7.253	98	11188	0.505	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	100.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	3461	0.500	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	100.000%
Target Compounds						
					Qvalue	
3) Vinyl chloride	1.280	62	214	0.021	ug/L #	21
13) 1,2-Dibromo-3-chloropr...	12.339	75	20	0.022	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
Data File : VV038105.D
Acq On : 14 Nov 2024 23:20
Operator : SY/MD
Sample : P4761-20 5X
Misc : 26mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Nov 15 00:35:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

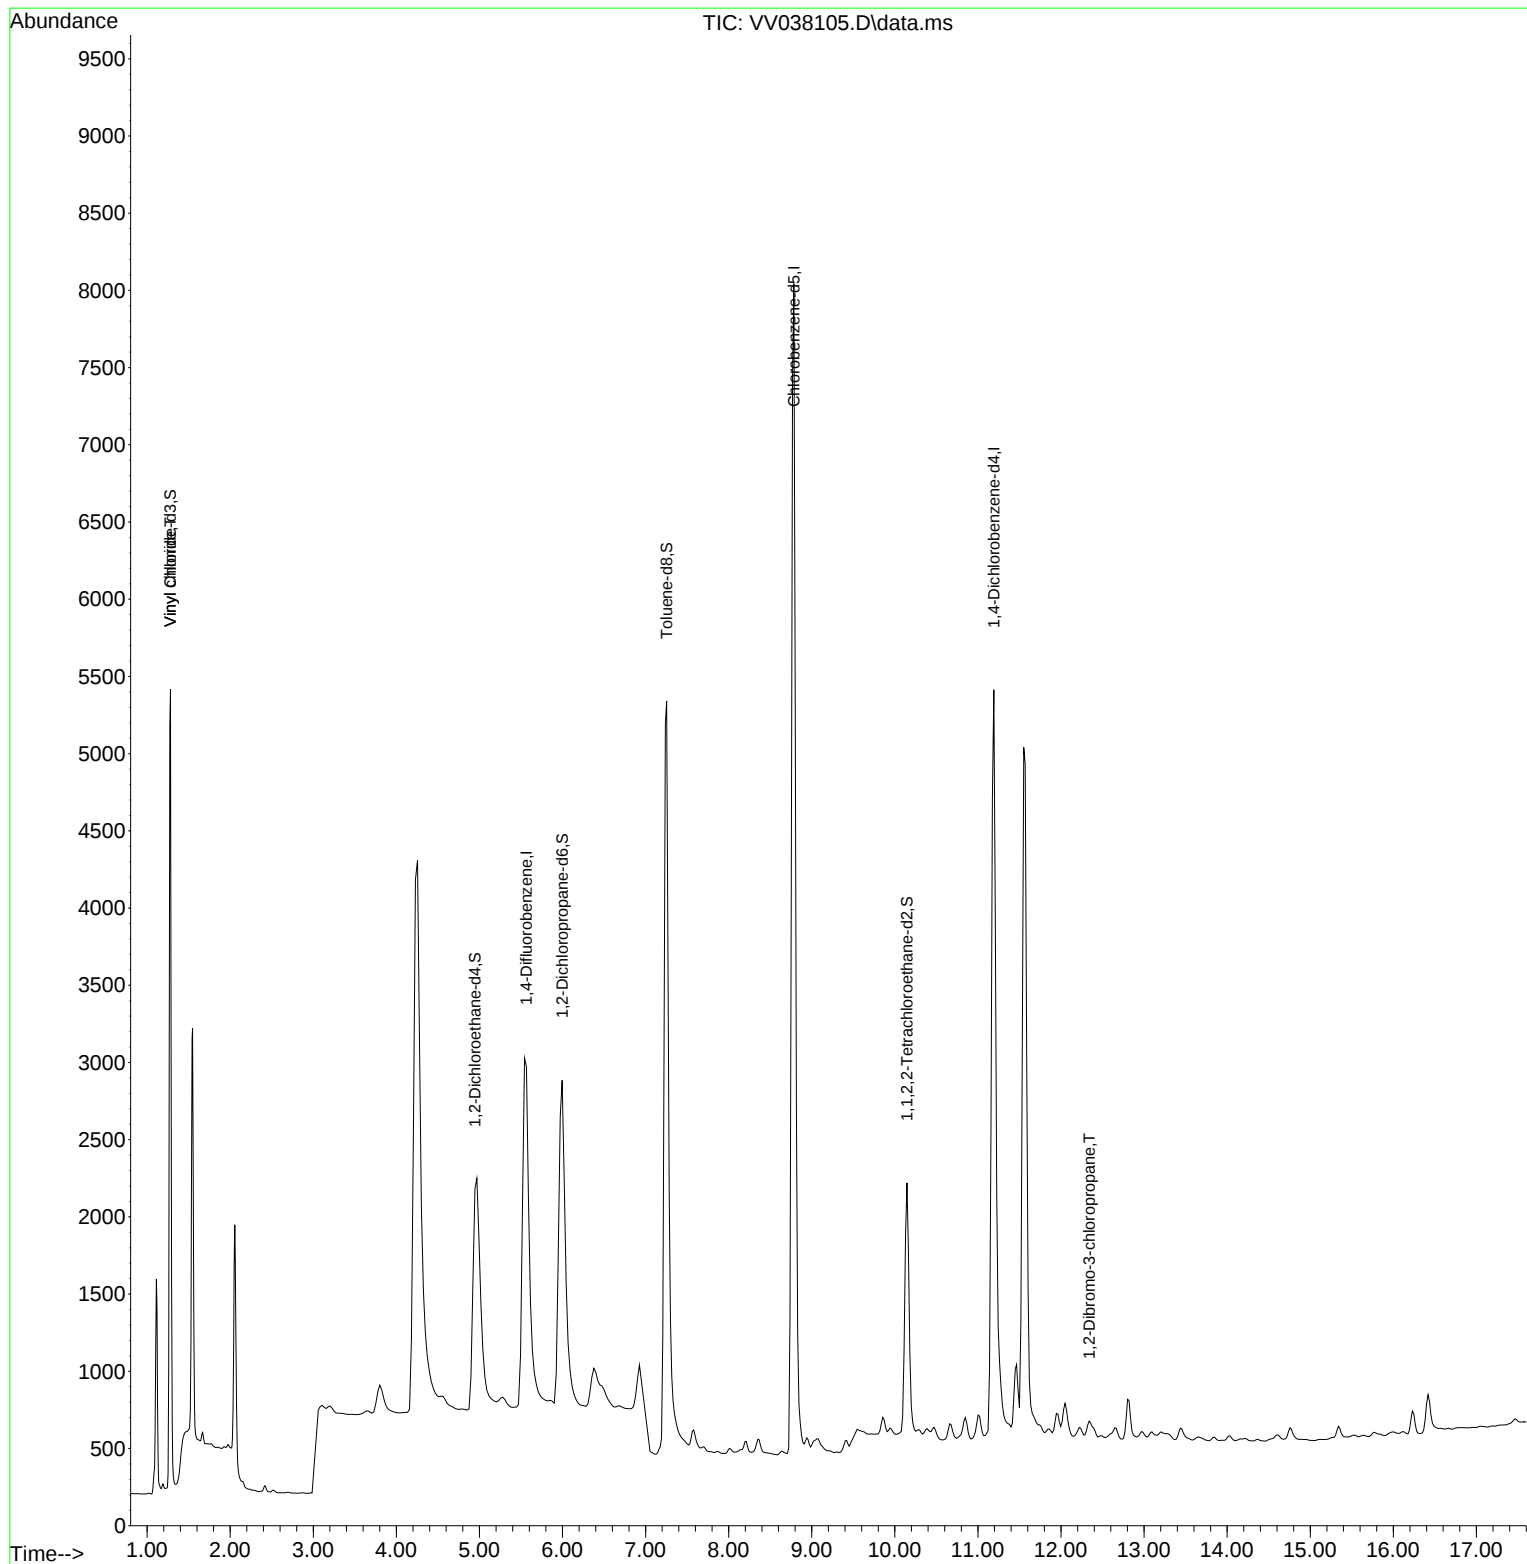

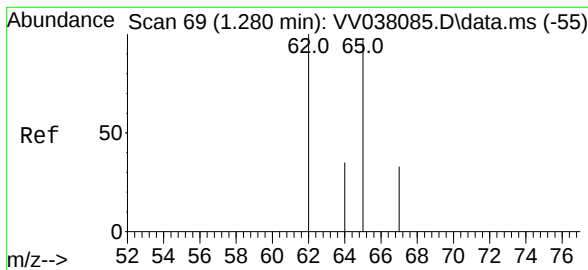

#3

Vinyl chloride

Concen: 0.021 ug/L

RT: 1.280 min Scan# 69

Delta R.T. 0.000 min

Lab File: VV038105.D

Acq: 14 Nov 2024 23:20

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 62 Resp: 214

Ion Ratio Lower Upper

62 100

64 82.8 25.3 47.1#

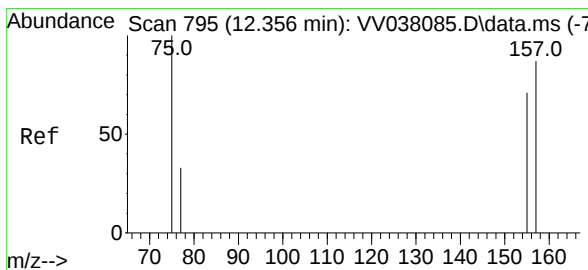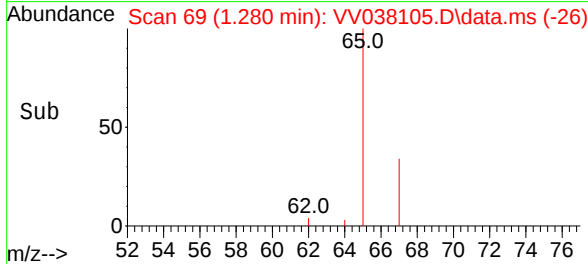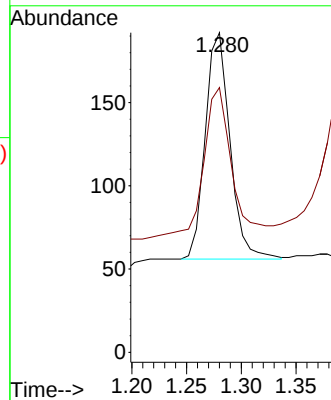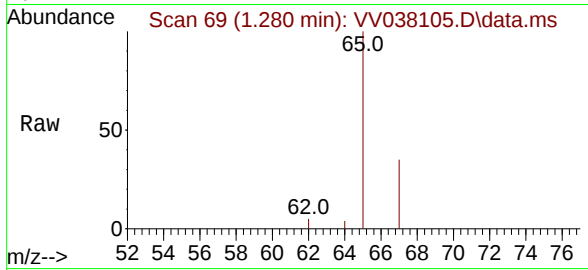

#13

1,2-Dibromo-3-chloropropane

Concen: 0.022 ug/L

RT: 12.339 min Scan# 794

Delta R.T. -0.017 min

Lab File: VV038105.D

Acq: 14 Nov 2024 23:20

Tgt Ion: 75 Resp: 20

Ion Ratio Lower Upper

75 100

157 77.4 69.4 104.0

155 77.4 61.3 91.9

