

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
 Data File : VV038111.D
 Acq On : 15 Nov 2024 02:32
 Operator : SY/MD
 Sample : P4761-09
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 15 04:17:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 00:15:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	8477	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.785	117	8557	0.500	ug/L	-0.02
11) 1,4-Dichlorobenzene-d4	11.191	152	4496	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.273	65	5347	0.609	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	122.000%
4) 1,2-Dichloroethane-d4	4.970	65	3248	0.611	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	122.000%
7) 1,2-Dichloropropane-d6	5.996	67	3956	0.571	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	114.000%
8) Toluene-d8	7.254	98	9565	0.539	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	108.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	3217	0.581	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	116.000%
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.322	75	28	0.036	ug/L	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
Data File : VV038111.D
Acq On : 15 Nov 2024 02:32
Operator : SY/MD
Sample : P4761-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Nov 15 04:17:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

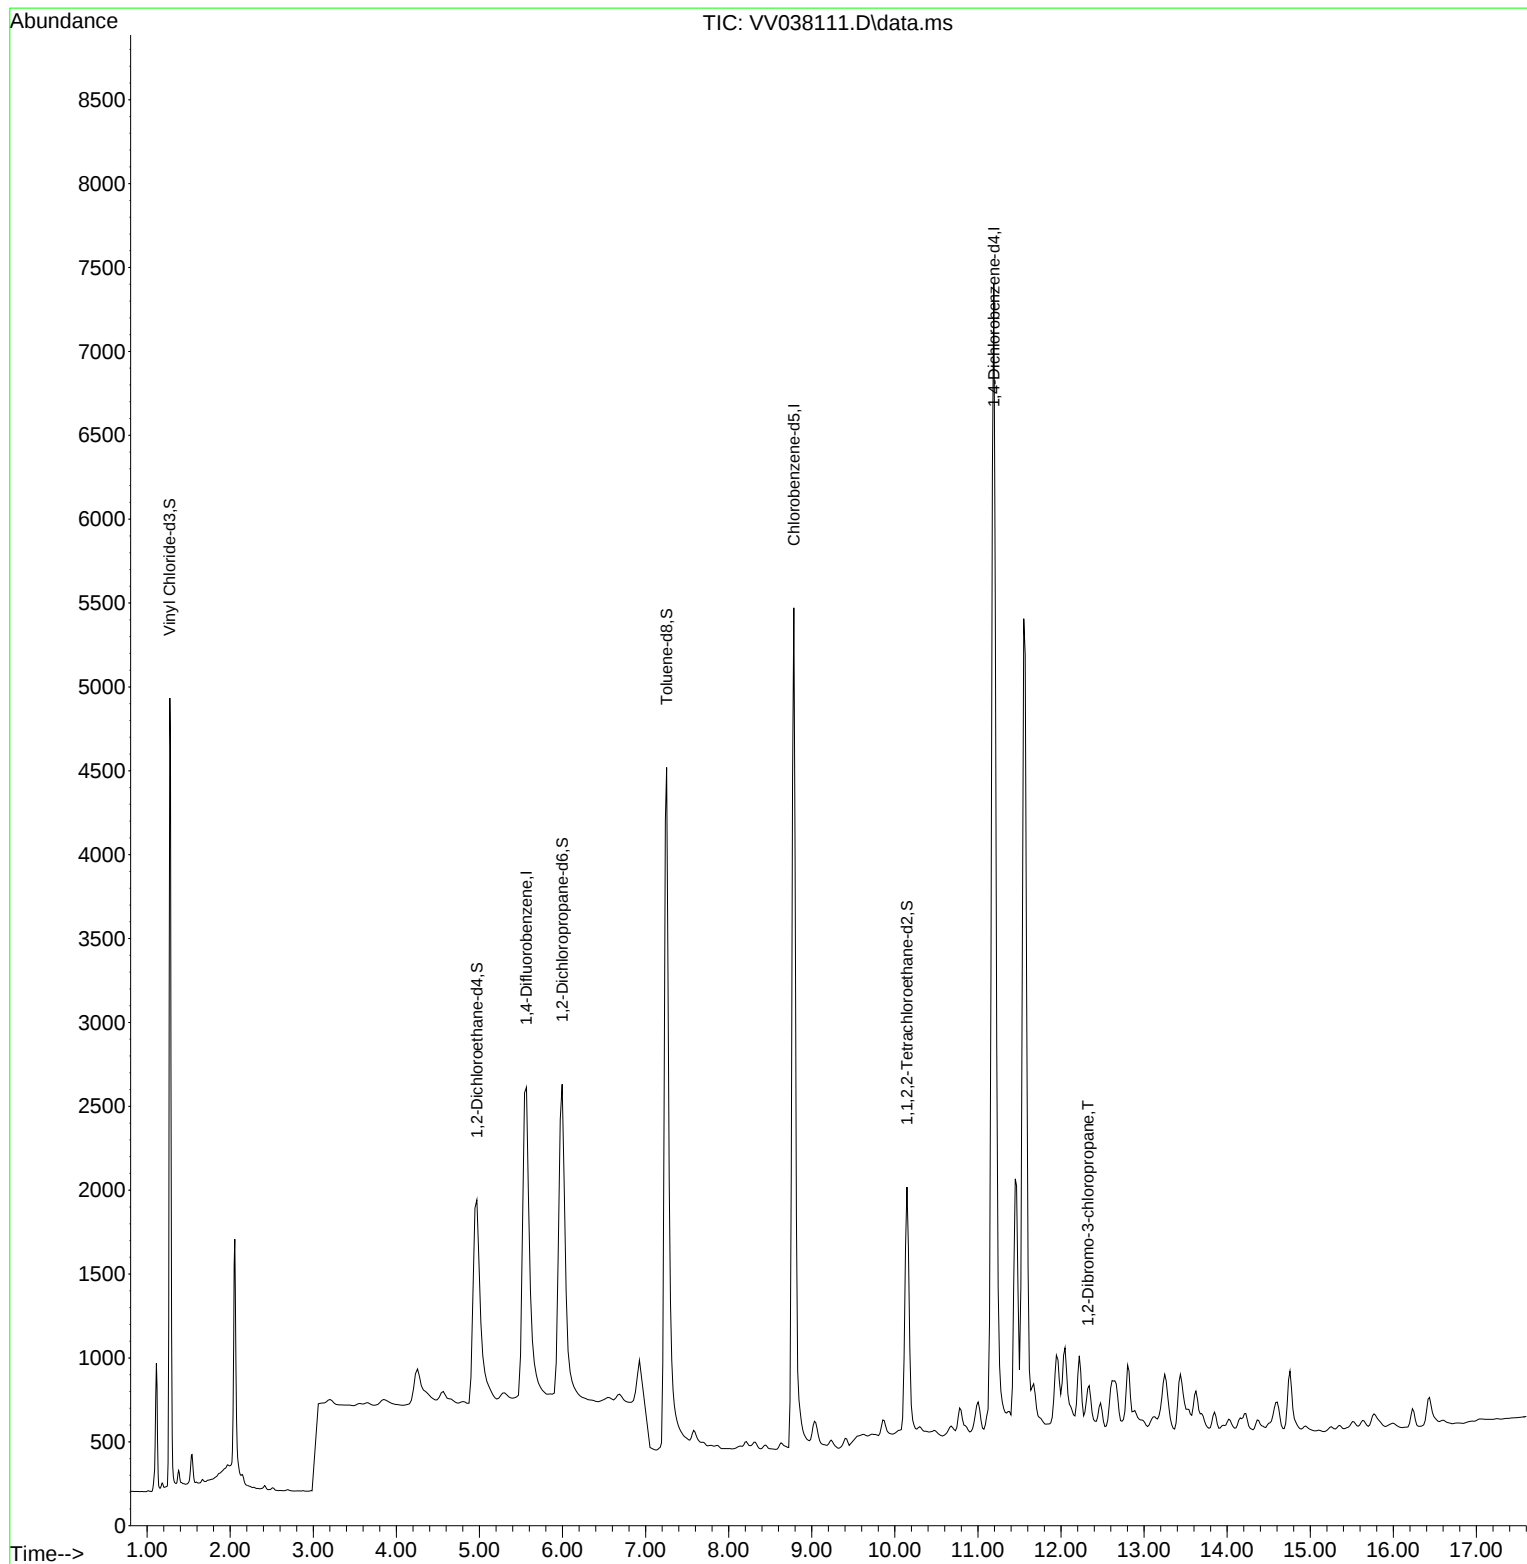

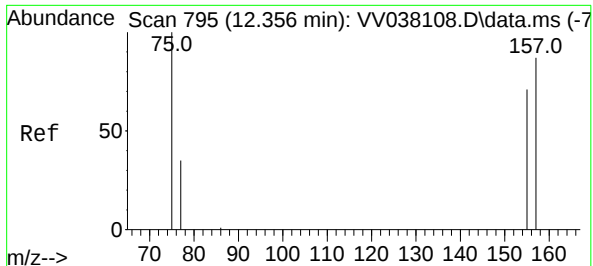

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.036 ug/L
 RT: 12.322 min Scan# 795
 Delta R.T. -0.034 min
 Lab File: VV038111.D
 Acq: 15 Nov 2024 02:32

Instrument :
 MSVOA_V
 ClientSampleId :

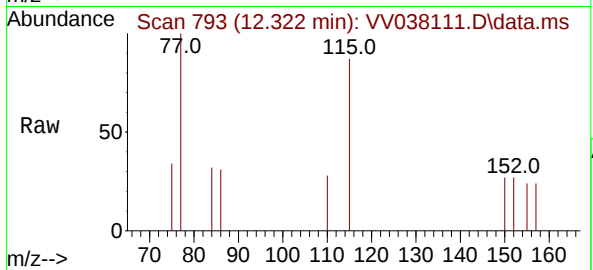

Tgt Ion: 75	Resp:	28
Ion	Ratio	Lower Upper
75	100	
157	71.6	69.4 104.0
155	71.6	61.3 91.9

