

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
 Data File : VV038112.D
 Acq On : 15 Nov 2024 02:56
 Operator : SY/MD
 Sample : P4761-14
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 15 04:17:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 00:15:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	8742	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	8769	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	4269	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	11916	1.315	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	= 264.000%#	
4) 1,2-Dichloroethane-d4	4.970	65	3363	0.613	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	= 122.000%	
7) 1,2-Dichloropropane-d6	5.996	67	3927	0.553	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	= 110.000%	
8) Toluene-d8	7.254	98	10062	0.553	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	= 110.000%	
10) 1,1,2,2-Tetrachloroeth...	10.146	84	3352	0.590	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	= 118.000%	
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.168	75	29	0.039	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
Data File : VV038112.D
Acq On : 15 Nov 2024 02:56
Operator : SY/MD
Sample : P4761-14
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Nov 15 04:17:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

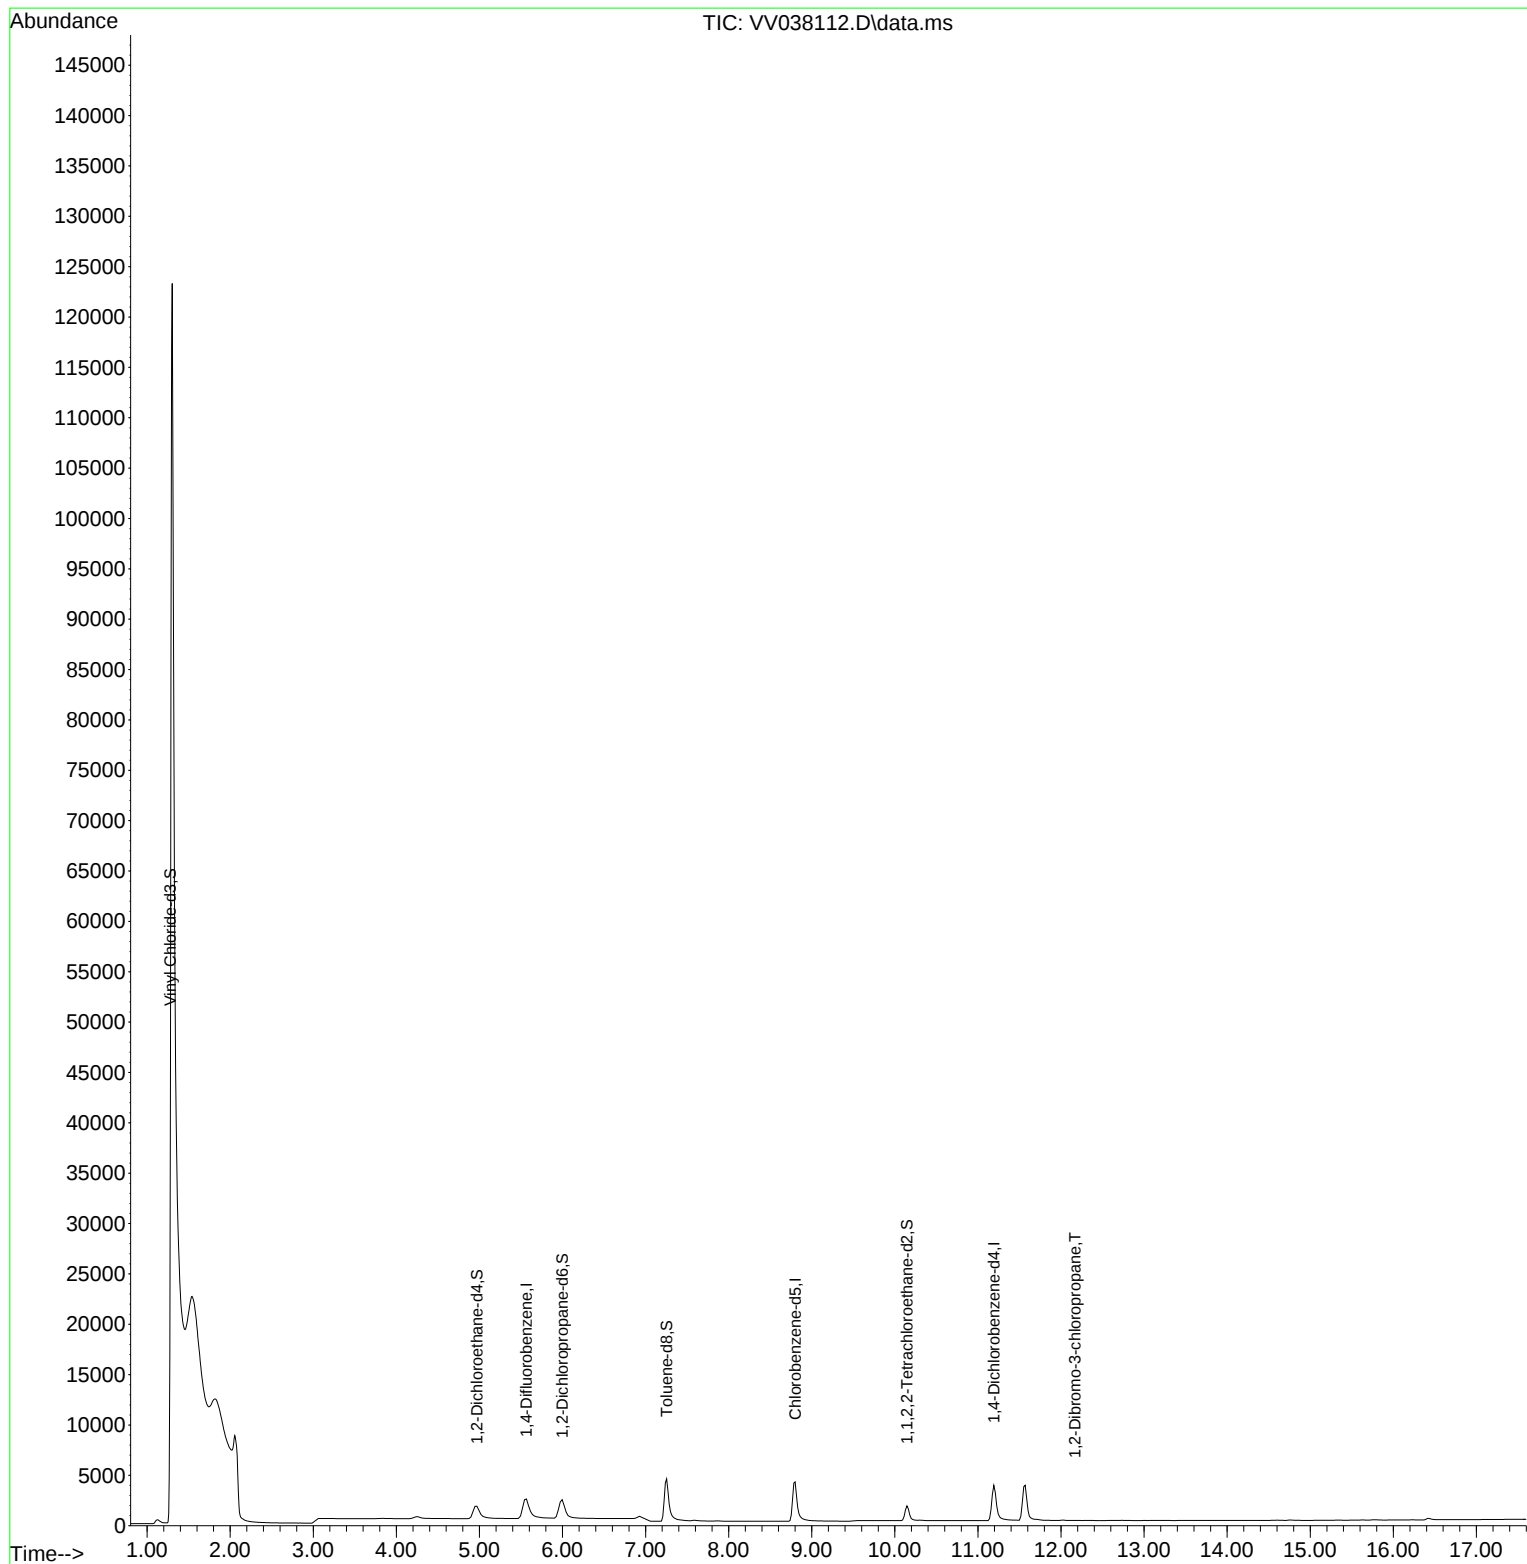

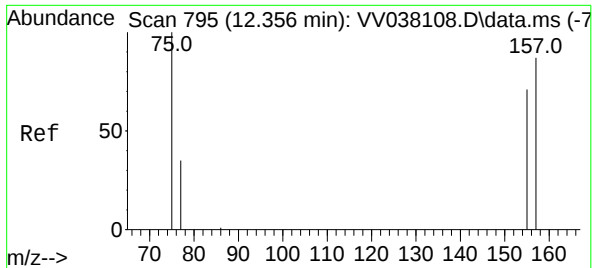

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.039 ug/L
 RT: 12.168 min Scan# 71
 Delta R.T. -0.188 min
 Lab File: VV038112.D
 Acq: 15 Nov 2024 02:56

Instrument :
 MSVOA_V
 ClientSampleId :

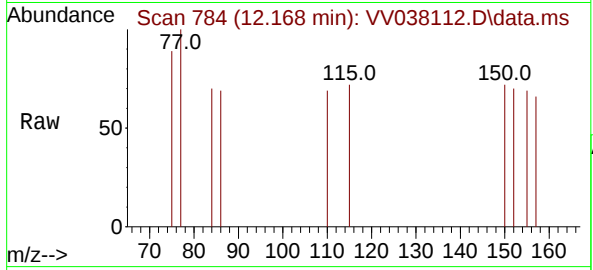

Tgt Ion: 75 Resp: 29

Ion	Ratio	Lower	Upper
75	100		
157	74.6	69.4	104.0
155	77.8	61.3	91.9

