

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
 Data File : VV038113.D
 Acq On : 15 Nov 2024 03:20
 Operator : SY/MD
 Sample : P4803-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 15 04:17:24 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 00:15:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	8759	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	8783	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	4324	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	10624	1.170	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	= 234.000%#	
4) 1,2-Dichloroethane-d4	4.969	65	3286	0.598	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	= 120.000%	
7) 1,2-Dichloropropane-d6	5.995	67	3838	0.539	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	= 108.000%	
8) Toluene-d8	7.253	98	9838	0.540	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	= 108.000%	
10) 1,1,2,2-Tetrachloroeth...	10.146	84	3308	0.582	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	= 116.000%	
Target Compounds						
3) Vinyl chloride	1.280	62	196	0.022	ug/L #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
Data File : VV038113.D
Acq On : 15 Nov 2024 03:20
Operator : SY/MD
Sample : P4803-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Nov 15 04:17:24 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

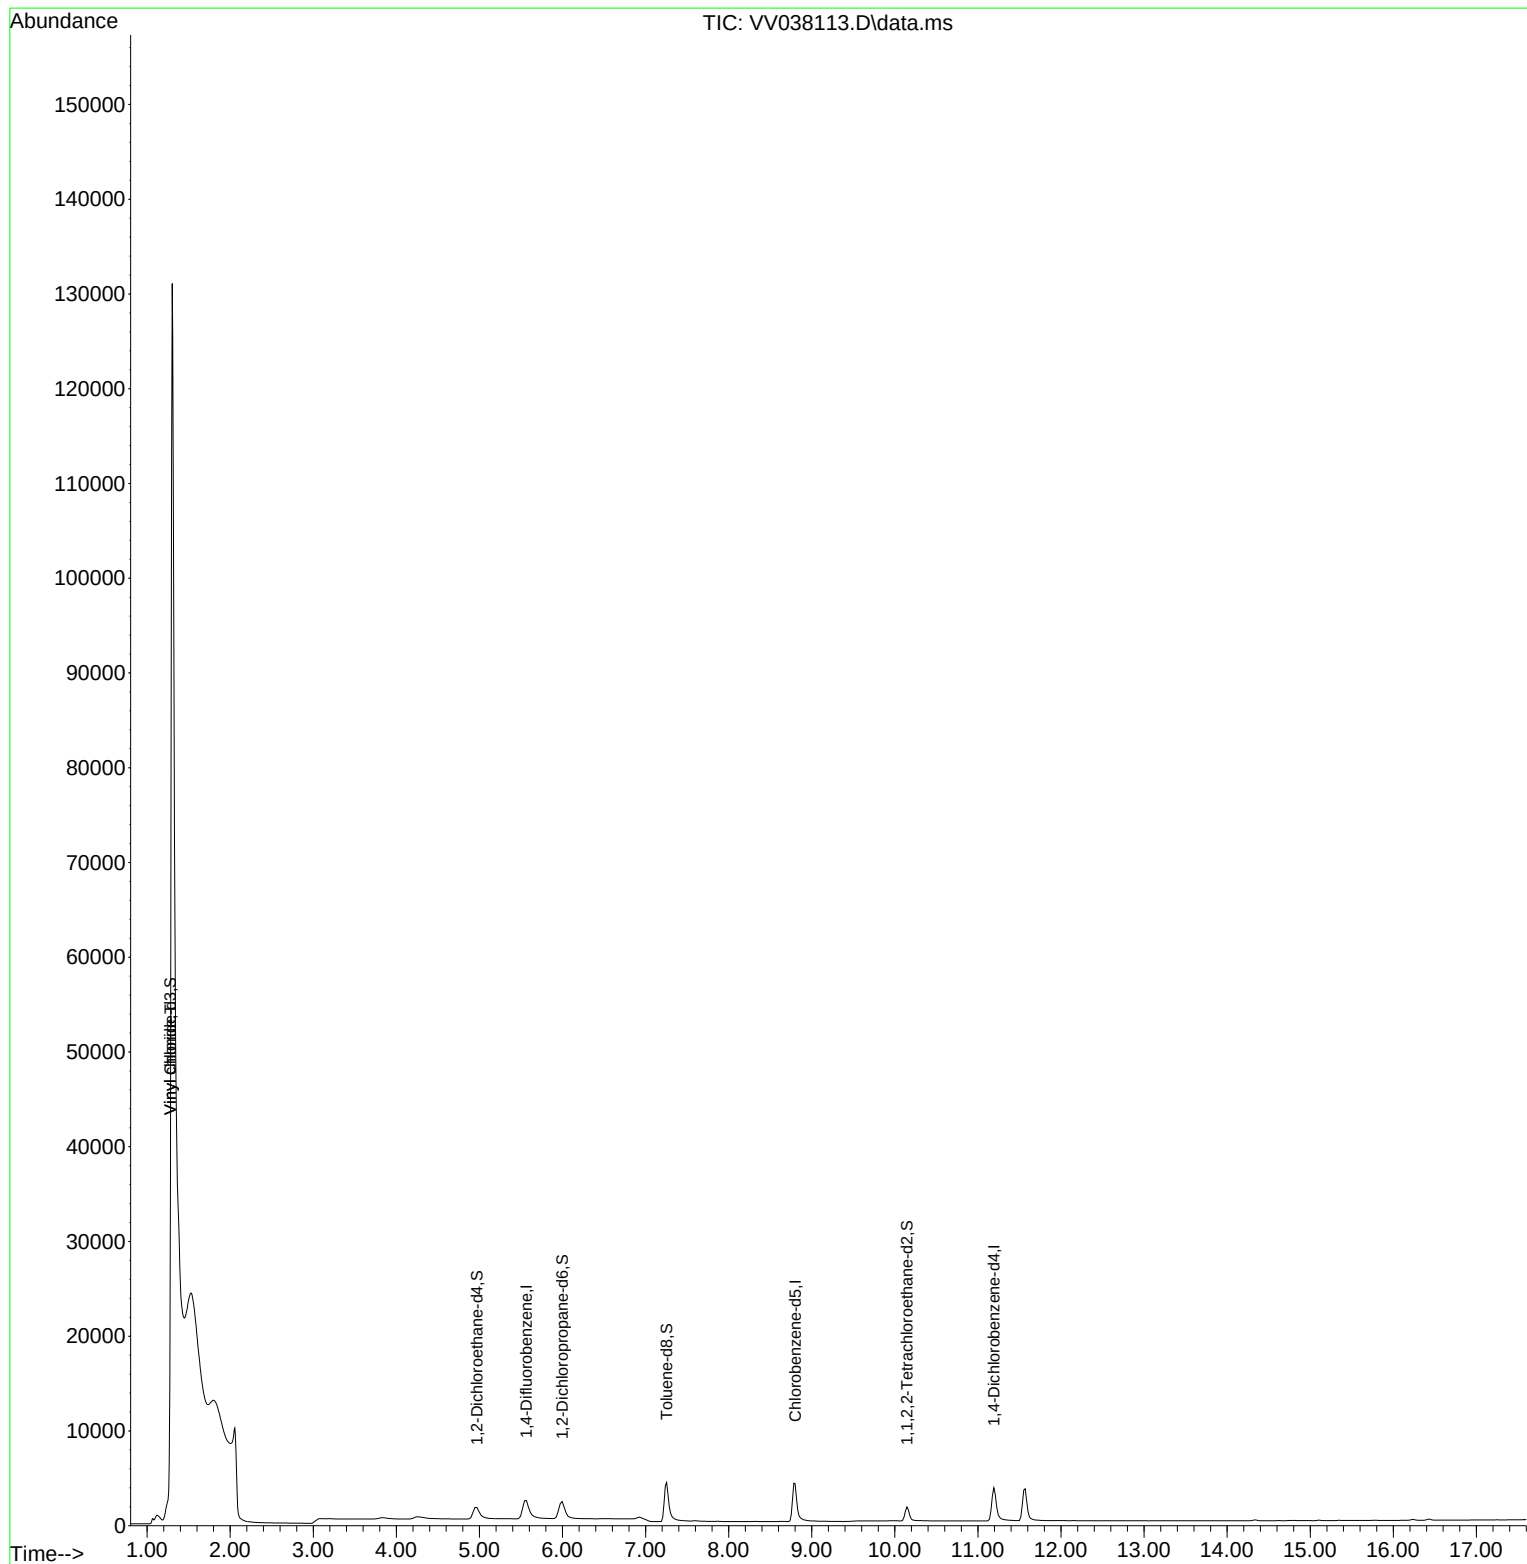

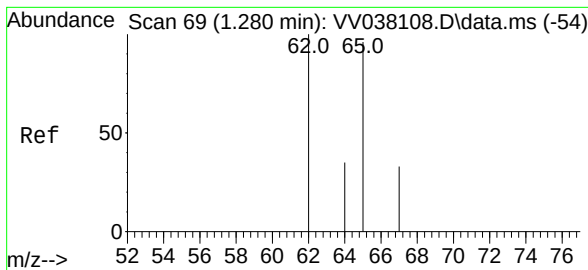

#3
 Vinyl chloride
 Concen: 0.022 ug/L
 RT: 1.280 min Scan# 69
 Delta R.T. 0.000 min
 Lab File: VV038113.D
 Acq: 15 Nov 2024 03:20

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 62 Resp: 196
 Ion Ratio Lower Upper
 62 100
 64 24097.7 25.3 47.1#

