

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
 Data File : VV038114.D
 Acq On : 15 Nov 2024 03:44
 Operator : SY/MD
 Sample : P4803-14
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 15 04:17:35 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 00:15:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	8766	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	8659	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	4347	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.273	65	5881	0.647	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	130.000%
4) 1,2-Dichloroethane-d4	4.969	65	3164	0.575	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	116.000%
7) 1,2-Dichloropropane-d6	5.995	67	3800	0.542	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	108.000%
8) Toluene-d8	7.253	98	9606	0.535	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	106.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	3101	0.553	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	110.000%
Target Compounds						
3) Vinyl chloride	1.379	62	1061	0.117	ug/L	Qvalue # 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
Data File : VV038114.D
Acq On : 15 Nov 2024 03:44
Operator : SY/MD
Sample : P4803-14
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Nov 15 04:17:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

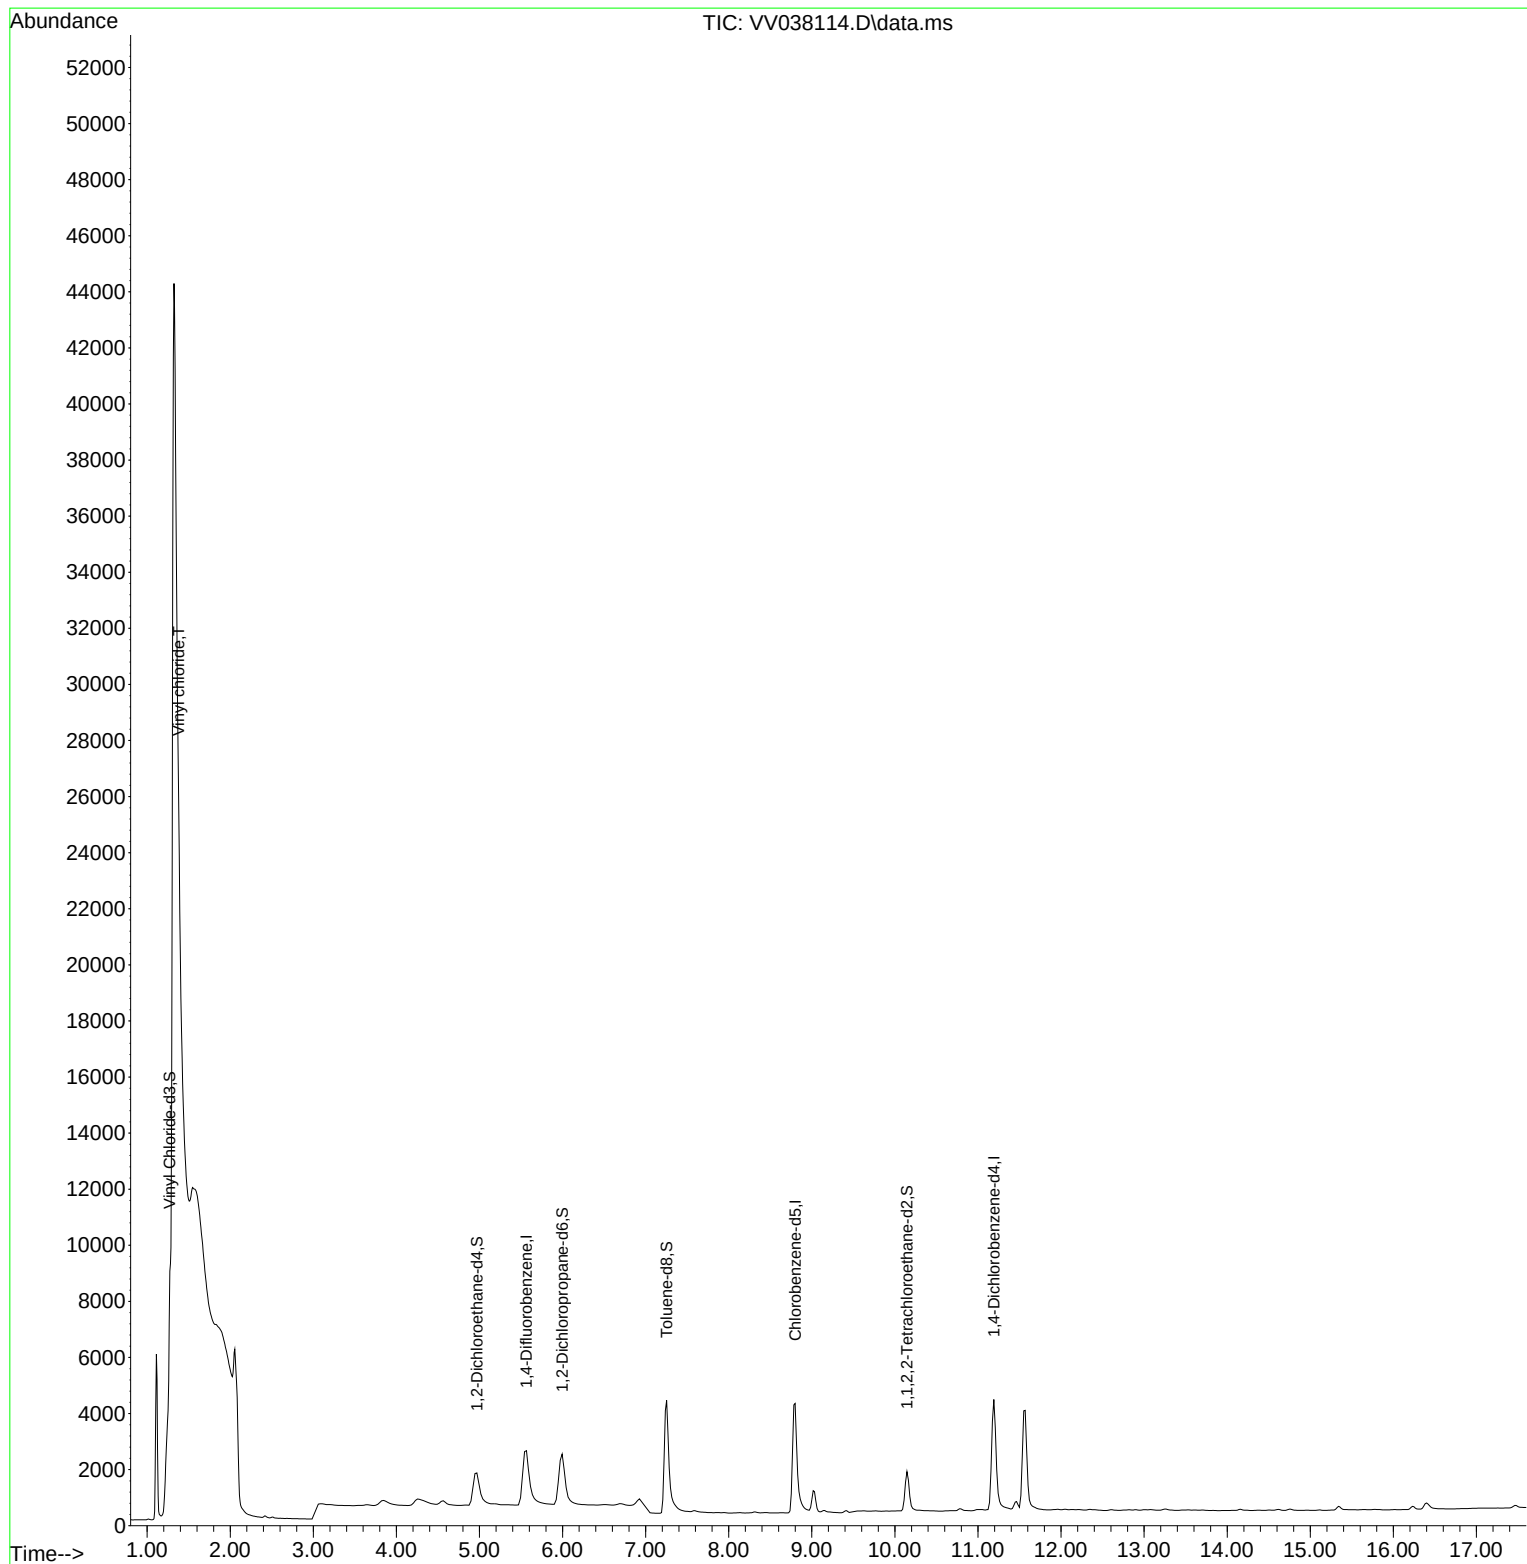

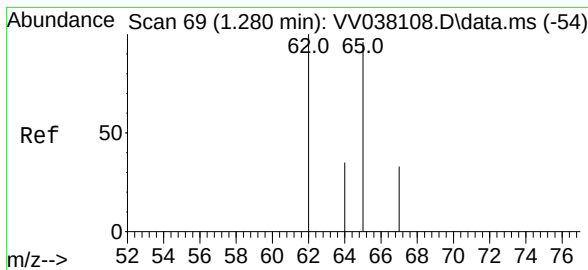

#3

Vinyl chloride

Concen: 0.117 ug/L

RT: 1.379 min Scan# 81

Delta R.T. 0.099 min


Lab File: VV038114.D

Acq: 15 Nov 2024 03:44

Instrument :

MSVOA_V

ClientSampleId :

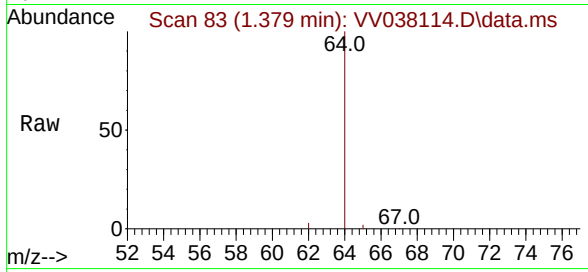

Tgt Ion: 62 Resp: 1061

Ion	Ratio	Lower	Upper
62	100		
64	3397.0	25.3	47.1#

