




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
Data File : VV038099.D
Acq On : 14 Nov 2024 20:56
Operator : SY/MD
Sample : P4761-02 2X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A0AL2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 11/18/2024
Supervised By :Mahesh Dadoda 11/18/2024

Quant Time: Nov 15 00:34:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

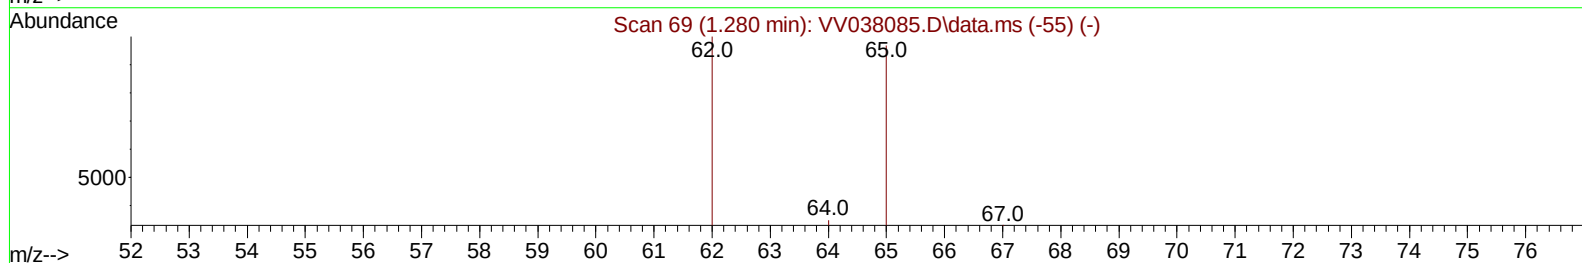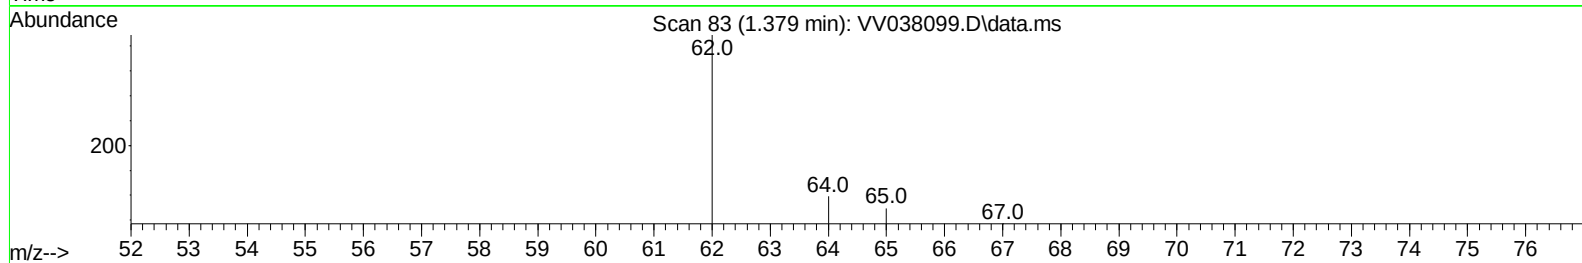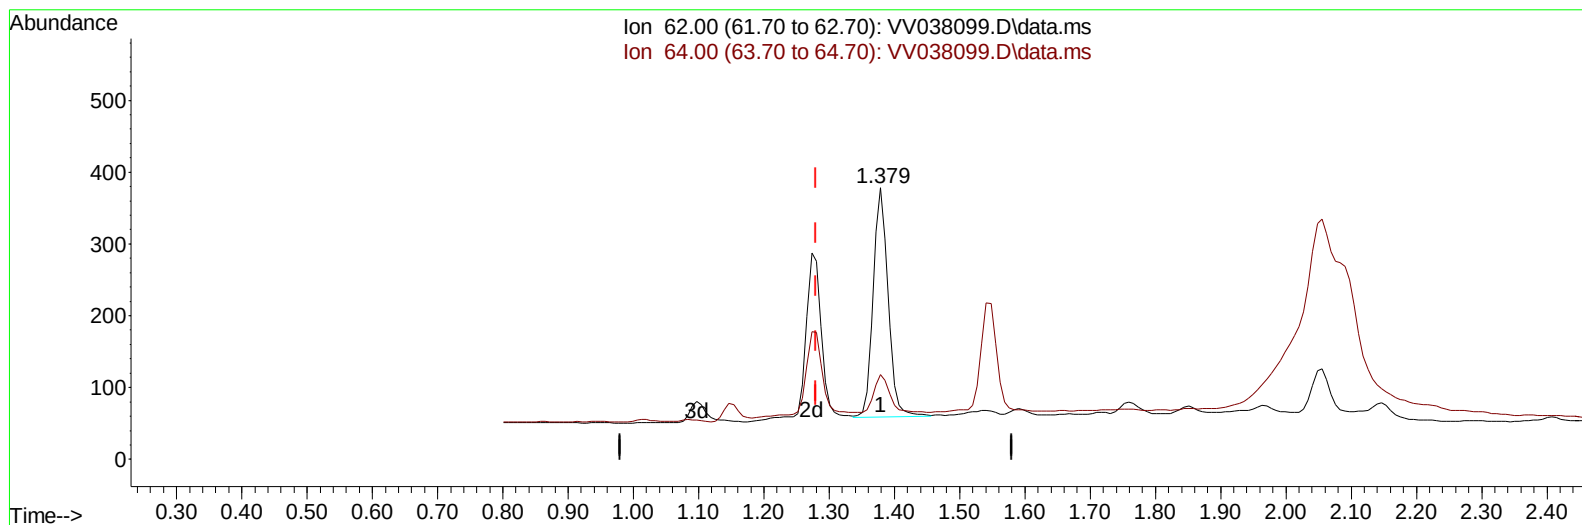

TIC: VV038099.D\data.ms

(3) Vinyl chloride (T)

1.379min (+ 0.099) 0.05 ug/L

response 512

Ion	Exp%	Act%
62.00	100.00	100.00
64.00	36.20	31.22
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
 Data File : VV038099.D
 Acq On : 14 Nov 2024 20:56
 Operator : SY/MD
 Sample : P4761-02 2X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A0AL2

Manual IntegrationsAPPROVED

Quant Time: Nov 15 00:34:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 00:15:53 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 11/18/2024
 Supervised By :Mahesh Dadoda 11/18/2024

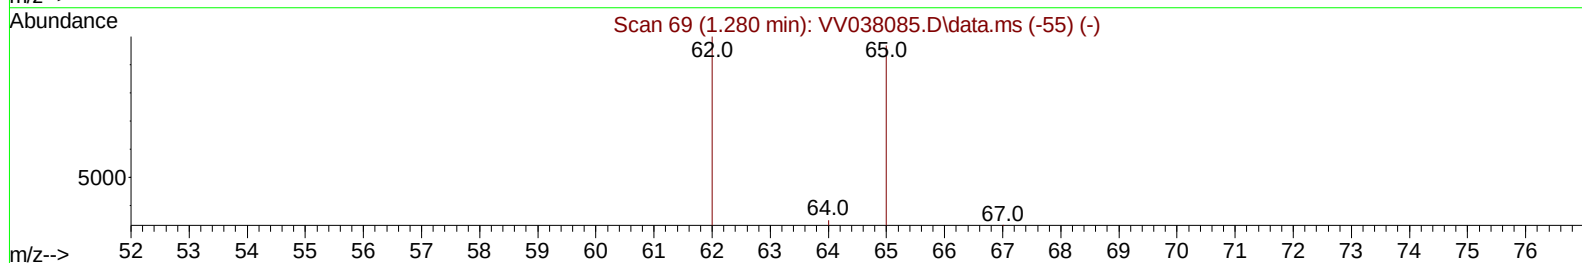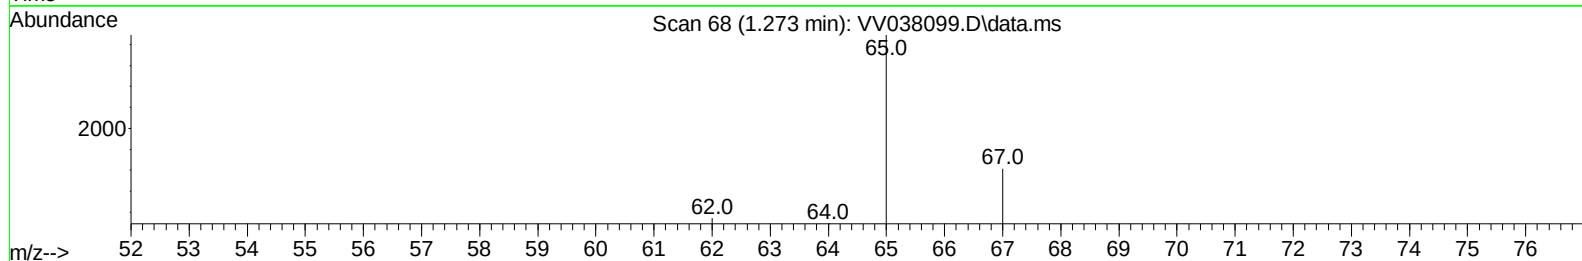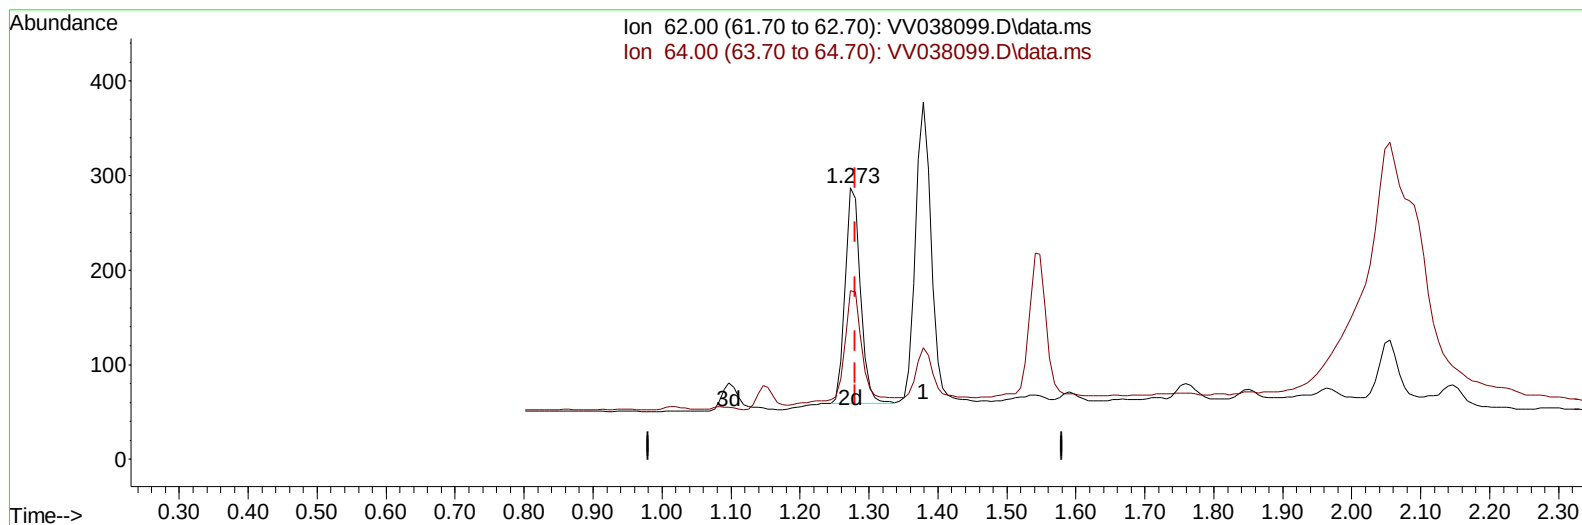

TIC: VV038099.D\data.ms

(3) Vinyl chloride (T)

1.273min (-0.007) 0.04 ug/L m

response 355

Ion	Exp%	Act%
62.00	100.00	100.00
64.00	36.20	62.02#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
 Data File : VV038099.D
 Acq On : 14 Nov 2024 20:56
 Operator : SY/MD
 Sample : P4761-02 2X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A0AL2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 11/18/2024
 Supervised By :Mahesh Dadoda 11/18/2024

Quant Time: Nov 15 00:34:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 00:15:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	9802	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.785	117	9826	0.500	ug/L	#-0.02
11) 1,4-Dichlorobenzene-d4	11.191	152	5118	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.273	65	5663	0.557	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery = 112.000%			
4) 1,2-Dichloroethane-d4	4.969	65	3482	0.566	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 114.000%			
7) 1,2-Dichloropropane-d6	5.995	67	4674	0.587	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery = 118.000%			
8) Toluene-d8	7.253	98	11002	0.540	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 108.000%			
10) 1,1,2,2-Tetrachloroeth...	10.146	84	3239	0.509	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery = 102.000%			
Target Compounds						
3) Vinyl chloride	1.273	62	355m	0.035	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
Data File : VV038099.D
Acq On : 14 Nov 2024 20:56
Operator : SY/MD
Sample : P4761-02 2X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A0AL2

Manual IntegrationsAPPROVED

Quant Time: Nov 15 00:34:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 11/18/2024
Supervised By :Mahesh Dadoda 11/18/2024

