




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
Data File : VV038101.D
Acq On : 14 Nov 2024 21:44
Operator : SY/MD
Sample : P4761-05 2X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A0AL7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 11/18/2024
Supervised By :Mahesh Dadoda 11/18/2024

Quant Time: Nov 15 00:35:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

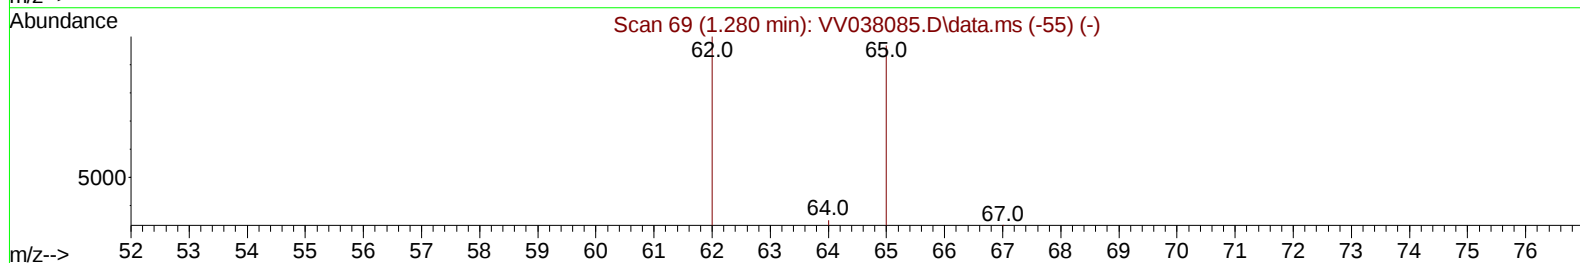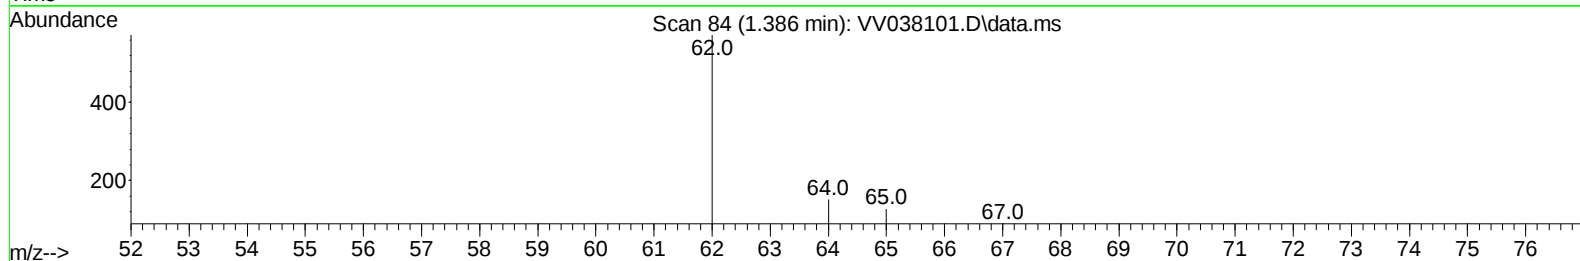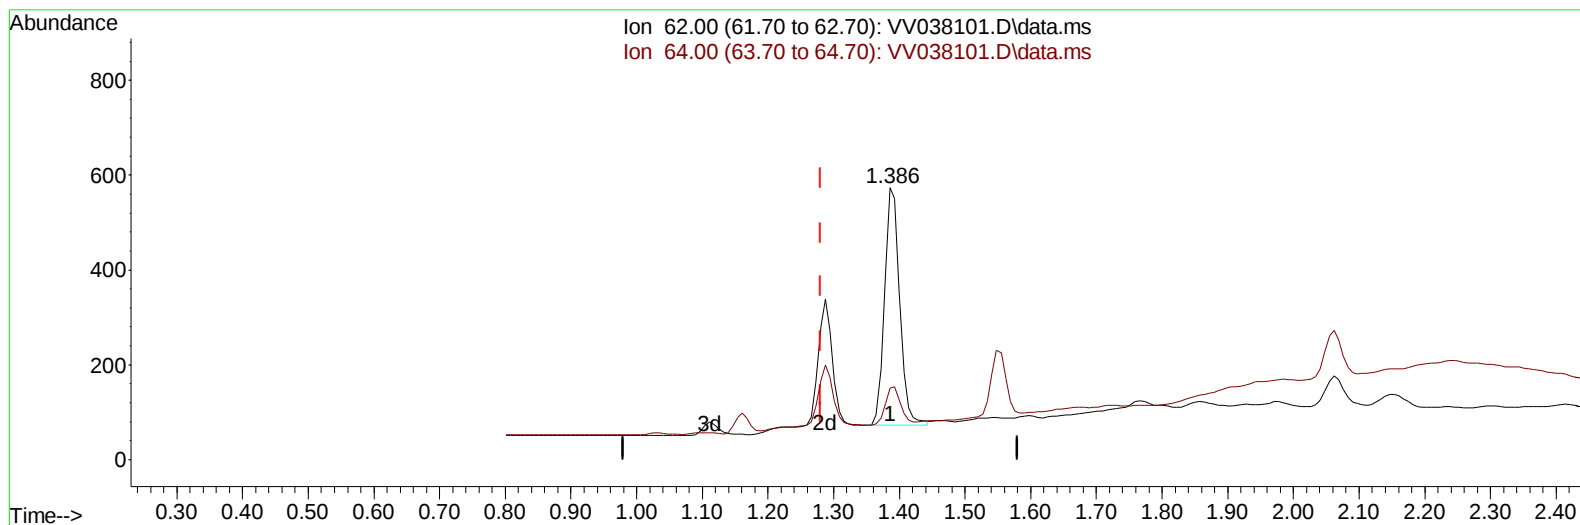

TIC: VV038101.D\data.ms

(3) Vinyl chloride (T)

1.386min (+ 0.106) 0.08 ug/L

response 815

Ion	Exp%	Act%
62.00	100.00	100.00
64.00	36.20	26.35
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
Data File : VV038101.D
Acq On : 14 Nov 2024 21:44
Operator : SY/MD
Sample : P4761-05 2X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A0AL7

Manual IntegrationsAPPROVED

Quant Time: Nov 15 00:35:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 11/18/2024
Supervised By :Mahesh Dadoda 11/18/2024

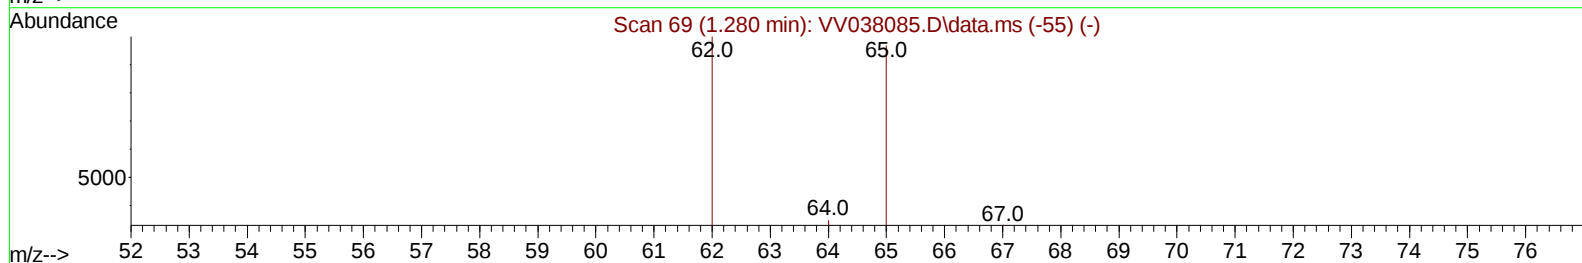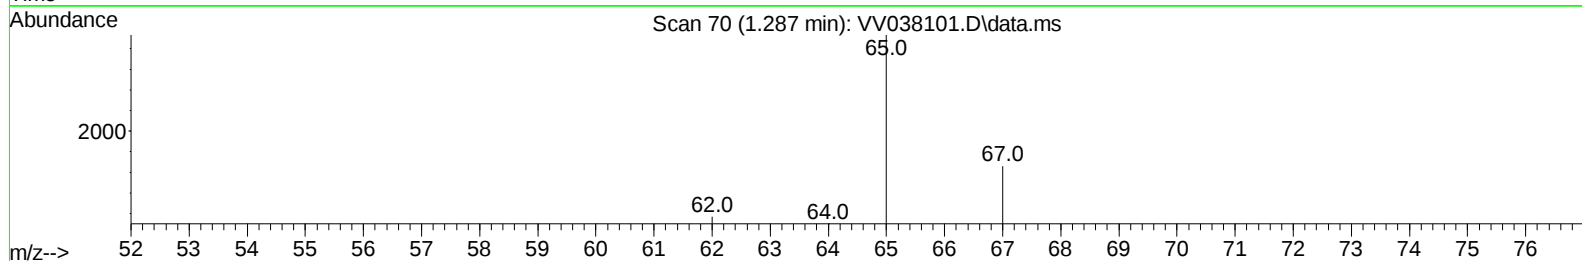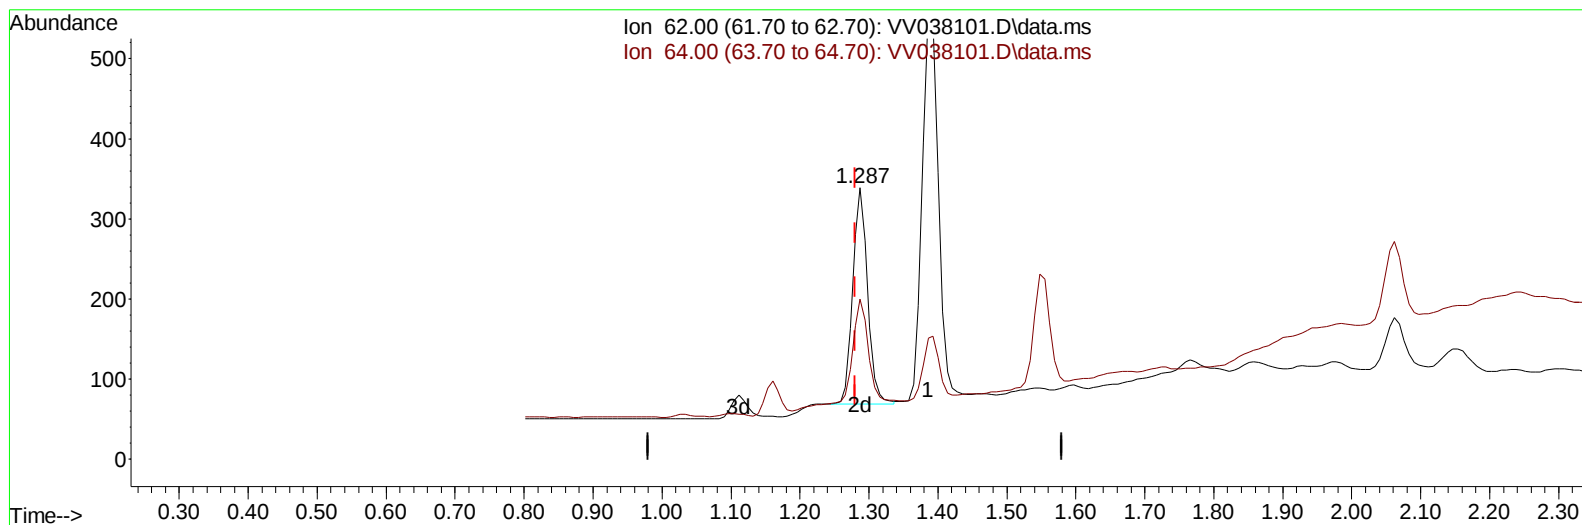

TIC: VV038101.D\data.ms

(3) Vinyl chloride (T)

1.287min (+ 0.007) 0.04 ug/L m

response 404

Ion	Exp%	Act%
62.00	100.00	100.00
64.00	36.20	59.00#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
 Data File : VV038101.D
 Acq On : 14 Nov 2024 21:44
 Operator : SY/MD
 Sample : P4761-05 2X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A0AL7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 11/18/2024
 Supervised By :Mahesh Dadoda 11/18/2024

Quant Time: Nov 15 00:35:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 00:15:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	10083	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.785	117	10317	0.500	ug/L	#-0.02
11) 1,4-Dichlorobenzene-d4	11.191	152	5044	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.287	65	5623	0.538	ug/L	0.01
Spiked Amount 0.500	Range 40 - 130		Recovery = 108.000%			
4) 1,2-Dichloroethane-d4	4.969	65	3522	0.557	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 112.000%			
7) 1,2-Dichloropropane-d6	6.019	67	4885	0.585	ug/L	0.02
Spiked Amount 0.500	Range 60 - 140		Recovery = 116.000%			
8) Toluene-d8	7.253	98	11204	0.524	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 104.000%			
10) 1,1,2,2-Tetrachloroeth...	10.146	84	3110	0.466	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery = 94.000%			
Target Compounds						
3) Vinyl chloride	1.287	62	404m	0.039	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
Data File : VV038101.D
Acq On : 14 Nov 2024 21:44
Operator : SY/MD
Sample : P4761-05 2X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A0AL7

Manual IntegrationsAPPROVED

Quant Time: Nov 15 00:35:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 11/18/2024
Supervised By :Mahesh Dadoda 11/18/2024

