




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
Data File : VV038123.D
Acq On : 15 Nov 2024 07:20
Operator : SY/MD
Sample : P4803-20 2X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A0AS9

Manual IntegrationsAPPROVED

Quant Time: Nov 15 07:38:32 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 11/18/2024
Supervised By :Mahesh Dadoda 11/18/2024

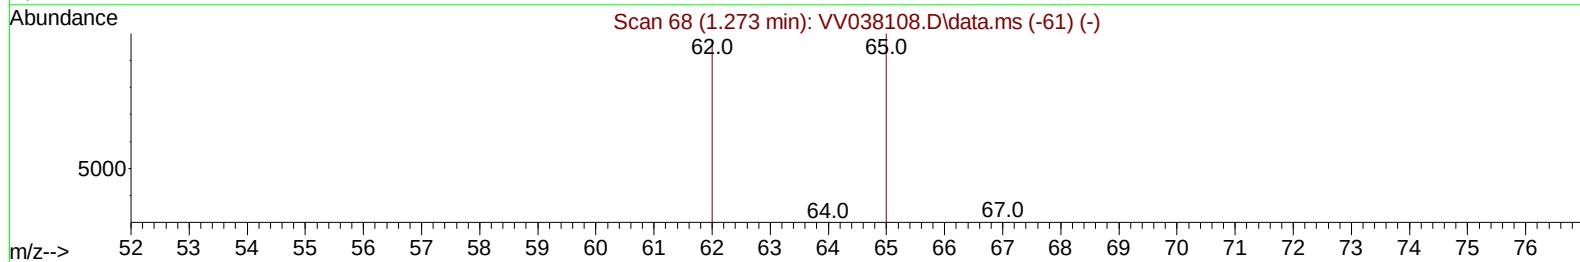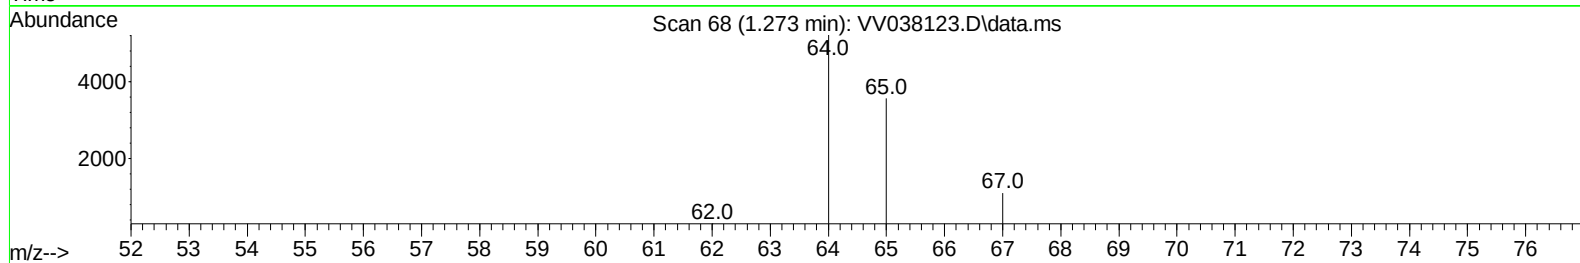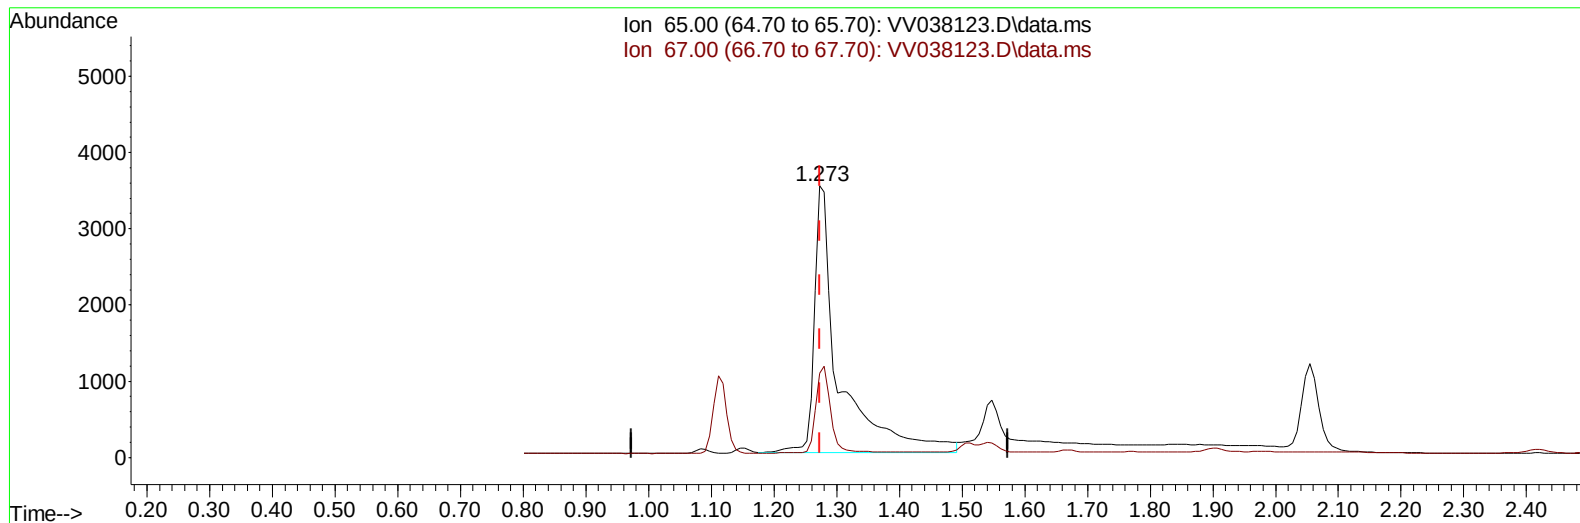

TIC: VV038123.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.273min (+ 0.000) 0.97 ug/L

response 9765

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	33.70	19.24#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
Data File : VV038123.D
Acq On : 15 Nov 2024 07:20
Operator : SY/MD
Sample : P4803-20 2X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A0AS9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 11/18/2024
Supervised By :Mahesh Dadoda 11/18/2024

Quant Time: Nov 15 07:38:32 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

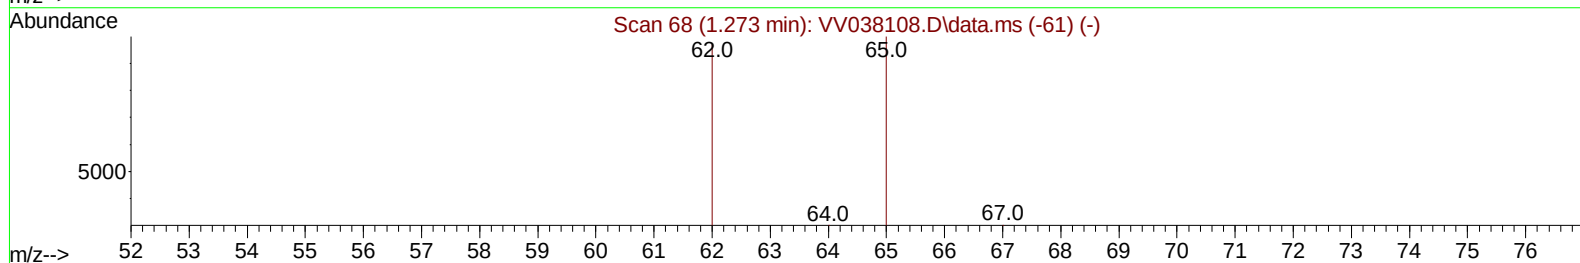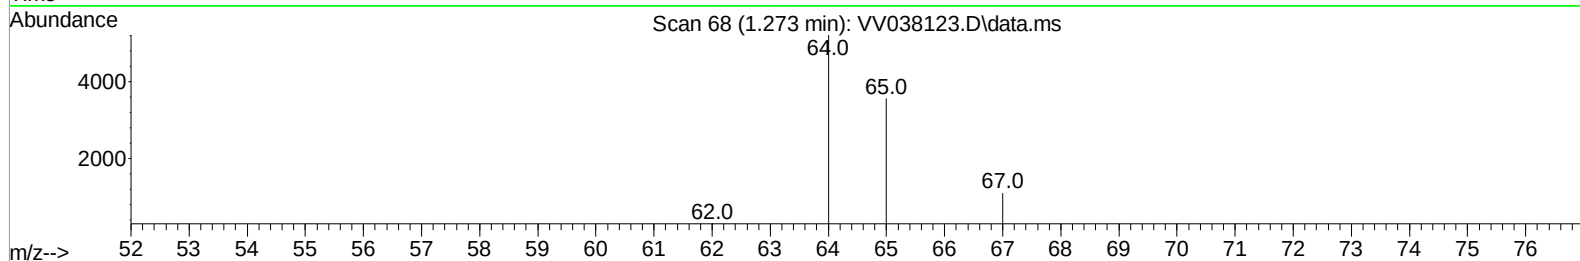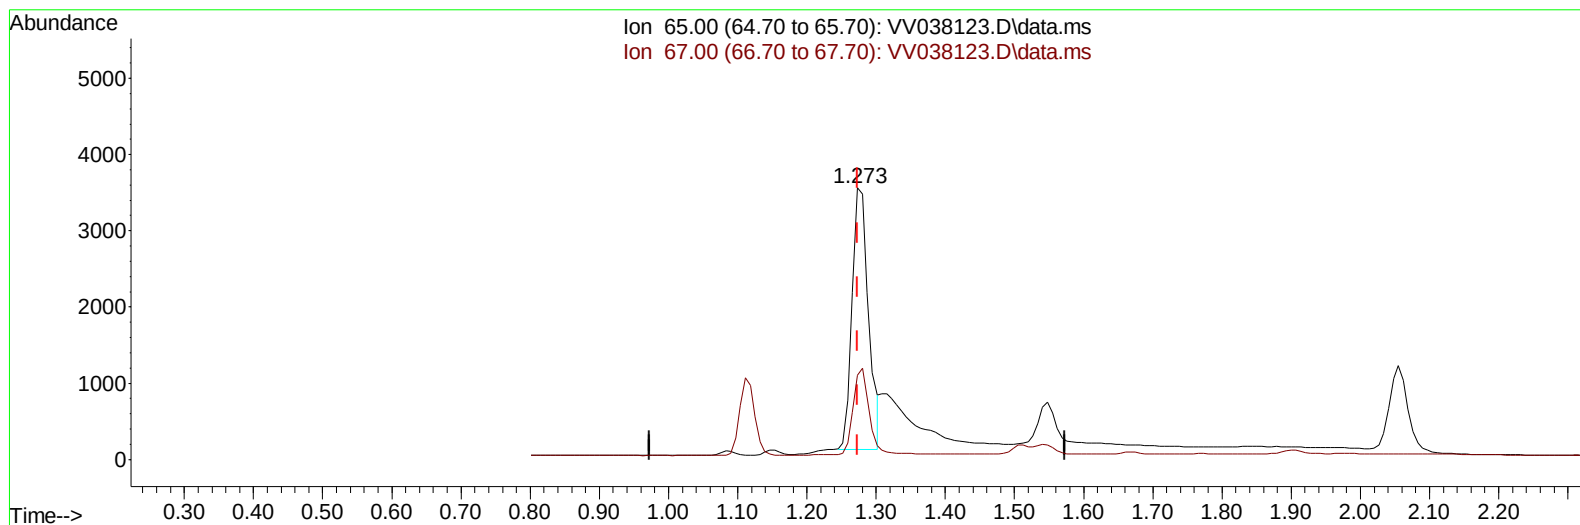

TIC: VV038123.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.273min (+ 0.000) 0.56 ug/L m

response 5634

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	33.70	33.35
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
 Data File : VV038123.D
 Acq On : 15 Nov 2024 07:20
 Operator : SY/MD
 Sample : P4803-20 2X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A0AS9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 11/18/2024
 Supervised By :Mahesh Dadoda 11/18/2024

Quant Time: Nov 15 07:38:32 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 00:15:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	9705	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.785	117	9398	0.500	ug/L	-0.02
11) 1,4-Dichlorobenzene-d4	11.191	152	5075	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.273	65	5634m	0.560	ug/L	0.00
Spiked Amount	0.500	Range 40 - 130	Recovery	= 112.000%		
4) 1,2-Dichloroethane-d4	4.945	65	3163	0.520	ug/L	-0.02
Spiked Amount	0.500	Range 70 - 130	Recovery	= 104.000%		
7) 1,2-Dichloropropane-d6	5.995	67	4140	0.544	ug/L	0.00
Spiked Amount	0.500	Range 60 - 140	Recovery	= 108.000%		
8) Toluene-d8	7.253	98	10265	0.527	ug/L	0.00
Spiked Amount	0.500	Range 70 - 130	Recovery	= 106.000%		
10) 1,1,2,2-Tetrachloroeth...	10.146	84	3887	0.639	ug/L	0.00
Spiked Amount	0.500	Range 65 - 120	Recovery	= 128.000%#		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
Data File : VV038123.D
Acq On : 15 Nov 2024 07:20
Operator : SY/MD
Sample : P4803-20 2X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A0AS9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 11/18/2024
Supervised By :Mahesh Dadoda 11/18/2024

Quant Time: Nov 15 07:38:32 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

