

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
 Data File : VV038101.D
 Acq On : 14 Nov 2024 21:44
 Operator : SY/MD
 Sample : P4761-05 2X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A0AL7

Quant Time: Nov 15 00:35:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 00:15:53 2024
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Semsettin Yesilyurt 11/18/2024
 Supervised By :Mahesh Dadoda 11/18/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	10083	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.785	117	10317	0.500	ug/L	#-0.02
11) 1,4-Dichlorobenzene-d4	11.191	152	5044	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.287	65	5623	0.538	ug/L	0.01
Spiked Amount 0.500	Range 40 - 130		Recovery = 108.000%			
4) 1,2-Dichloroethane-d4	4.969	65	3522	0.557	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 112.000%			
7) 1,2-Dichloropropane-d6	6.019	67	4885	0.585	ug/L	0.02
Spiked Amount 0.500	Range 60 - 140		Recovery = 116.000%			
8) Toluene-d8	7.253	98	11204	0.524	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 104.000%			
10) 1,1,2,2-Tetrachloroeth...	10.146	84	3110	0.466	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery = 94.000%			
Target Compounds						
3) Vinyl chloride	1.287	62	404m	0.039	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
Data File : VV038101.D
Acq On : 14 Nov 2024 21:44
Operator : SY/MD
Sample : P4761-05 2X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A0AL7


Quant Time: Nov 15 00:35:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 11/18/2024
Supervised By :Mahesh Dadoda 11/18/2024

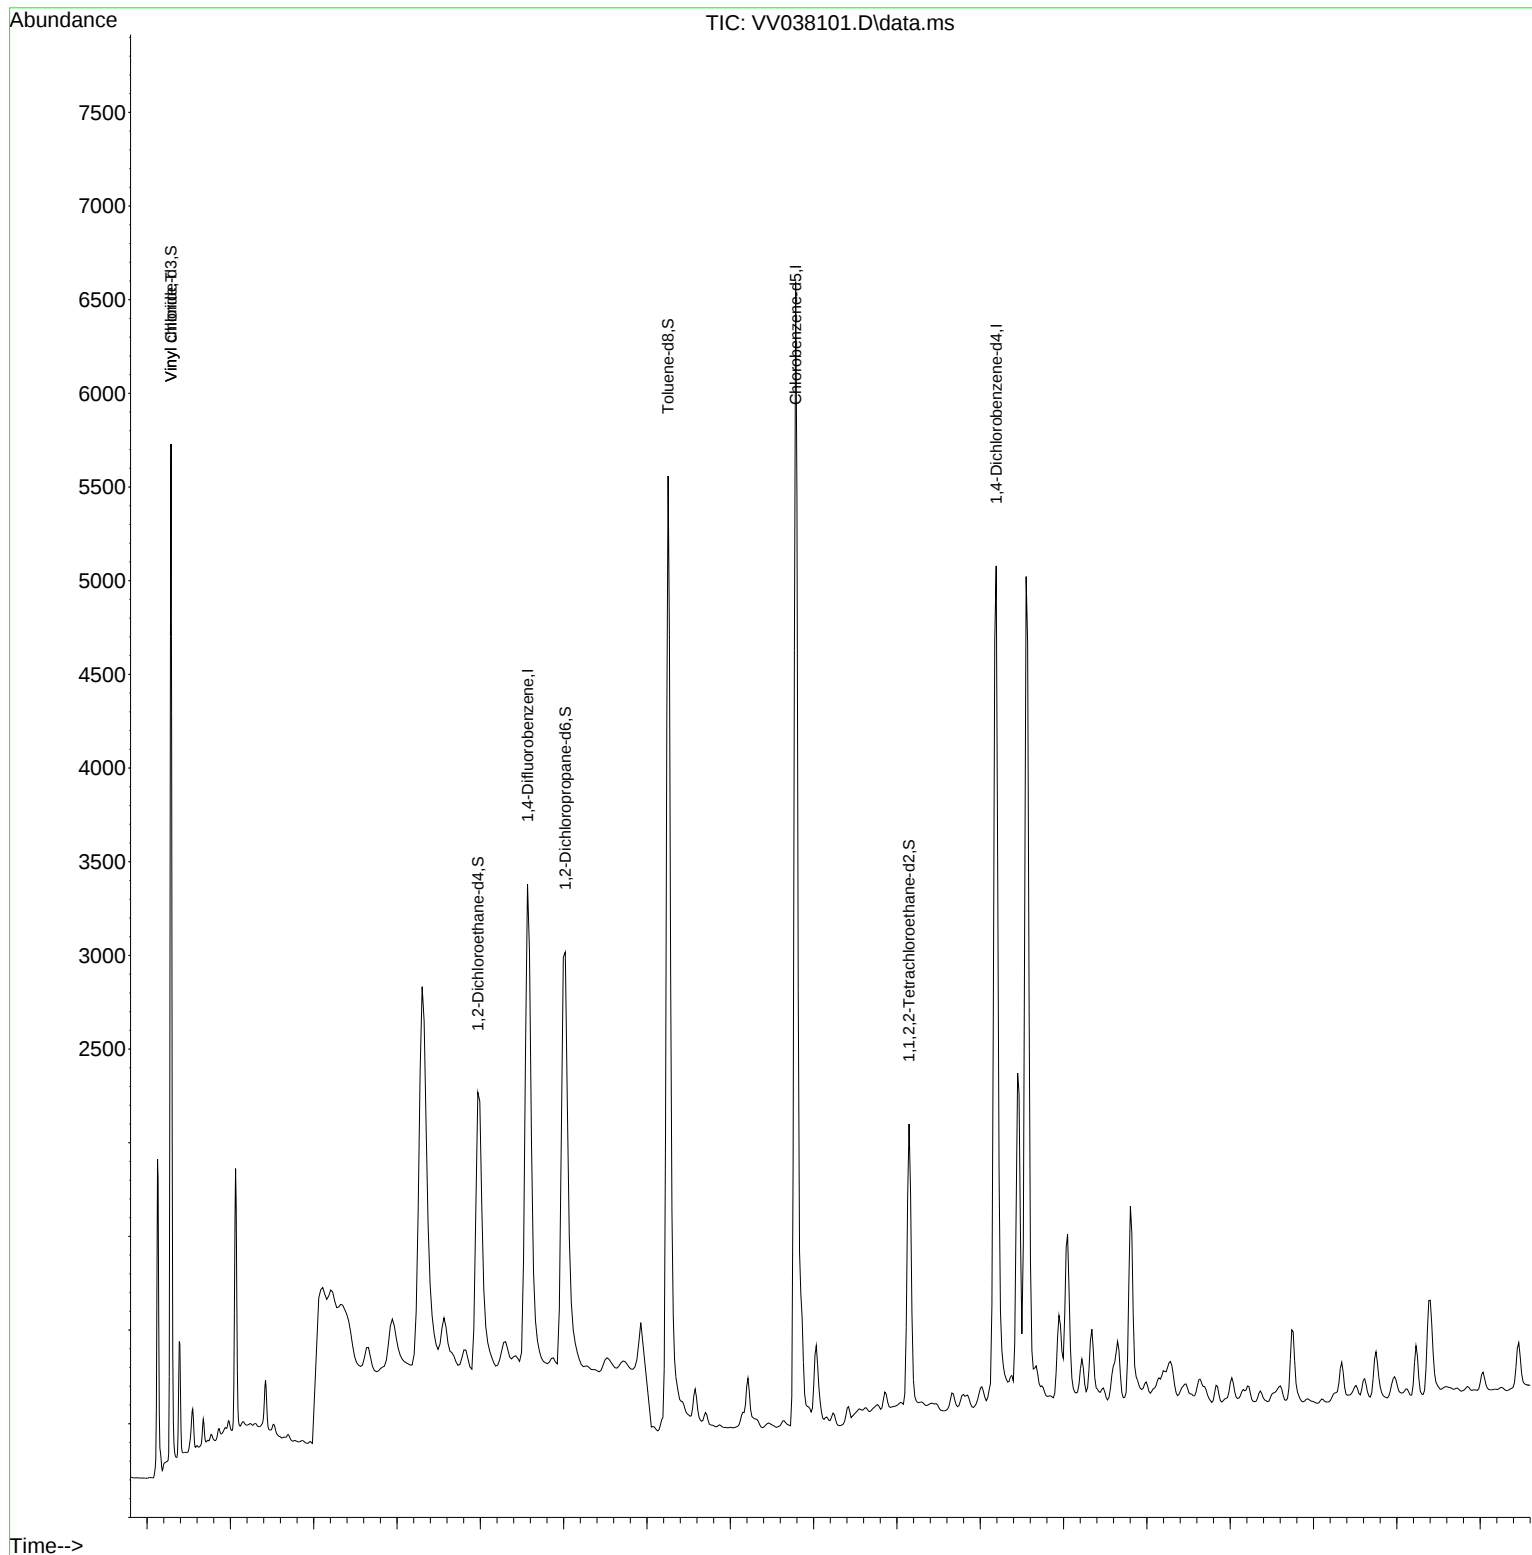


Abundance Scan 69 (1.280 min): VV038085.D\data.ms (-55)

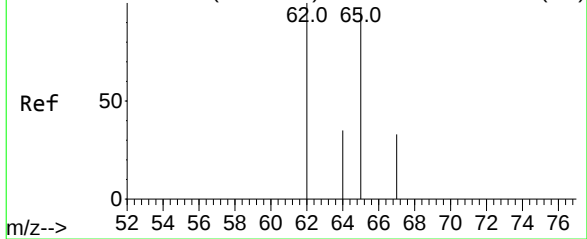

#3
Vinyl chloride
Concen: 0.039 ug/L m
RT: 1.287 min Scan# 70
Delta R.T. 0.007 min
Lab File: VV038101.D
Acq: 14 Nov 2024 21:44

Instrument :
MSVOA_V
ClientSampleId :
A0AL7

Abundance Scan 70 (1.287 min): VV038101.D\data.ms

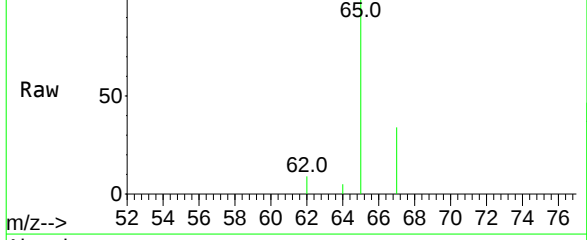

Tgt Ion: 62 Resp: 404
Ion Ratio Lower Upper
62 100
64 59.0 25.3 47.1#

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 11/18/2024
Supervised By :Mahesh Dadoda 11/18/2024

Abundance Scan 70 (1.287 min): VV038101.D\data.ms (-26)

