

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
 Data File : VV038106.D
 Acq On : 14 Nov 2024 23:44
 Operator : SY/MD
 Sample : P4761-21 10X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A0AP0

Quant Time: Nov 15 00:35:53 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 00:15:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	10165	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.785	117	9777	0.500	ug/L	-0.02
11) 1,4-Dichlorobenzene-d4	11.191	152	4693	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	6047	0.574	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	114.000%
4) 1,2-Dichloroethane-d4	4.970	65	4251	0.667	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	134.000%#
7) 1,2-Dichloropropane-d6	5.996	67	4258	0.538	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	108.000%
8) Toluene-d8	7.254	98	11034	0.544	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	108.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	3339	0.527	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	106.000%
Target Compounds						
3) Vinyl chloride	1.280	62	17850	1.704	ug/L	96
6) Trichloroethene	5.852	95	4122	0.576	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
Data File : VV038106.D
Acq On : 14 Nov 2024 23:44
Operator : SY/MD
Sample : P4761-21 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A0AP0

Quant Time: Nov 15 00:35:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

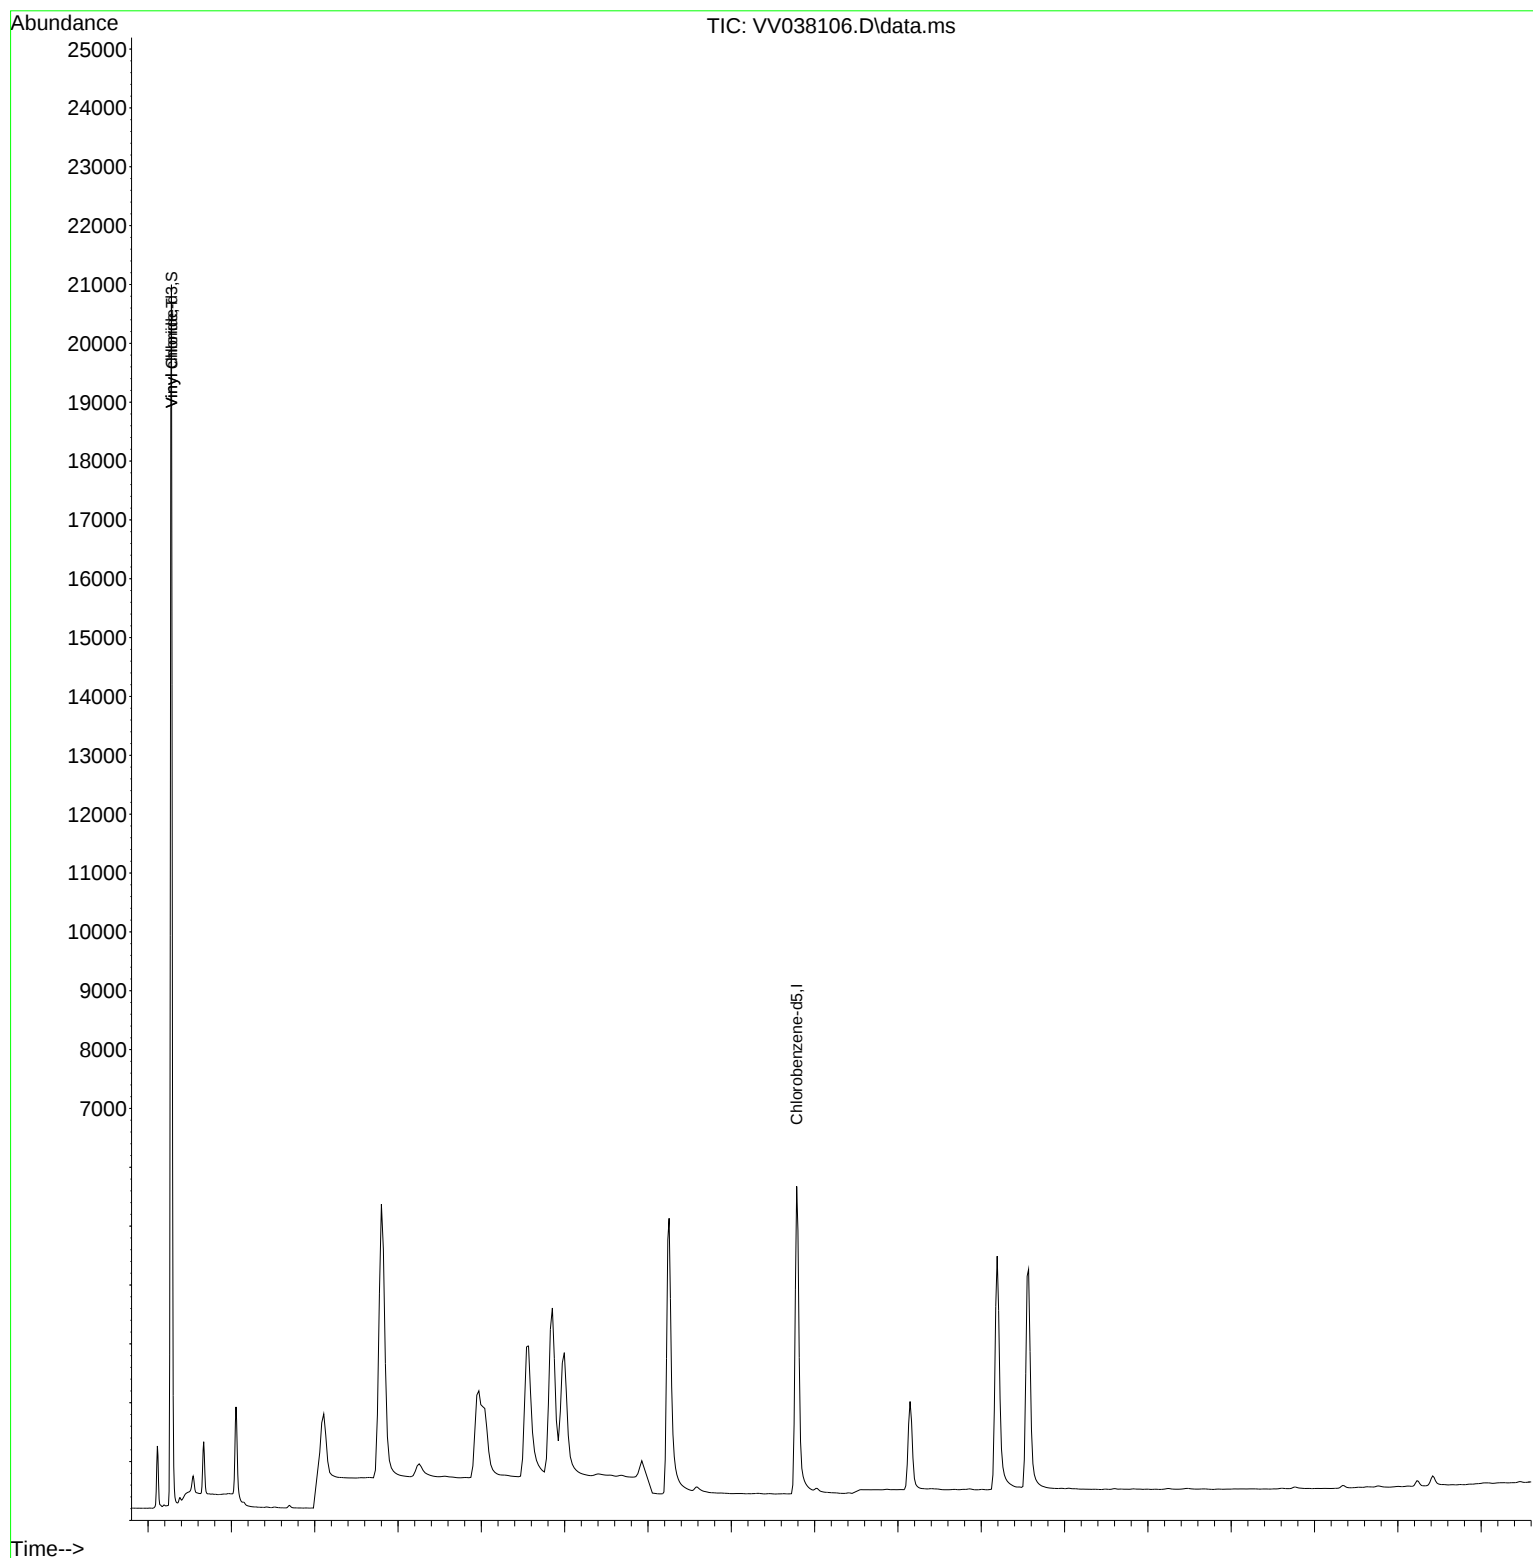

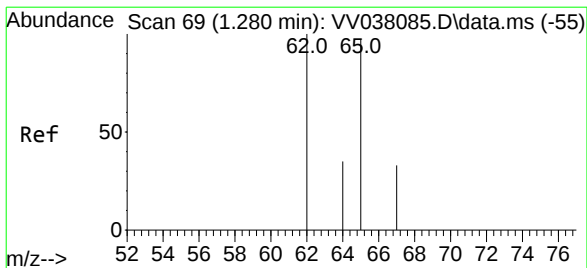

#3

Vinyl chloride

Concen: 1.704 ug/L

RT: 1.280 min Scan# 69

Delta R.T. 0.000 min

Lab File: VV038106.D

Acq: 14 Nov 2024 23:44

Instrument :

MSVOA_V

ClientSampleId :





A0AP0

Tgt Ion: 62 Resp: 17850

Ion Ratio Lower Upper

62 100

64 34.1 25.3 47.1

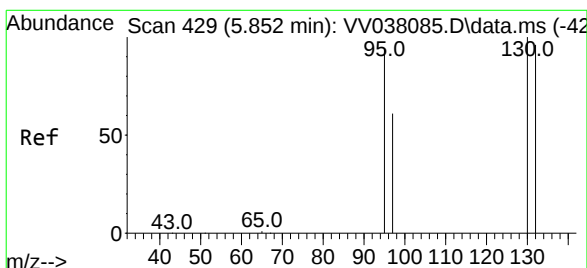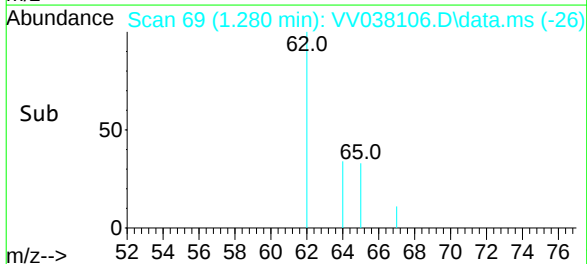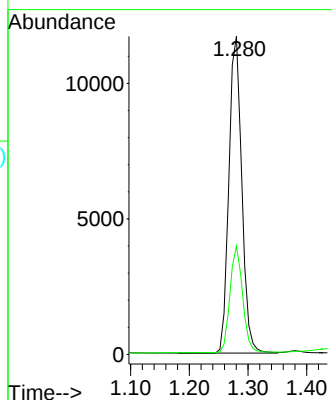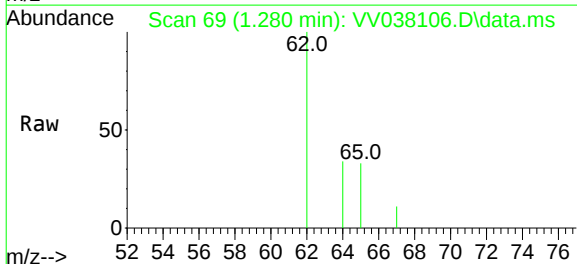

#6

Trichloroethene

Concen: 0.576 ug/L

RT: 5.852 min Scan# 429

Delta R.T. 0.000 min

Lab File: VV038106.D

Acq: 14 Nov 2024 23:44

Tgt Ion: 95 Resp: 4122

Ion Ratio Lower Upper

95 100

97 67.2 46.5 86.5

132 101.0 70.3 130.7

130 104.8 73.4 136.4

