

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
 Data File : VV038110.D
 Acq On : 15 Nov 2024 02:08
 Operator : SY/MD
 Sample : P4761-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A0AM8

Quant Time: Nov 15 04:16:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 00:15:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	8883	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	8762	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	4197	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	5616	0.610	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	122.000%
4) 1,2-Dichloroethane-d4	4.969	65	3373	0.605	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	122.000%
7) 1,2-Dichloropropane-d6	5.995	67	3948	0.556	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	112.000%
8) Toluene-d8	7.253	98	9960	0.548	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	110.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	3216	0.567	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	114.000%
Target Compounds						
6) Trichloroethene	5.852	95	190	0.030	ug/L	Qvalue 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
Data File : VV038110.D
Acq On : 15 Nov 2024 02:08
Operator : SY/MD
Sample : P4761-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A0AM8

Quant Time: Nov 15 04:16:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

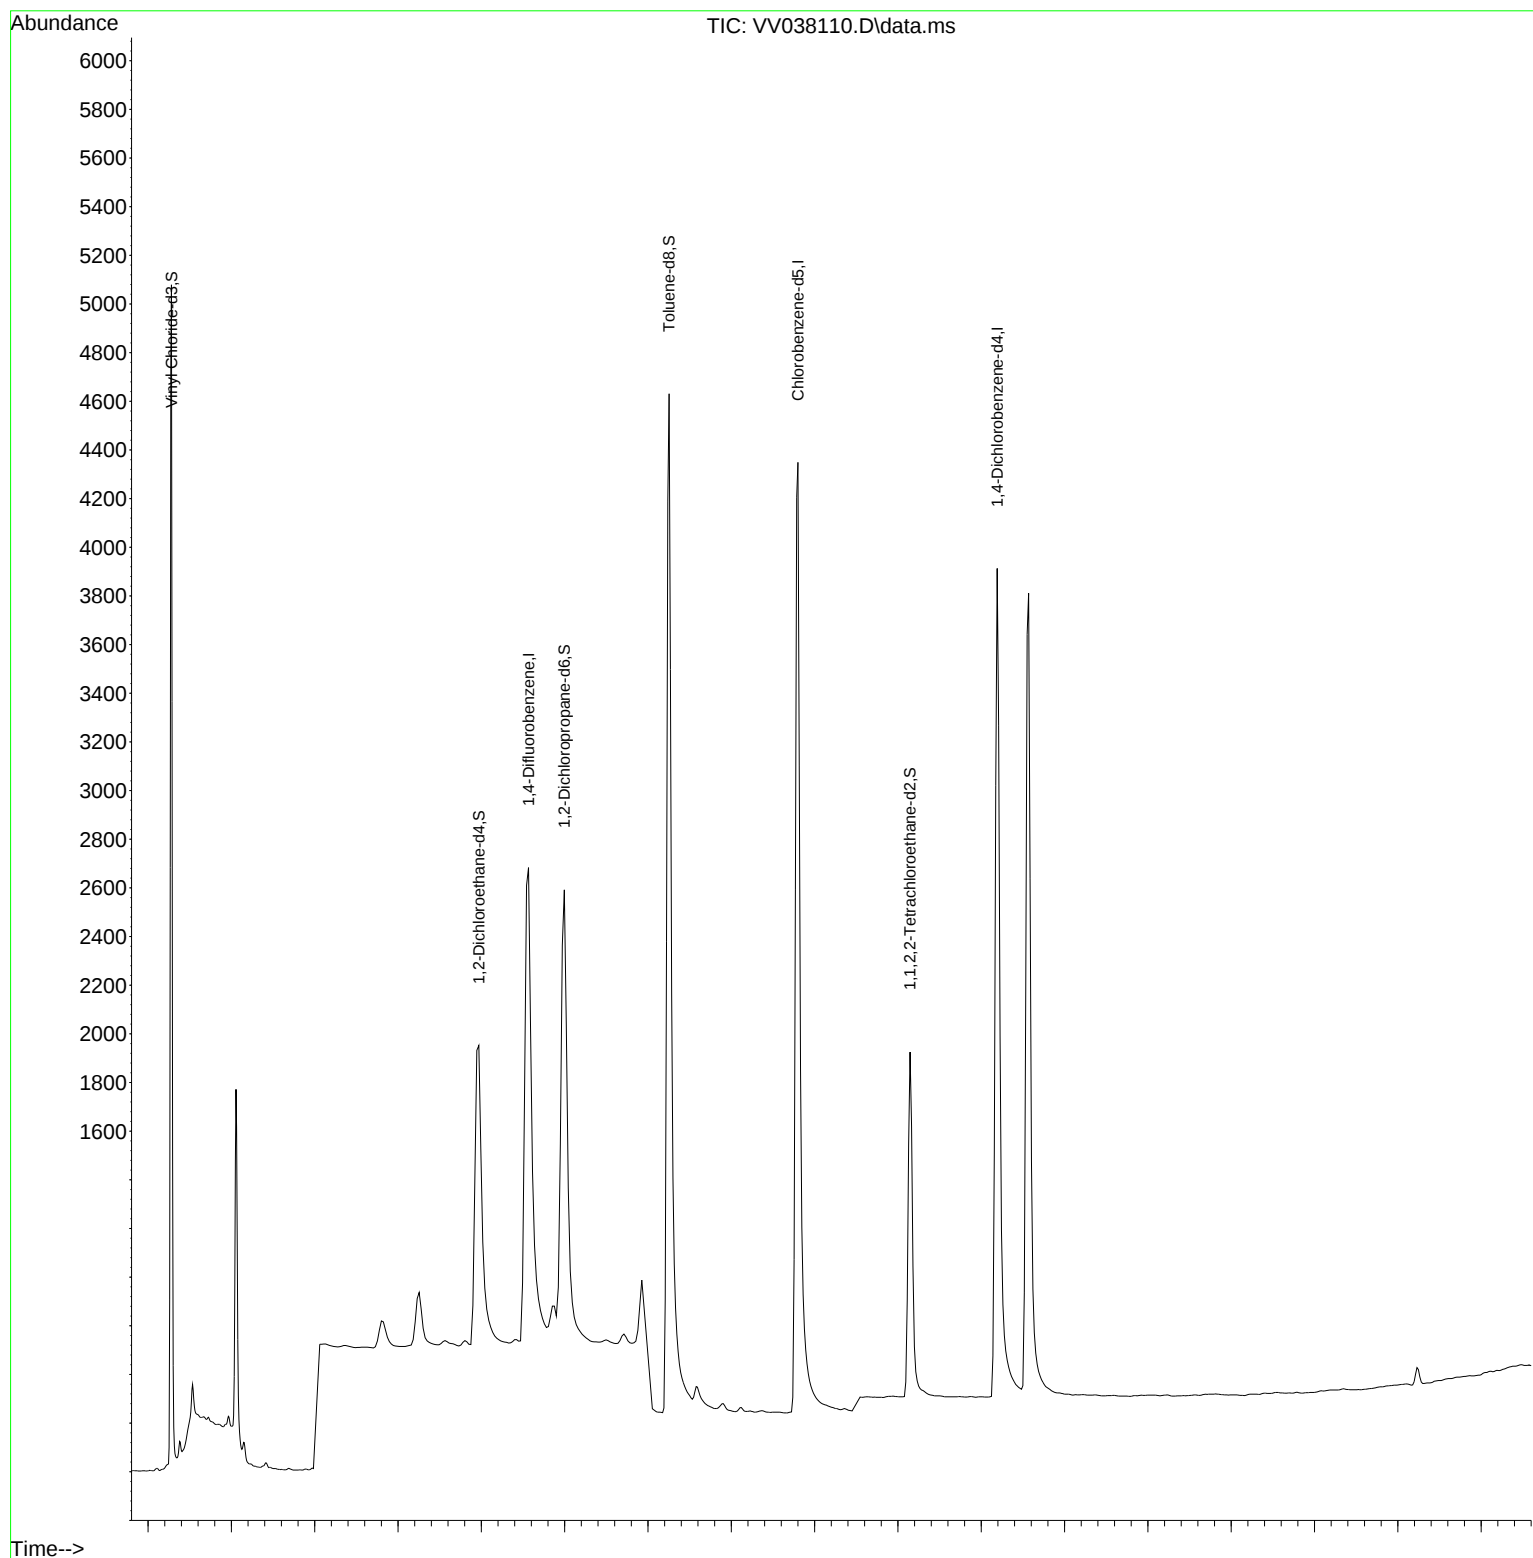

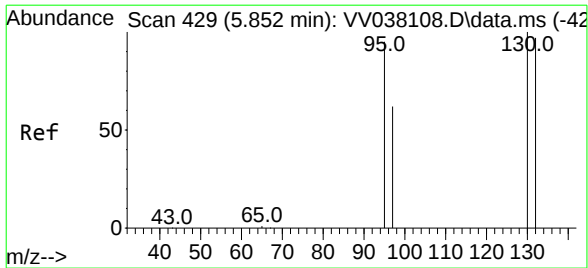

Trichloroethene

Concen: 0.030 ug/L

RT: 5.852 min Scan# 42

Delta R.T. 0.000 min

Lab File: VV038110.D


Acq: 15 Nov 2024 02:08

Instrument :

MSVOA_V

ClientSampleId :

A0AM8

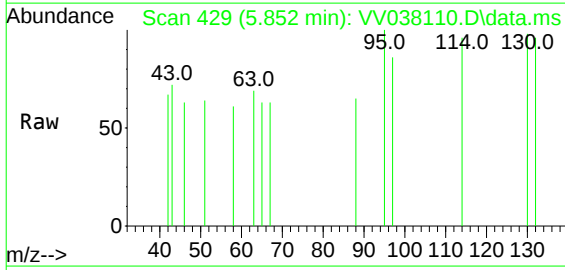

Tgt Ion: 95 Resp: 190

Ion Ratio Lower Upper

95 100

97 85.5 46.5 86.5

132 96.4 70.3 130.7

130 97.6 73.4 136.4

