

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
 Data File : VV038117.D
 Acq On : 15 Nov 2024 04:56
 Operator : SY/MD
 Sample : P4803-06 2X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A0AQ1

Quant Time: Nov 15 06:19:34 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 00:15:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	9523	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.785	117	9697	0.500	ug/L	-0.01
11) 1,4-Dichlorobenzene-d4	11.192	152	5133	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.274	65	5439	0.551	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	110.000%
4) 1,2-Dichloroethane-d4	4.970	65	3440	0.576	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	116.000%
7) 1,2-Dichloropropane-d6	5.996	67	4056	0.516	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	104.000%
8) Toluene-d8	7.254	98	10198	0.507	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	102.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	3265	0.520	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	104.000%
Target Compounds						
3) Vinyl chloride	1.274	62	1253	0.128	ug/L	Qvalue 82

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
Data File : VV038117.D
Acq On : 15 Nov 2024 04:56
Operator : SY/MD
Sample : P4803-06 2X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A0AQ1

Quant Time: Nov 15 06:19:34 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

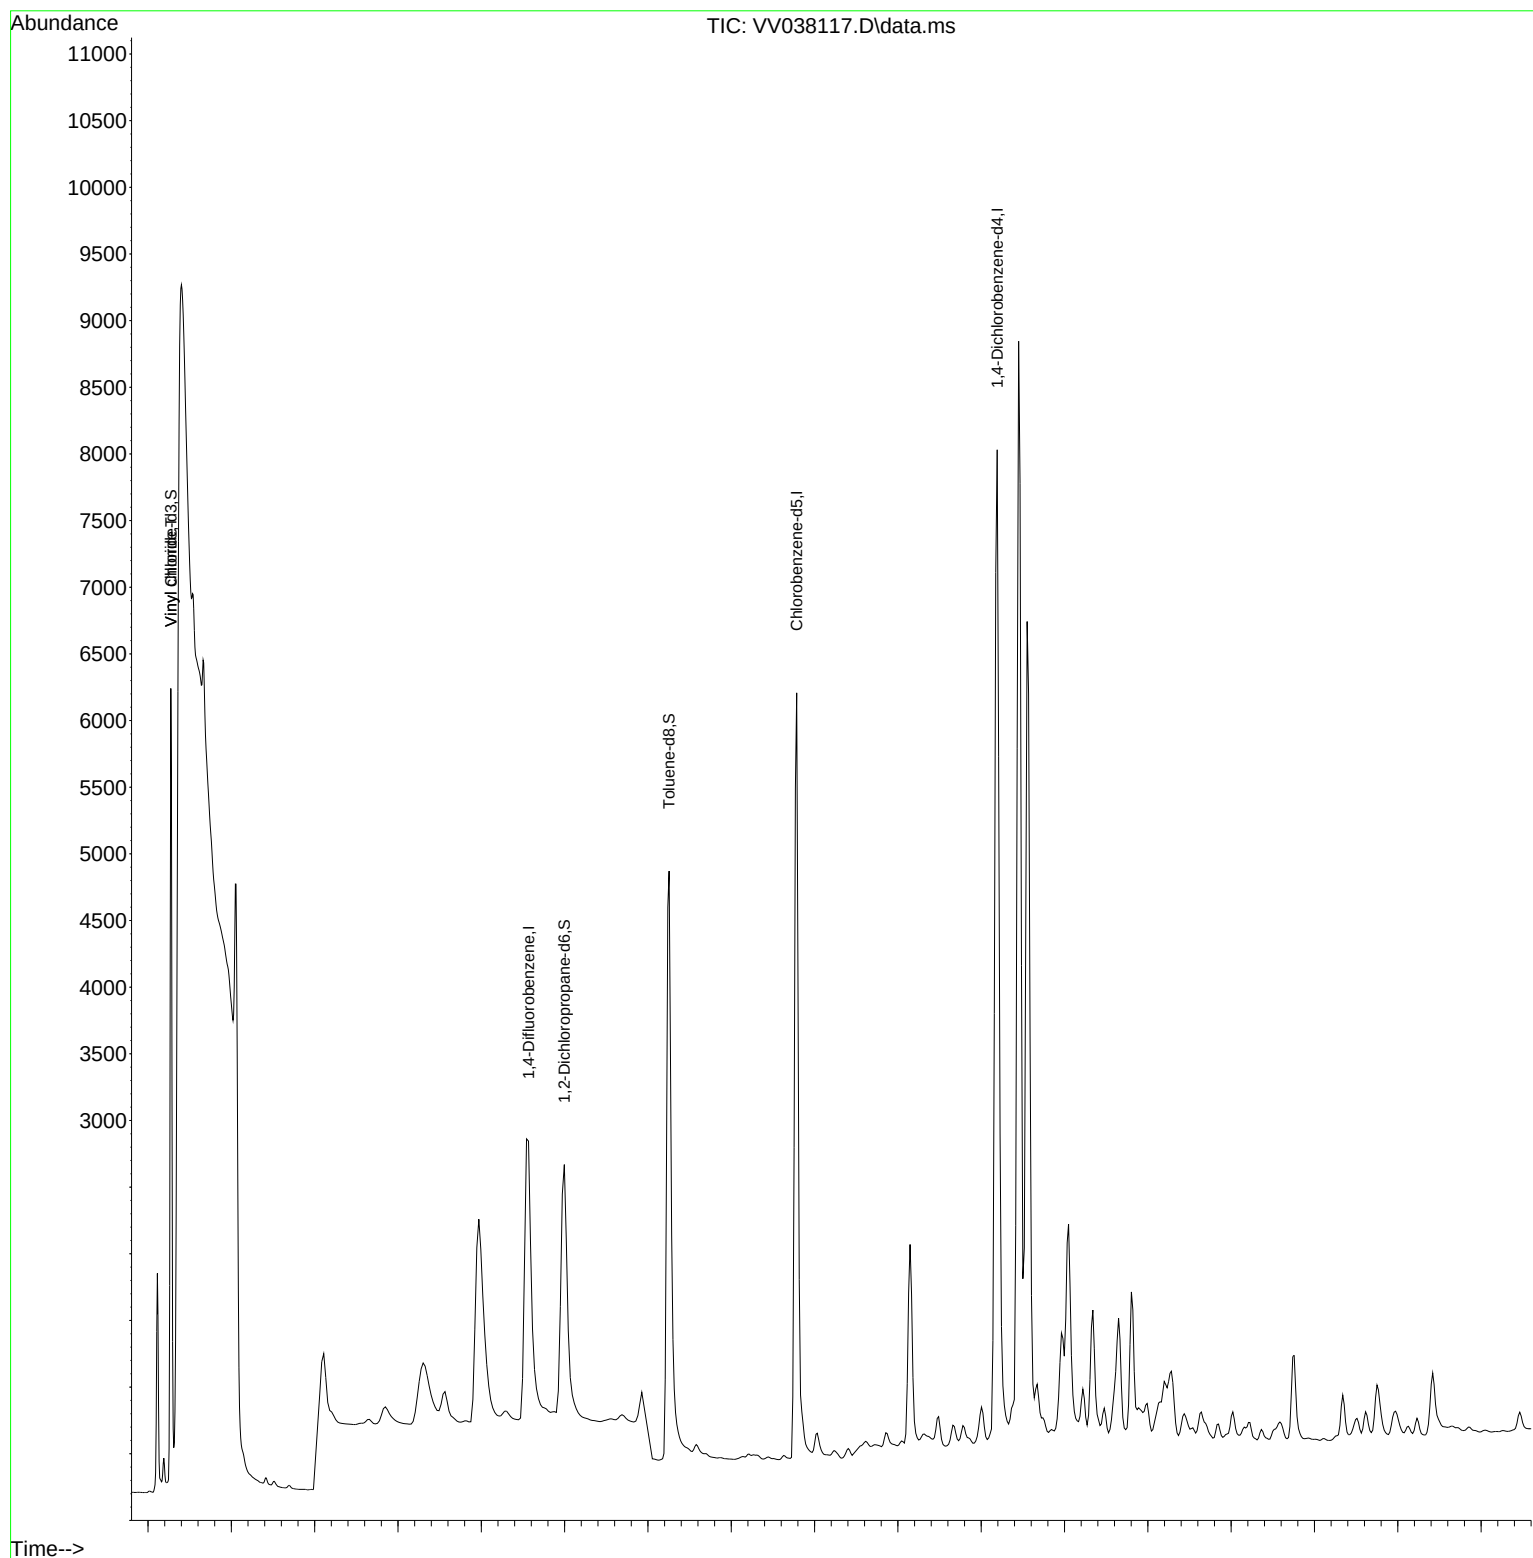

Abundance Scan 69 (1.280 min): VV038108.D\data.ms (-54)

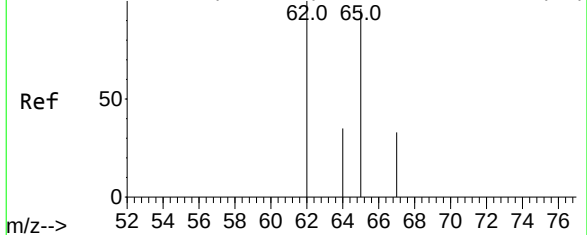

#3

Vinyl chloride

Concen: 0.128 ug/L

RT: 1.274 min Scan# 68

Delta R.T. -0.007 min

Lab File: VV038117.D

Acq: 15 Nov 2024 04:56


Instrument :

MSVOA_V

ClientSampleId :

A0AQ1

Abundance Scan 68 (1.274 min): VV038117.D\data.ms

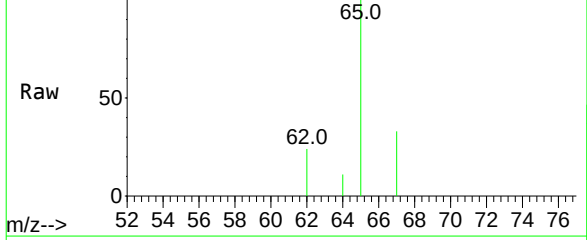

Tgt Ion: 62 Resp: 1253

Ion Ratio Lower Upper

62 100

64 46.8 25.3 47.1

Abundance Scan 68 (1.274 min): VV038117.D\data.ms (-26)

