
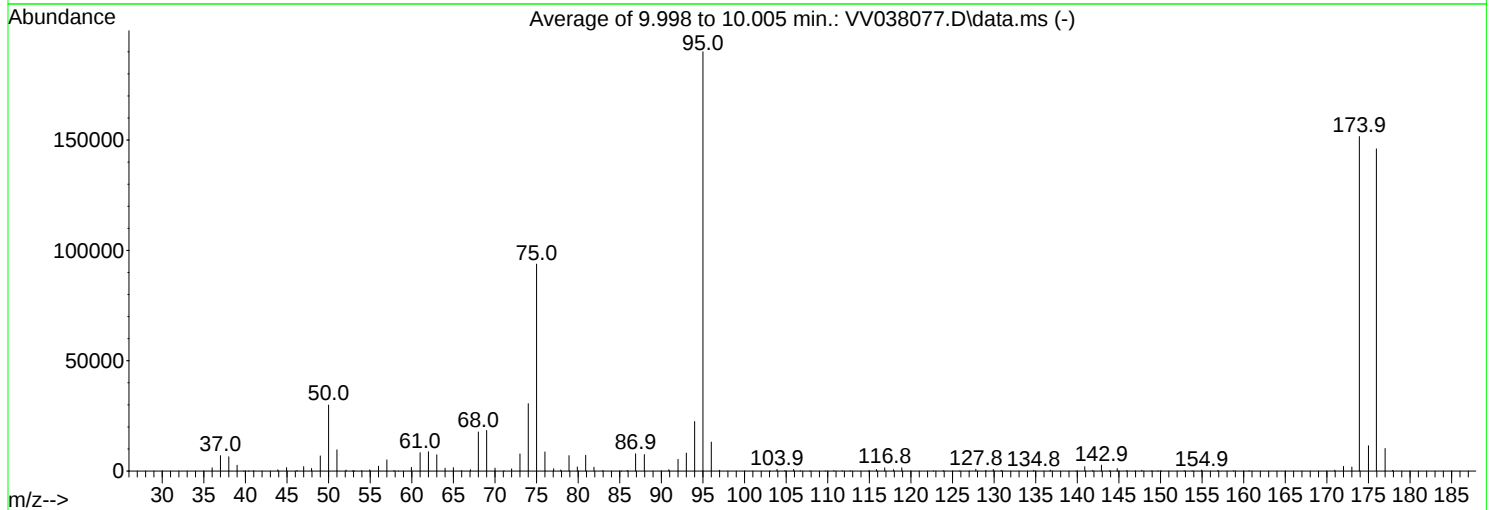


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
Data File : VV038077.D
Acq On : 14 Nov 2024 08:11
Operator : SY/MD
Sample : BFB222
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB222

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Title : TRACE VOA SOM01.0
Last Update : Fri Nov 15 00:15:53 2024

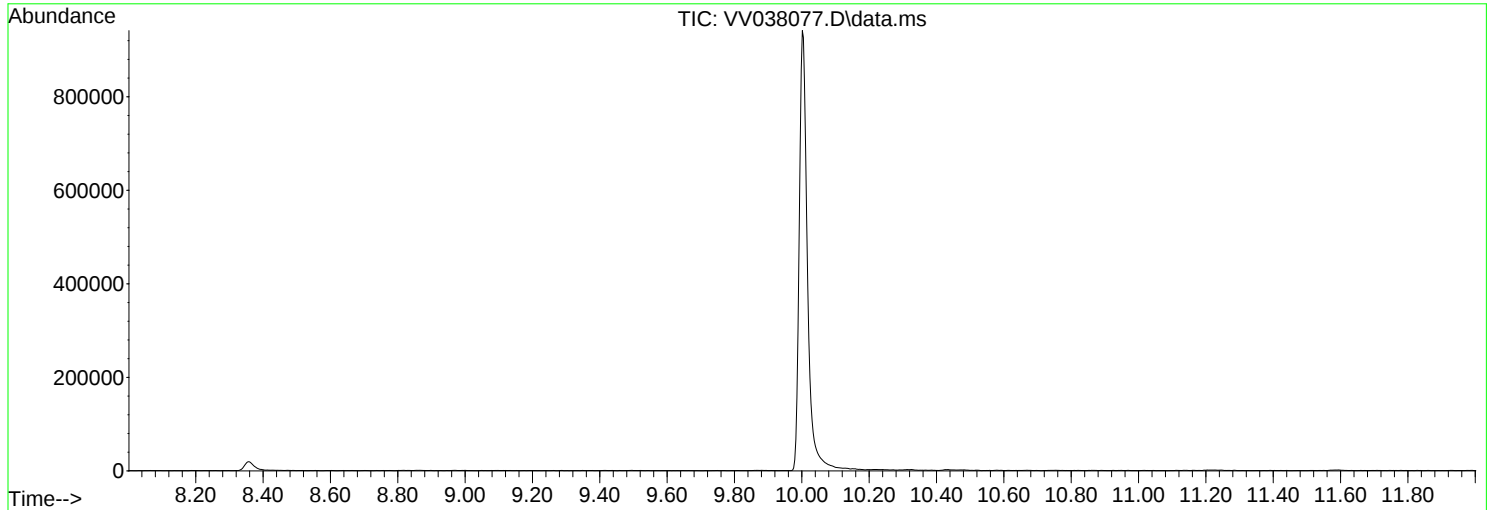

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2775

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	29936	PASS
75	95	30	80	49.4	93813	PASS
95	95	100	100	100.0	190037	PASS
96	95	5	9	6.9	13156	PASS
173	174	0.00	2	1.2	1850	PASS
174	95	50	120	79.8	151616	PASS
175	174	5	9	7.6	11489	PASS
176	174	95	101	96.3	146027	PASS
177	176	5	9	7.0	10259	PASS

m/z	Abundance
39.80	287.0
43.90	415.0

Instrument :
MSVOA_V
ClientSampleId :
BFB222

m/z	Abundance
36.00	1426.0
37.00	6514.0
38.00	6320.0
39.00	2612.0
39.90	381.0
41.00	130.0
44.00	958.0
44.90	1527.0
46.20	248.0
47.00	1909.0
47.90	1262.0
49.00	6625.0
50.00	28720.0
51.00	9323.0
52.10	416.0
52.90	188.0
53.90	148.0
54.90	586.0
56.00	2178.0
57.00	4819.0
57.90	341.0
60.00	1661.0
61.00	8030.0
62.00	8313.0
63.00	7153.0
64.00	1153.0
65.00	1557.0
66.00	223.0
67.10	589.0
68.00	17048.0
69.00	17576.0
70.00	1224.0
72.00	926.0
73.00	7841.0
74.00	29736.0
75.00	89888.0
76.00	8238.0
77.00	1040.0
77.80	422.0
78.90	6434.0
79.90	1756.0
80.90	6816.0
81.90	1620.0
82.90	214.0
85.90	279.0
86.90	7639.0
87.90	6601.0
90.90	641.0
92.00	4921.0
93.00	7689.0
94.00	21472.0
95.00	181440.0
96.00	12378.0
97.00	406.0
103.10	103.0
103.90	750.0
104.80	265.0
105.90	670.0
106.70	217.0
110.70	217.0
111.70	126.0
112.70	173.0
115.00	198.0
115.80	656.0
116.90	1323.0
117.90	619.0
118.90	1371.0
122.70	135.0
123.90	223.0
127.80	757.0
129.00	323.0
129.90	662.0
130.80	356.0
134.80	404.0
136.80	529.0
139.90	129.0
140.90	1954.0
141.80	254.0
142.90	2632.0
143.90	190.0
144.80	1058.0
145.90	256.0
147.80	327.0
149.00	134.0
149.70	196.0
152.80	187.0
153.80	173.0
154.90	463.0
156.80	282.0
158.80	160.0
160.60	134.0
171.00	508.0

Instrument :
MSVOA_V
ClientSampleId :
BFB222

172.00	2126.0
173.00	1853.0
173.90	138240.0
175.00	11234.0
175.90	135104.0
177.00	10206.0
177.90	309.0

Instrument :
MSVOA_V
ClientSampleId :
BFB222

m/z	Abundance
36.00	1583.0
37.00	7296.0
38.00	6801.0
39.00	2731.0
39.80	409.0
41.00	125.0
44.00	987.0
45.00	1709.0
46.20	315.0
47.00	2110.0
48.00	1236.0
49.00	7245.0
50.00	30920.0
51.00	10088.0
52.10	482.0
52.90	210.0
53.90	166.0
54.90	566.0
56.00	2275.0
57.00	5352.0
57.80	282.0
60.00	1741.0
61.00	8562.0
62.00	9166.0
63.00	7608.0
64.00	1346.0
65.00	1630.0
66.00	206.0
67.10	672.0
68.00	18384.0
69.00	19168.0
70.00	1394.0
72.00	983.0
73.00	8025.0
74.00	31520.0
75.00	97024.0
76.00	9186.0
77.00	1081.0
77.90	467.0
78.90	7387.0
79.90	1968.0
80.90	7501.0
81.90	1808.0
83.00	254.0
85.20	104.0
85.90	305.0
86.90	8093.0
88.00	7681.0
90.90	710.0
92.00	5548.0
93.00	8453.0
94.00	23112.0
95.00	196544.0
96.00	13659.0
97.00	383.0
103.90	821.0
104.90	271.0
105.90	776.0
106.70	224.0
107.80	110.0
109.70	132.0
110.70	233.0
111.80	177.0
112.70	185.0
115.00	225.0
115.80	743.0
116.90	1575.0
117.90	697.0
118.90	1585.0
122.70	169.0
123.90	248.0
125.80	112.0
127.80	903.0
129.00	317.0
129.90	749.0
130.80	353.0
134.80	399.0
136.80	475.0
139.80	109.0
140.90	2058.0
141.80	274.0
142.90	2810.0
143.90	220.0
144.80	1229.0
145.90	255.0
146.90	120.0
147.70	404.0
148.90	116.0
149.70	215.0
152.80	177.0
153.80	142.0
154.90	512.0

Instrument :
MSVOA_V
ClientSampleId :
BFB222

156.90	297.0
158.80	236.0
160.60	158.0
171.00	457.0
172.00	2221.0
173.00	1939.0
173.90	157056.0
175.00	11828.0
175.90	151680.0
177.00	10645.0
177.90	320.0

Instrument : MSVOA_V
ClientSampleId : BFB222

m/z	Abundance
36.00	1518.0
37.00	7236.0
38.00	6423.0
39.00	2668.0
39.80	412.0
40.40	170.0
43.90	1109.0
45.00	1549.0
46.20	330.0
47.00	2095.0
48.00	1031.0
49.00	6762.0
50.00	30168.0
51.00	9522.0
52.10	486.0
53.10	192.0
54.00	161.0
55.00	545.0
56.00	2229.0
57.00	5105.0
57.90	196.0
58.40	100.0
59.90	1664.0
61.00	8455.0
62.00	8820.0
63.00	7400.0
64.00	1398.0
65.00	1475.0
65.90	163.0
67.00	628.0
68.00	17784.0
69.00	18512.0
70.00	1423.0
71.10	117.0
72.00	1068.0
73.00	7529.0
74.00	30424.0
75.00	94528.0
76.00	8599.0
77.10	1156.0
78.00	585.0
78.90	7192.0
79.90	1997.0
80.90	7233.0
81.90	1852.0
83.00	225.0
85.20	111.0
85.90	305.0
86.90	7767.0
87.90	8175.0
90.90	701.0
92.00	5501.0
93.00	8356.0
94.00	22832.0
95.00	192128.0
96.00	13431.0
97.00	320.0
103.90	849.0
104.80	265.0
105.90	828.0
106.80	140.0
107.90	119.0
109.70	122.0
110.80	188.0
111.80	195.0
112.70	181.0
114.90	206.0
115.90	738.0
116.80	1588.0
117.90	738.0
118.90	1518.0
122.70	135.0
123.90	197.0
125.80	138.0
127.00	108.0
127.80	923.0
129.00	308.0
129.90	815.0
130.90	302.0
134.70	364.0
136.70	350.0
140.90	1969.0
141.90	252.0
142.90	2723.0
143.90	238.0
144.80	1109.0
146.00	222.0
147.00	153.0
147.70	388.0
150.10	238.0
152.90	168.0
155.00	457.0

Instrument :
MSVOA_V
ClientSampleId :
BFB222

157.00	326.0
158.80	287.0
160.70	183.0
170.90	352.0
172.00	2048.0
173.00	1758.0
173.90	159552.0
175.00	11404.0
176.00	151296.0
177.00	9925.0
177.90	287.0

Instrument :
MSVOA_V
ClientSampleId :
BFB222