

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111524\
 Data File : VV038130.D
 Acq On : 15 Nov 2024 11:45
 Operator : SY/MD
 Sample : P4847-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 15 22:10:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 00:15:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	7797	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	7791	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	3877	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.273	65	4025	0.498	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	100.000%
4) 1,2-Dichloroethane-d4	4.970	65	2391	0.489	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	98.000%
7) 1,2-Dichloropropane-d6	5.996	67	2785	0.441	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	88.000%
8) Toluene-d8	7.254	98	6962	0.431	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	86.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	2238	0.444	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	88.000%
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.168	75	31	0.046	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111524\
Data File : VV038130.D
Acq On : 15 Nov 2024 11:45
Operator : SY/MD
Sample : P4847-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Nov 15 22:10:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

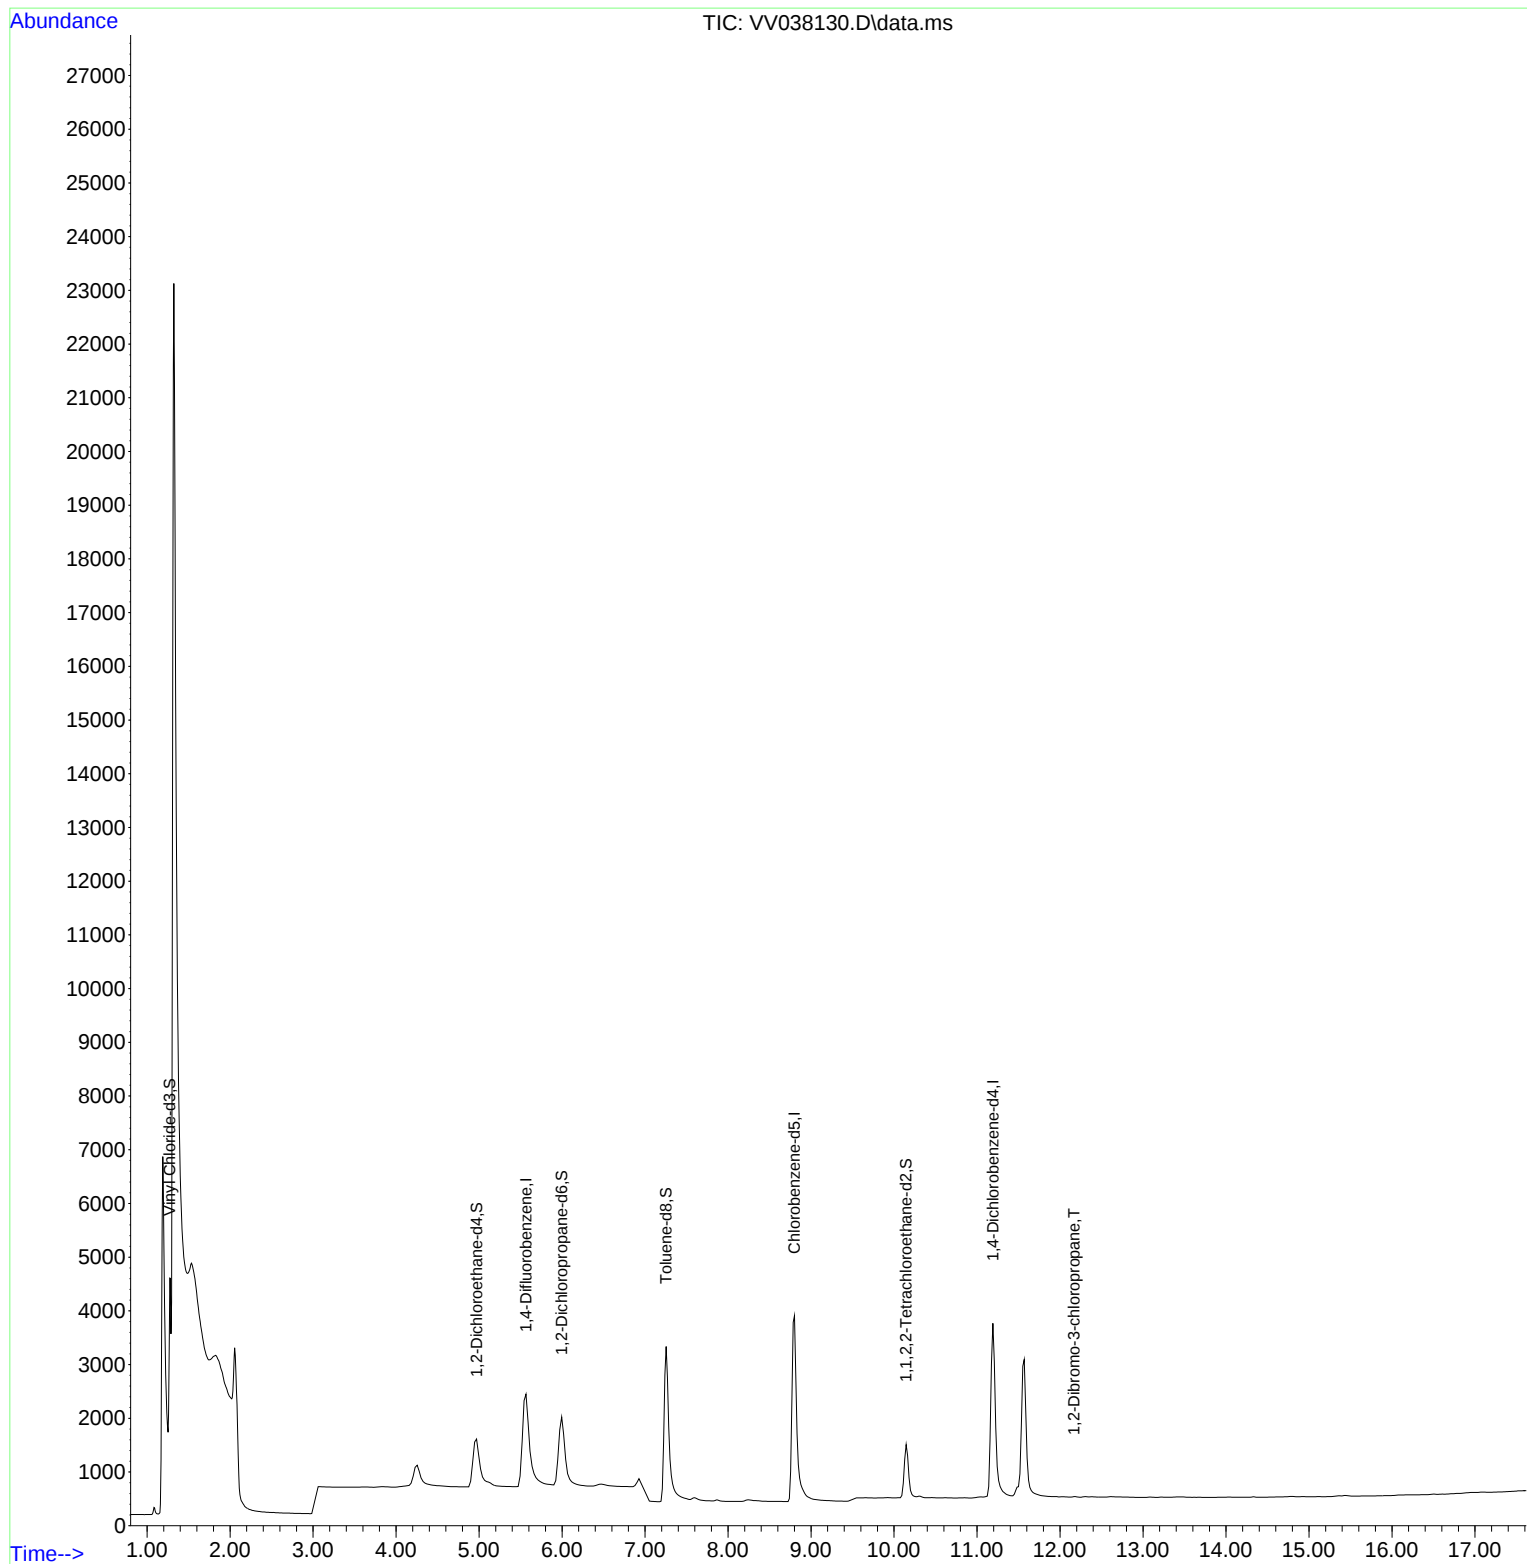

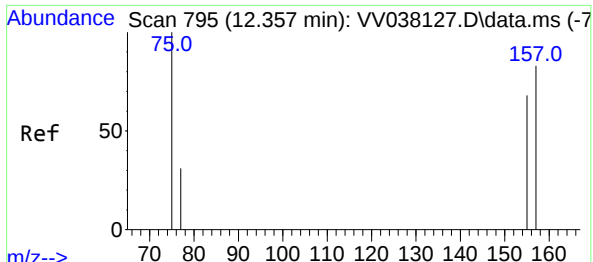

#13
1,2-Dibromo-3-chloropropane
Concen: 0.046 ug/L
RT: 12.168 min Scan# 74
Delta R.T. -0.188 min
Lab File: VV038130.D
Acq: 15 Nov 2024 11:45

Instrument :
MSVOA_V
ClientSampleId :

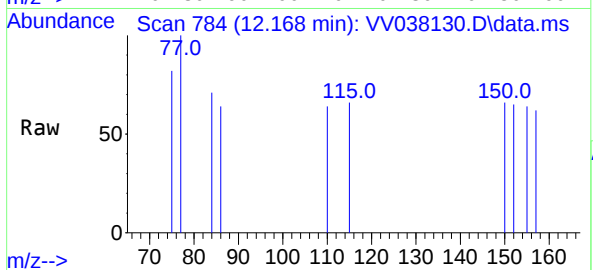

Tgt Ion:	75	Resp:	31
Ion	Ratio	Lower	Upper
75	100		
157	76.2	69.4	104.0
155	77.8	61.3	91.9

