

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111524\
 Data File : VV038131.D
 Acq On : 15 Nov 2024 12:09
 Operator : SY/MD
 Sample : P4847-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 15 22:10:55 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 00:15:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	9473	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.785	117	10248	0.500	ug/L	-0.02
11) 1,4-Dichlorobenzene-d4	11.191	152	5123	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.273	65	5958	0.607	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	122.000%
4) 1,2-Dichloroethane-d4	4.969	65	3542	0.596	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	120.000%
7) 1,2-Dichloropropane-d6	5.995	67	4462	0.538	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	108.000%
8) Toluene-d8	7.253	98	11091	0.522	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	104.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	3668	0.553	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	110.000%
Target Compounds						
						Qvalue
3) Vinyl chloride	1.280	62	195	0.020	ug/L	# 1
13) 1,2-Dibromo-3-chloropr...	12.476	75	23	0.026	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111524\
Data File : VV038131.D
Acq On : 15 Nov 2024 12:09
Operator : SY/MD
Sample : P4847-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Nov 15 22:10:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration




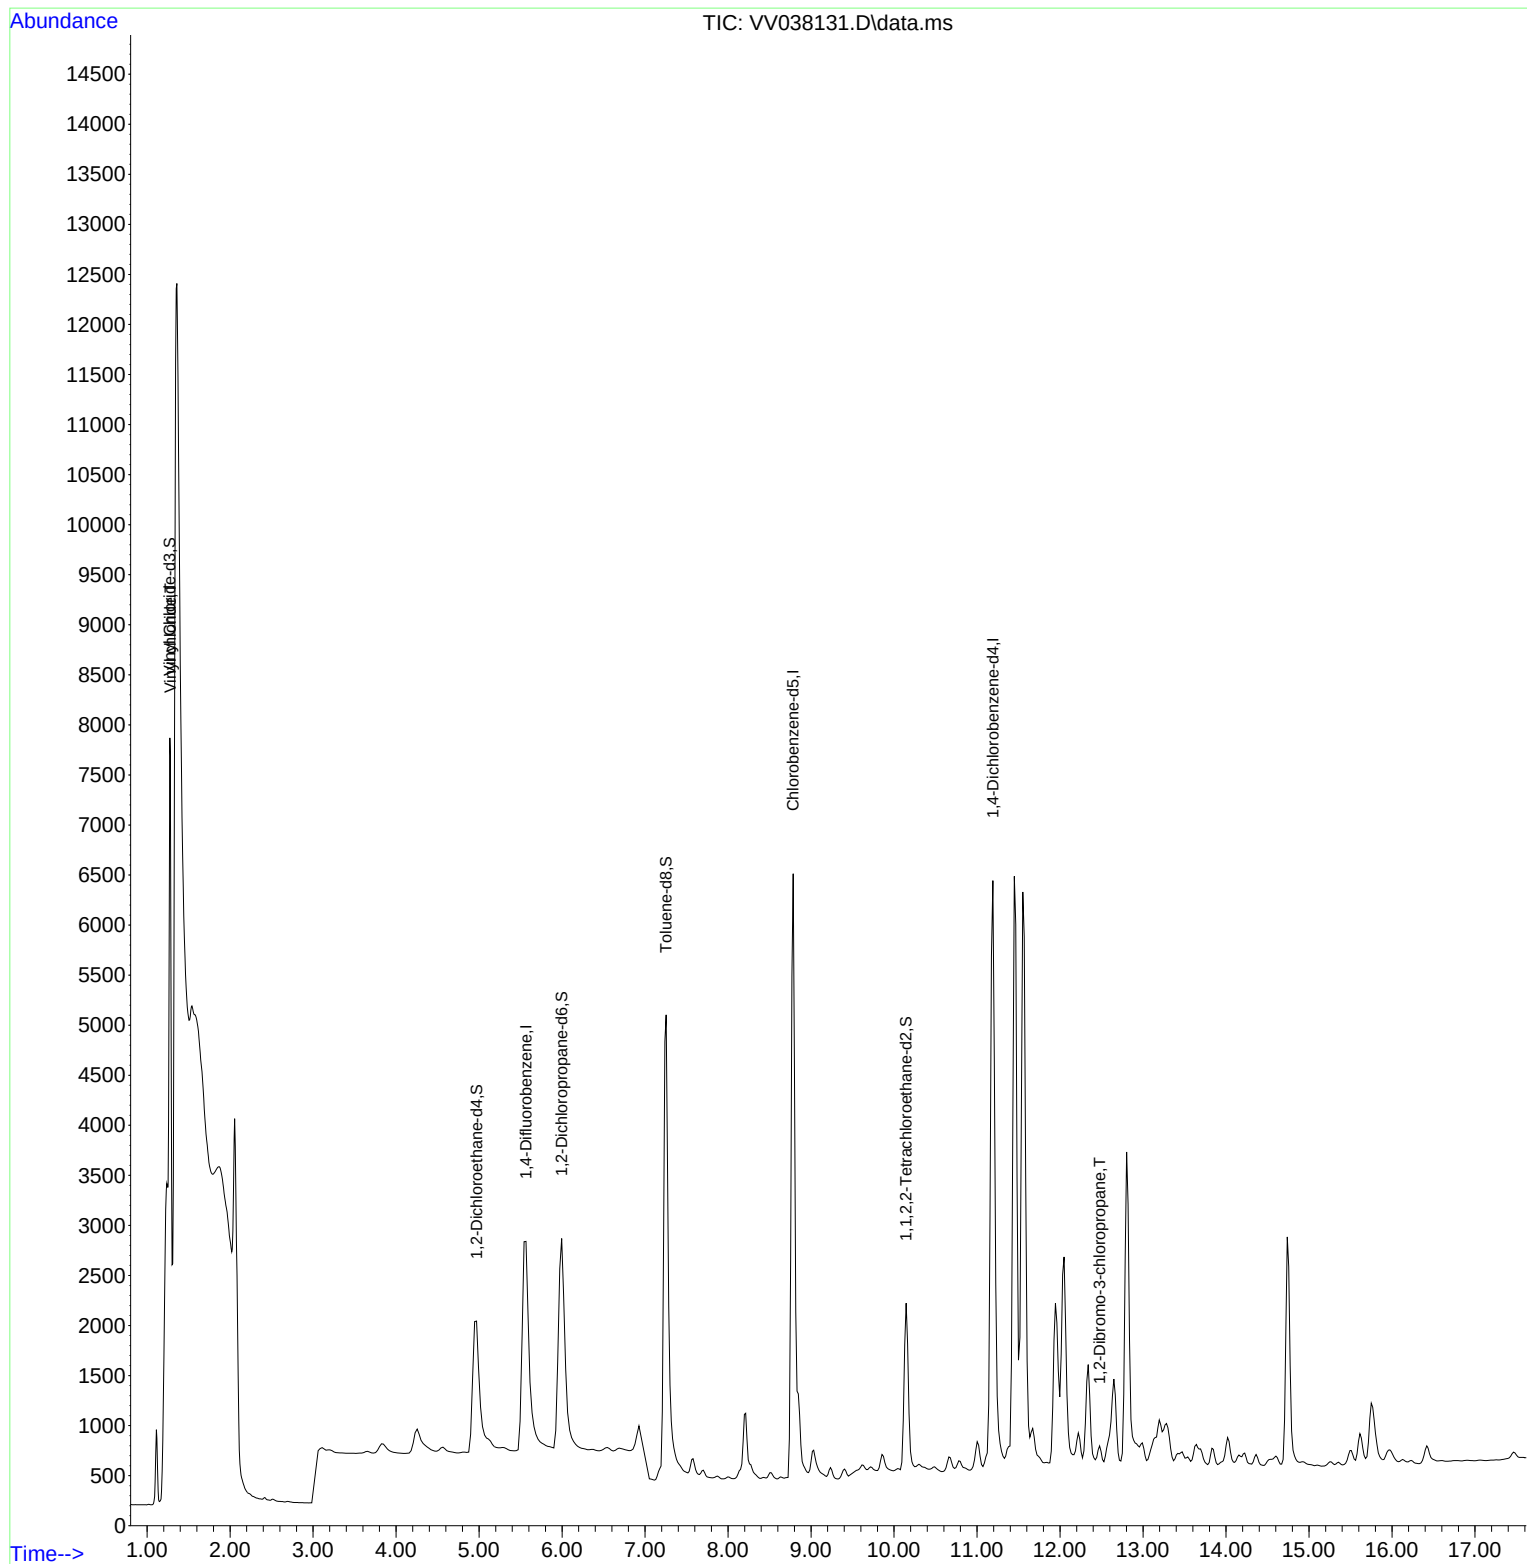


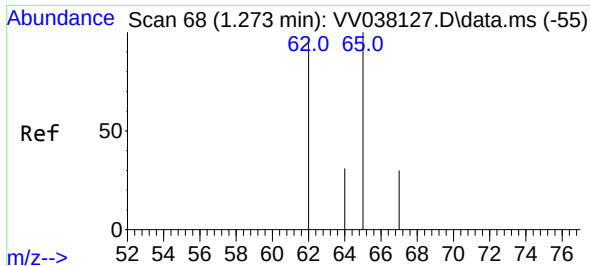

#3
Vinyl chloride
Concen: 0.020 ug/L
RT: 1.280 min Scan# 61
Delta R.T. 0.000 min
Lab File: VV038131.D
Acq: 15 Nov 2024 12:09

Instrument :
MSVOA_V
ClientSampleId :

Tgt Ion: 62 Resp: 195
Ion Ratio Lower Upper
62 100
64 1473.7 25.3 47.1#

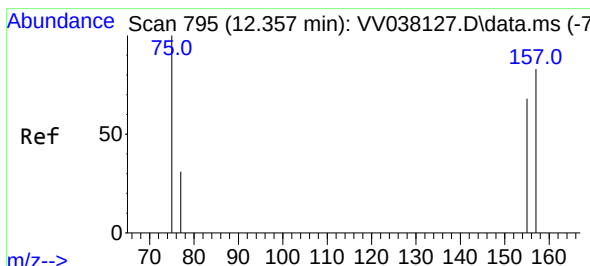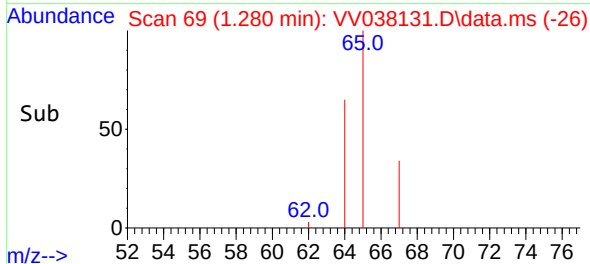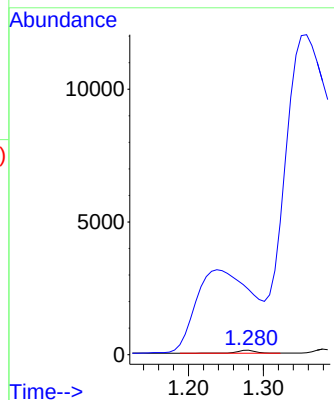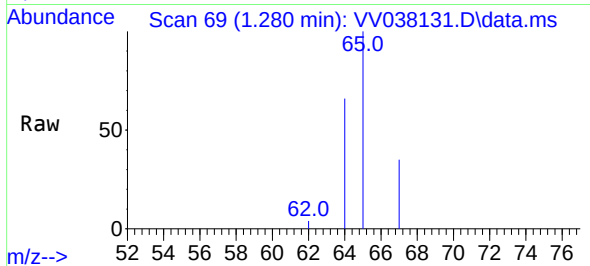

#13
1,2-Dibromo-3-chloropropane
Concen: 0.026 ug/L
RT: 12.476 min Scan# 802
Delta R.T. 0.120 min
Lab File: VV038131.D
Acq: 15 Nov 2024 12:09

Tgt Ion: 75 Resp: 23
Ion Ratio Lower Upper
75 100
157 70.0 69.4 104.0
155 70.0 61.3 91.9

