

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111524\
 Data File : VV038137.D
 Acq On : 15 Nov 2024 15:23
 Operator : SY/MD
 Sample : P4803-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 15 22:11:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 00:15:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	9823	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	9942	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	4866	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.273	65	5482	0.538	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery = 108.000%			
4) 1,2-Dichloroethane-d4	4.969	65	3065	0.497	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 100.000%			
7) 1,2-Dichloropropane-d6	5.995	67	3555	0.441	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery = 88.000%			
8) Toluene-d8	7.254	98	9439	0.458	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 92.000%			
10) 1,1,2,2-Tetrachloroeth...	10.146	84	3190	0.496	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery = 100.000%			
Target Compounds						
3) Vinyl chloride	1.132	62	1385	0.137	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111524\
Data File : VV038137.D
Acq On : 15 Nov 2024 15:23
Operator : SY/MD
Sample : P4803-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Nov 15 22:11:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

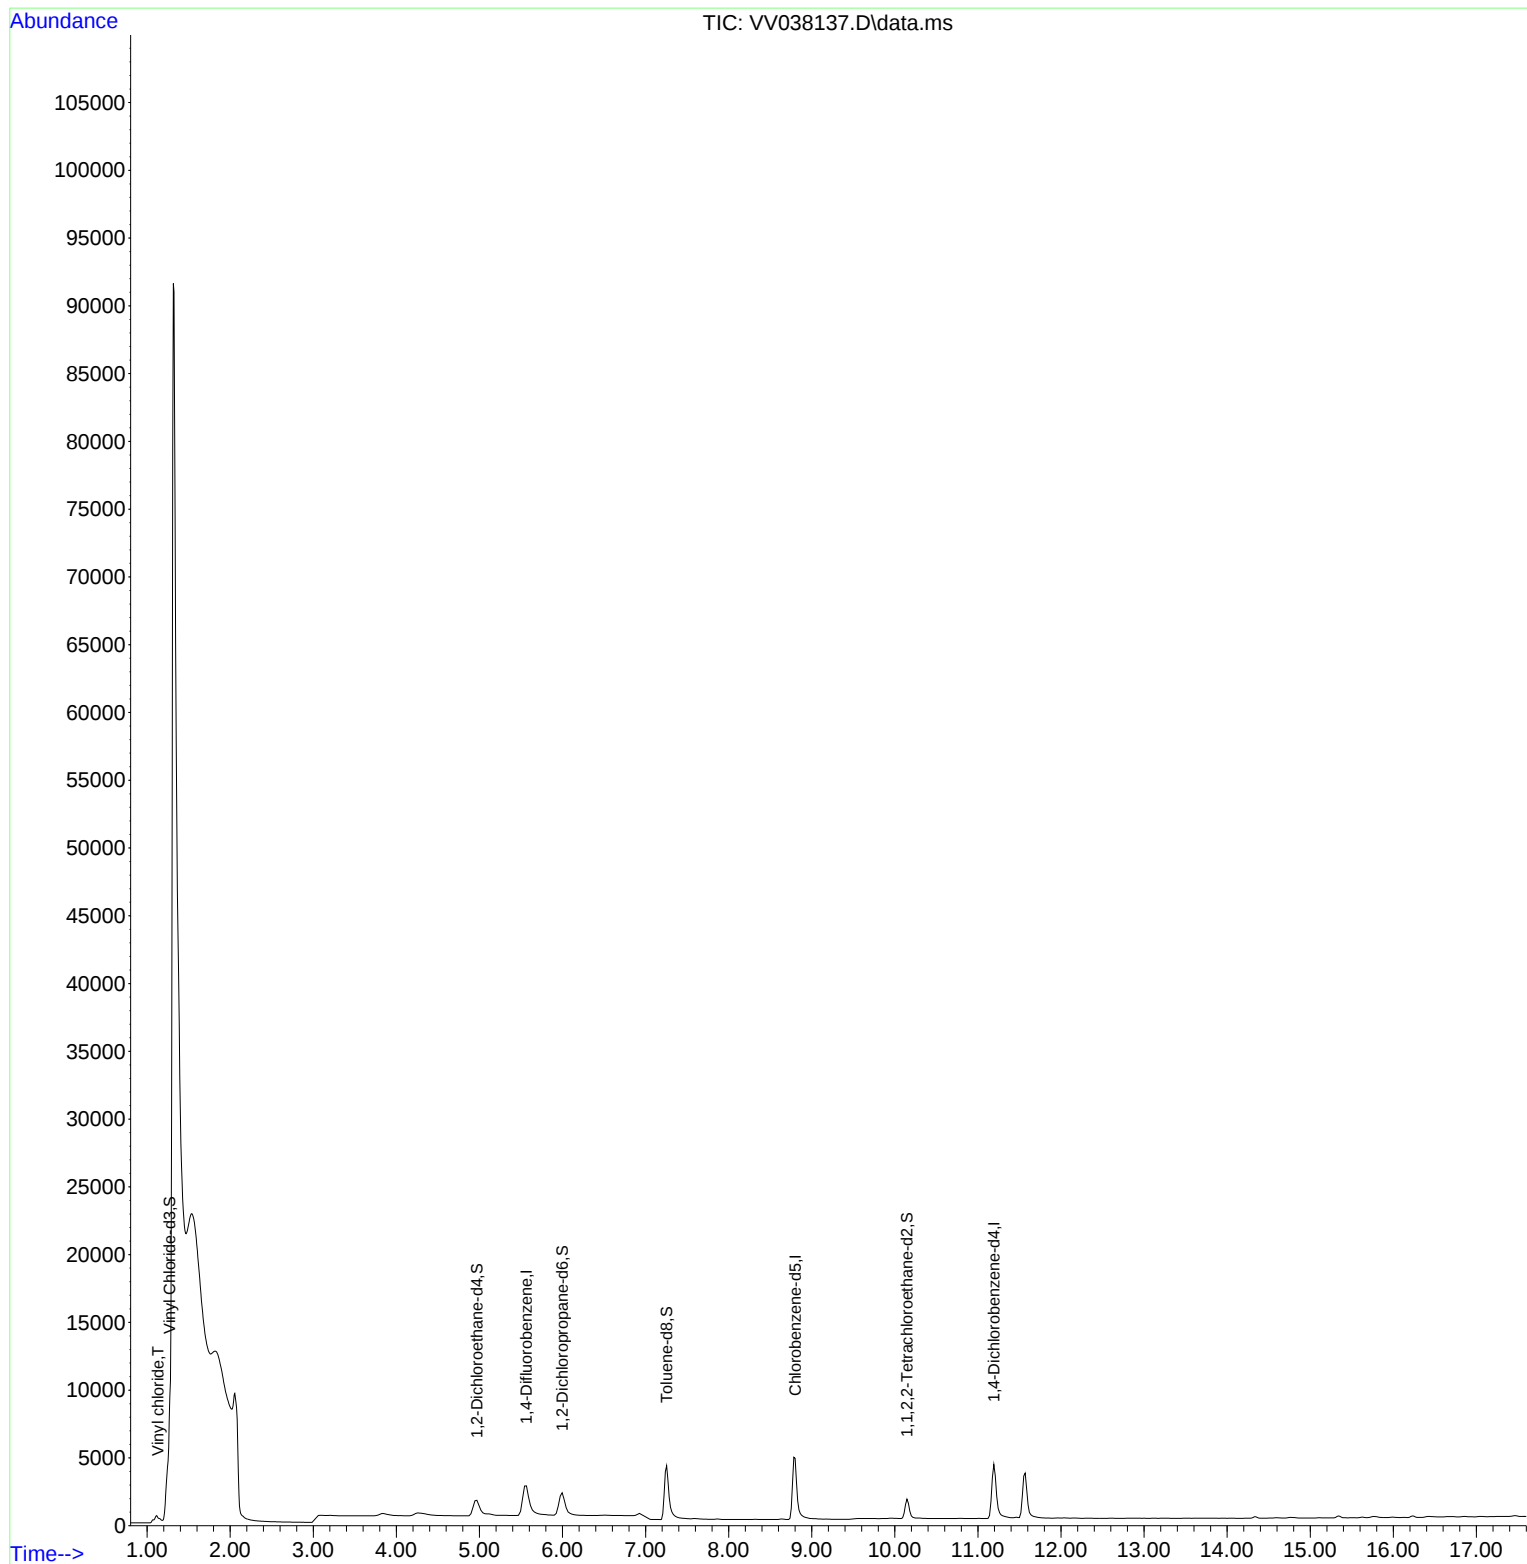

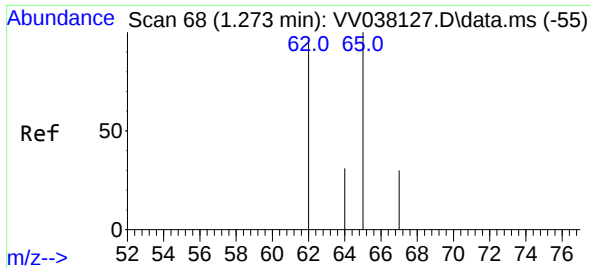

#3
Vinyl chloride
Concen: 0.137 ug/L
RT: 1.132 min Scan# 41
Delta R.T. -0.148 min
Lab File: VV038137.D
Acq: 15 Nov 2024 15:23

Instrument :
MSVOA_V
ClientSampleId :

Tgt Ion: 62 Resp: 1385
Ion Ratio Lower Upper
62 100
64 35.2 25.3 47.1

