

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111524\
 Data File : VV038139.D
 Acq On : 15 Nov 2024 16:15
 Operator : SY/MD
 Sample : P4803-05RE 2X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 15 22:11:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 00:15:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	12443	0.500	ug/L	-0.02
5) Chlorobenzene-d5	8.785	117	12503	0.500	ug/L	-0.02
11) 1,4-Dichlorobenzene-d4	11.191	152	6729	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.273	65	6387	0.495	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	= 100.000%	
4) 1,2-Dichloroethane-d4	4.969	65	4112	0.527	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	= 106.000%	
7) 1,2-Dichloropropane-d6	5.995	67	5107	0.504	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	= 100.000%	
8) Toluene-d8	7.253	98	13457	0.519	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	= 104.000%	
10) 1,1,2,2-Tetrachloroeth...	10.146	84	4238	0.523	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	= 104.000%	
Target Compounds						Qvalue
3) Vinyl chloride	1.273	62	285	0.022	ug/L #	1
13) 1,2-Dibromo-3-chloropr...	12.322	75	223	0.191	ug/L #	54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111524\
Data File : VV038139.D
Acq On : 15 Nov 2024 16:15
Operator : SY/MD
Sample : P4803-05RE 2X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Nov 15 22:11:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

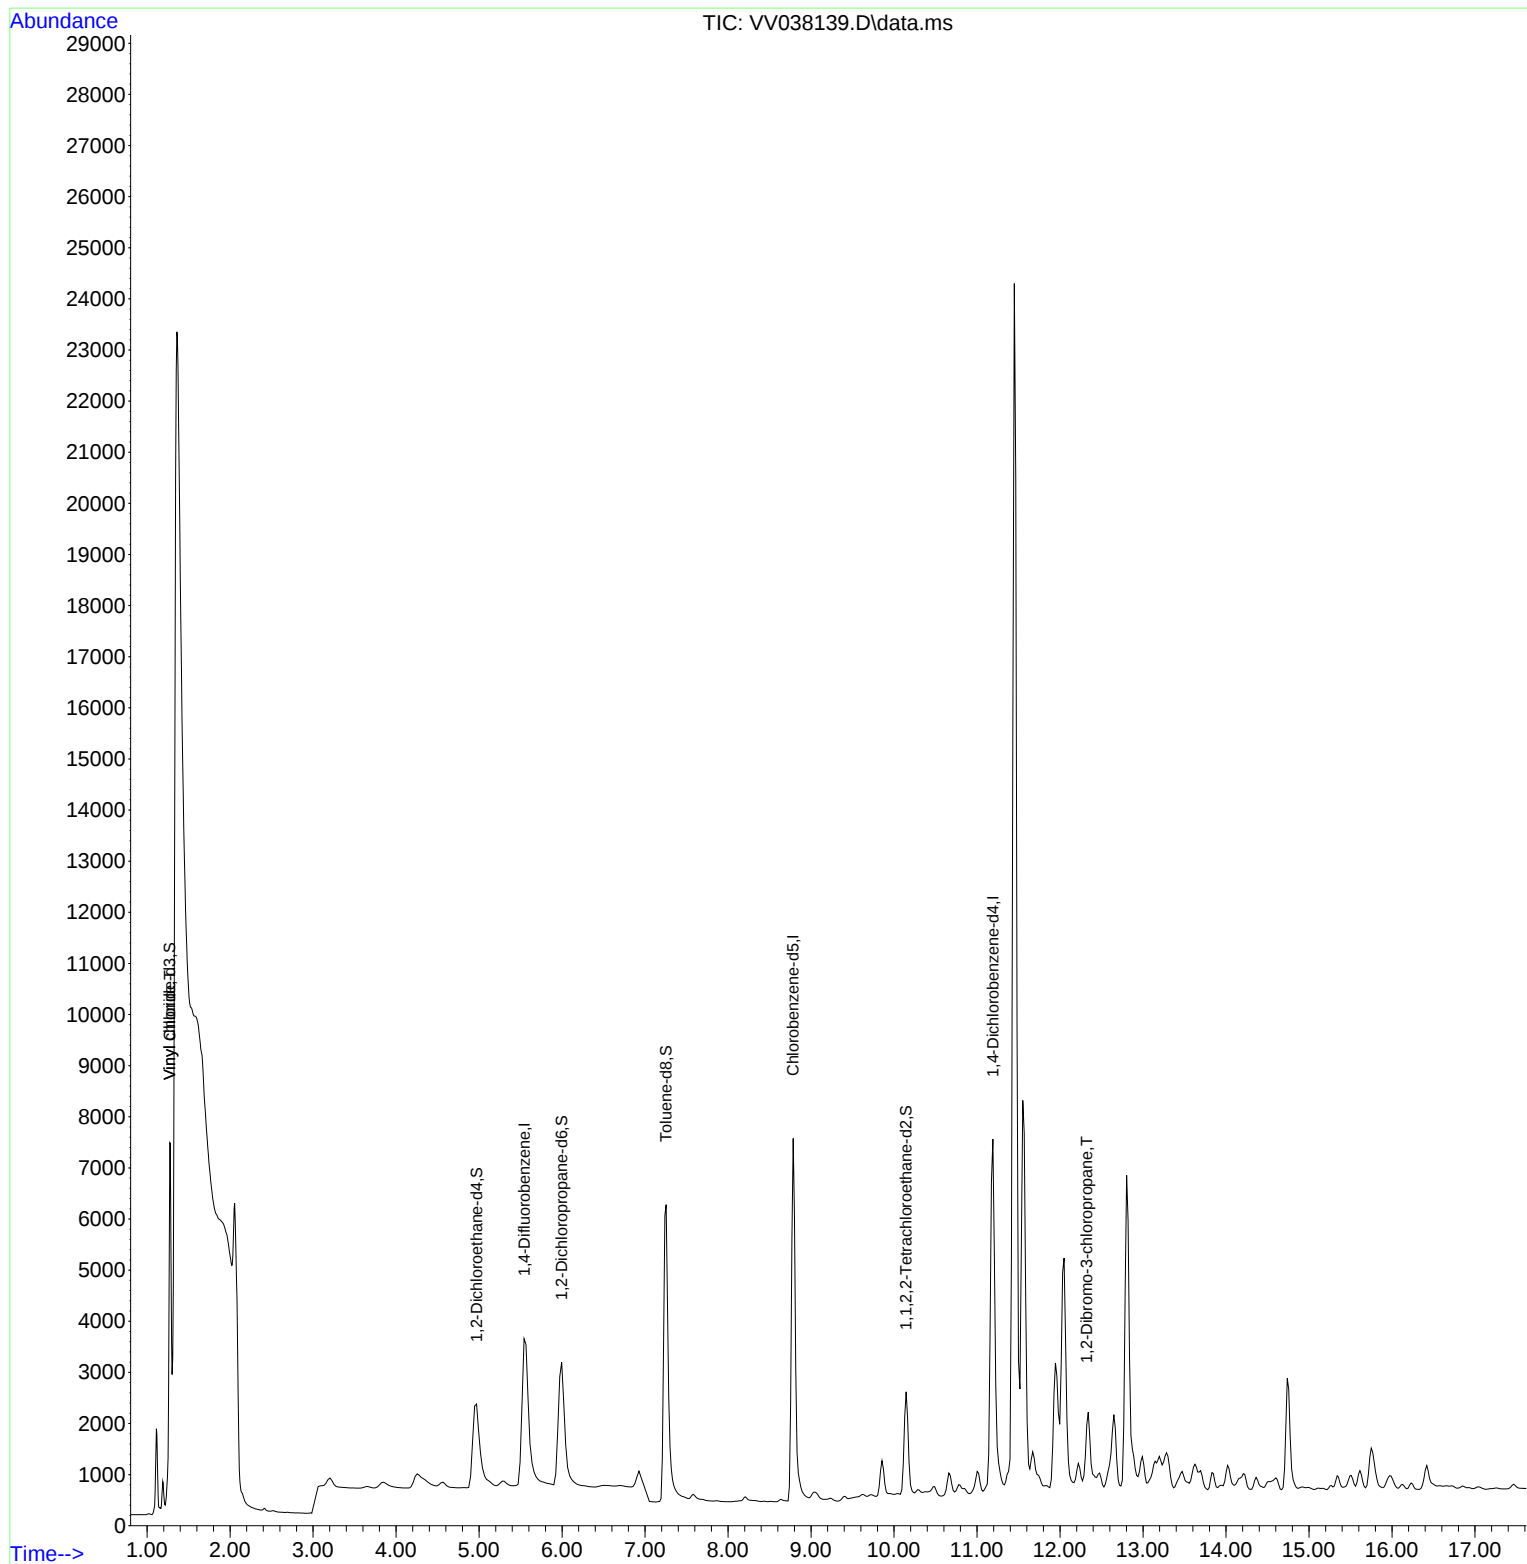



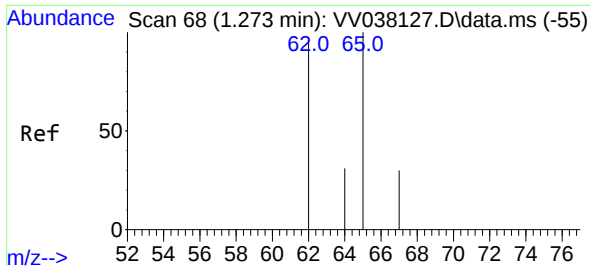


#3
 Vinyl chloride
 Concen: 0.022 ug/L
 RT: 1.273 min Scan# 61
 Delta R.T. -0.007 min
 Lab File: VV038139.D
 Acq: 15 Nov 2024 16:15

Instrument :
 MSVOA_V
 ClientSampleId :

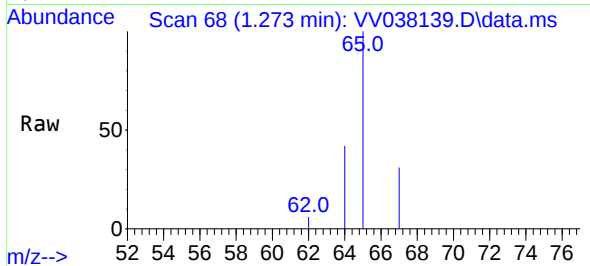

Tgt Ion: 62 Resp: 285
 Ion Ratio Lower Upper
 62 100
 64 733.1 25.3 47.1#

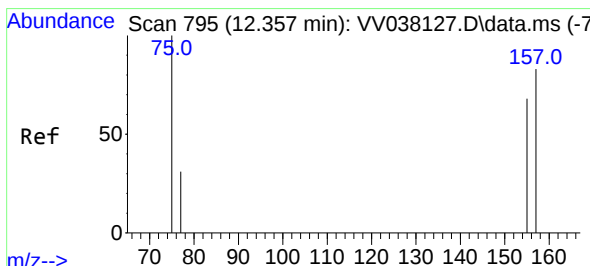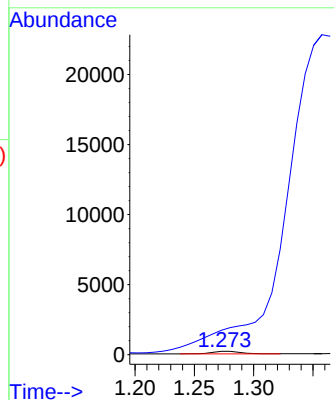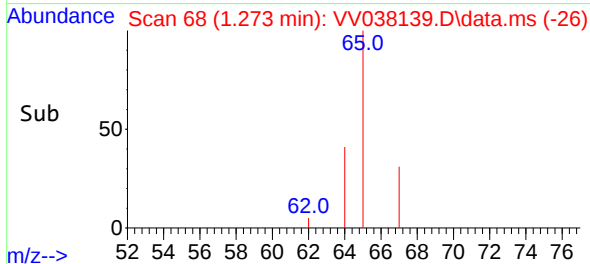

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.191 ug/L
 RT: 12.322 min Scan# 793
 Delta R.T. -0.034 min
 Lab File: VV038139.D
 Acq: 15 Nov 2024 16:15

Tgt Ion: 75 Resp: 223
 Ion Ratio Lower Upper
 75 100
 157 40.0 69.4 104.0#
 155 40.8 61.3 91.9#

