

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111524\
 Data File : VV038140.D
 Acq On : 15 Nov 2024 16:39
 Operator : SY/MD
 Sample : P4803-12RE 2X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 15 22:11:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 00:15:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	8591	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	8534	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	4219	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	6387	0.717	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	= 144.000%#	
4) 1,2-Dichloroethane-d4	4.969	65	3304	0.613	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	= 122.000%	
7) 1,2-Dichloropropane-d6	5.995	67	3957	0.572	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	= 114.000%	
8) Toluene-d8	7.253	98	10730	0.606	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	= 122.000%	
10) 1,1,2,2-Tetrachloroeth...	10.146	84	3331	0.603	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	= 120.000%	
Target Compounds						
3) Vinyl chloride	1.104	62	944	0.107	ug/L	Qvalue 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111524\
Data File : VV038140.D
Acq On : 15 Nov 2024 16:39
Operator : SY/MD
Sample : P4803-12RE 2X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Nov 15 22:11:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

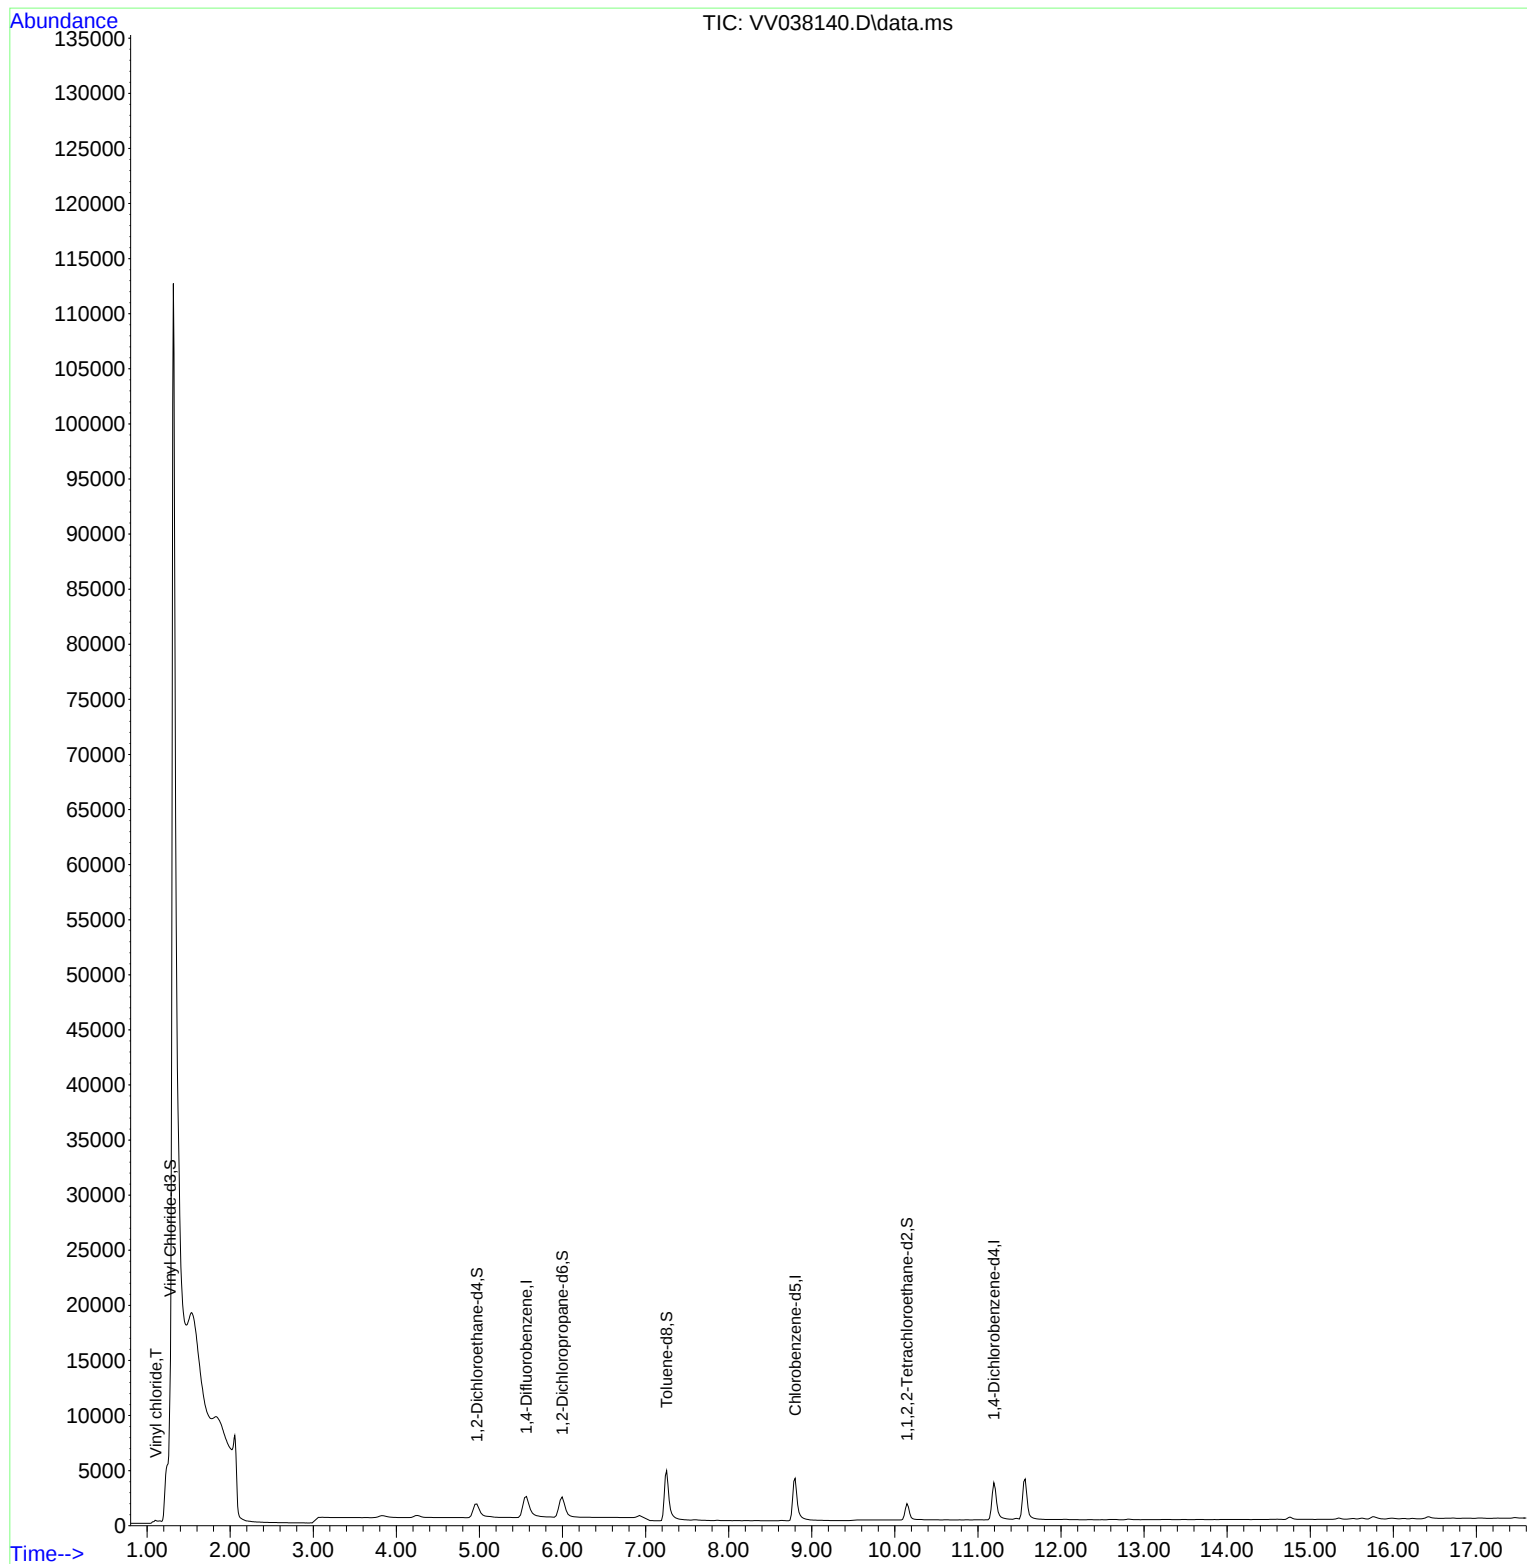

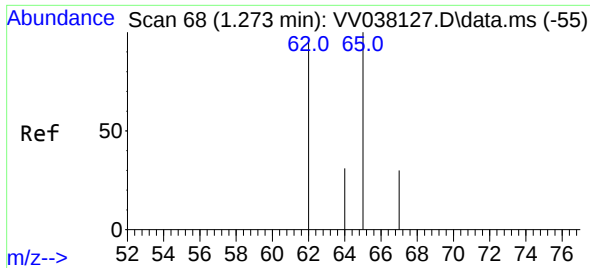

#3
Vinyl chloride
Concen: 0.107 ug/L
RT: 1.104 min Scan# 44
Delta R.T. -0.176 min
Lab File: VV038140.D
Acq: 15 Nov 2024 16:39

Instrument :
MSVOA_V
ClientSampleId :

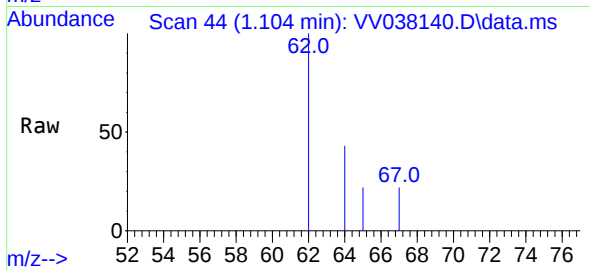

Tgt Ion: 62 Resp: 944
Ion Ratio Lower Upper
62 100
64 43.1 25.3 47.1

