

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111524\
 Data File : VV038143.D
 Acq On : 15 Nov 2024 17:52
 Operator : SY/MD
 Sample : P4803-18RE 2X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 15 22:11:53 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 00:15:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	8002	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.785	117	7922	0.500	ug/L	-0.02
11) 1,4-Dichlorobenzene-d4	11.191	152	3990	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.273	65	3698	0.446	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	90.000%		
4) 1,2-Dichloroethane-d4	4.969	65	2293	0.457	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	92.000%		
7) 1,2-Dichloropropane-d6	5.995	67	2700	0.421	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	84.000%		
8) Toluene-d8	7.253	98	6924	0.421	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	84.000%		
10) 1,1,2,2-Tetrachloroeth...	10.146	84	2187	0.426	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	86.000%		
Target Compounds						
3) Vinyl chloride	1.273	62	5574	0.676	ug/L	Qvalue # 14


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111524\
Data File : VV038143.D
Acq On : 15 Nov 2024 17:52
Operator : SY/MD
Sample : P4803-18RE 2X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Nov 15 22:11:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

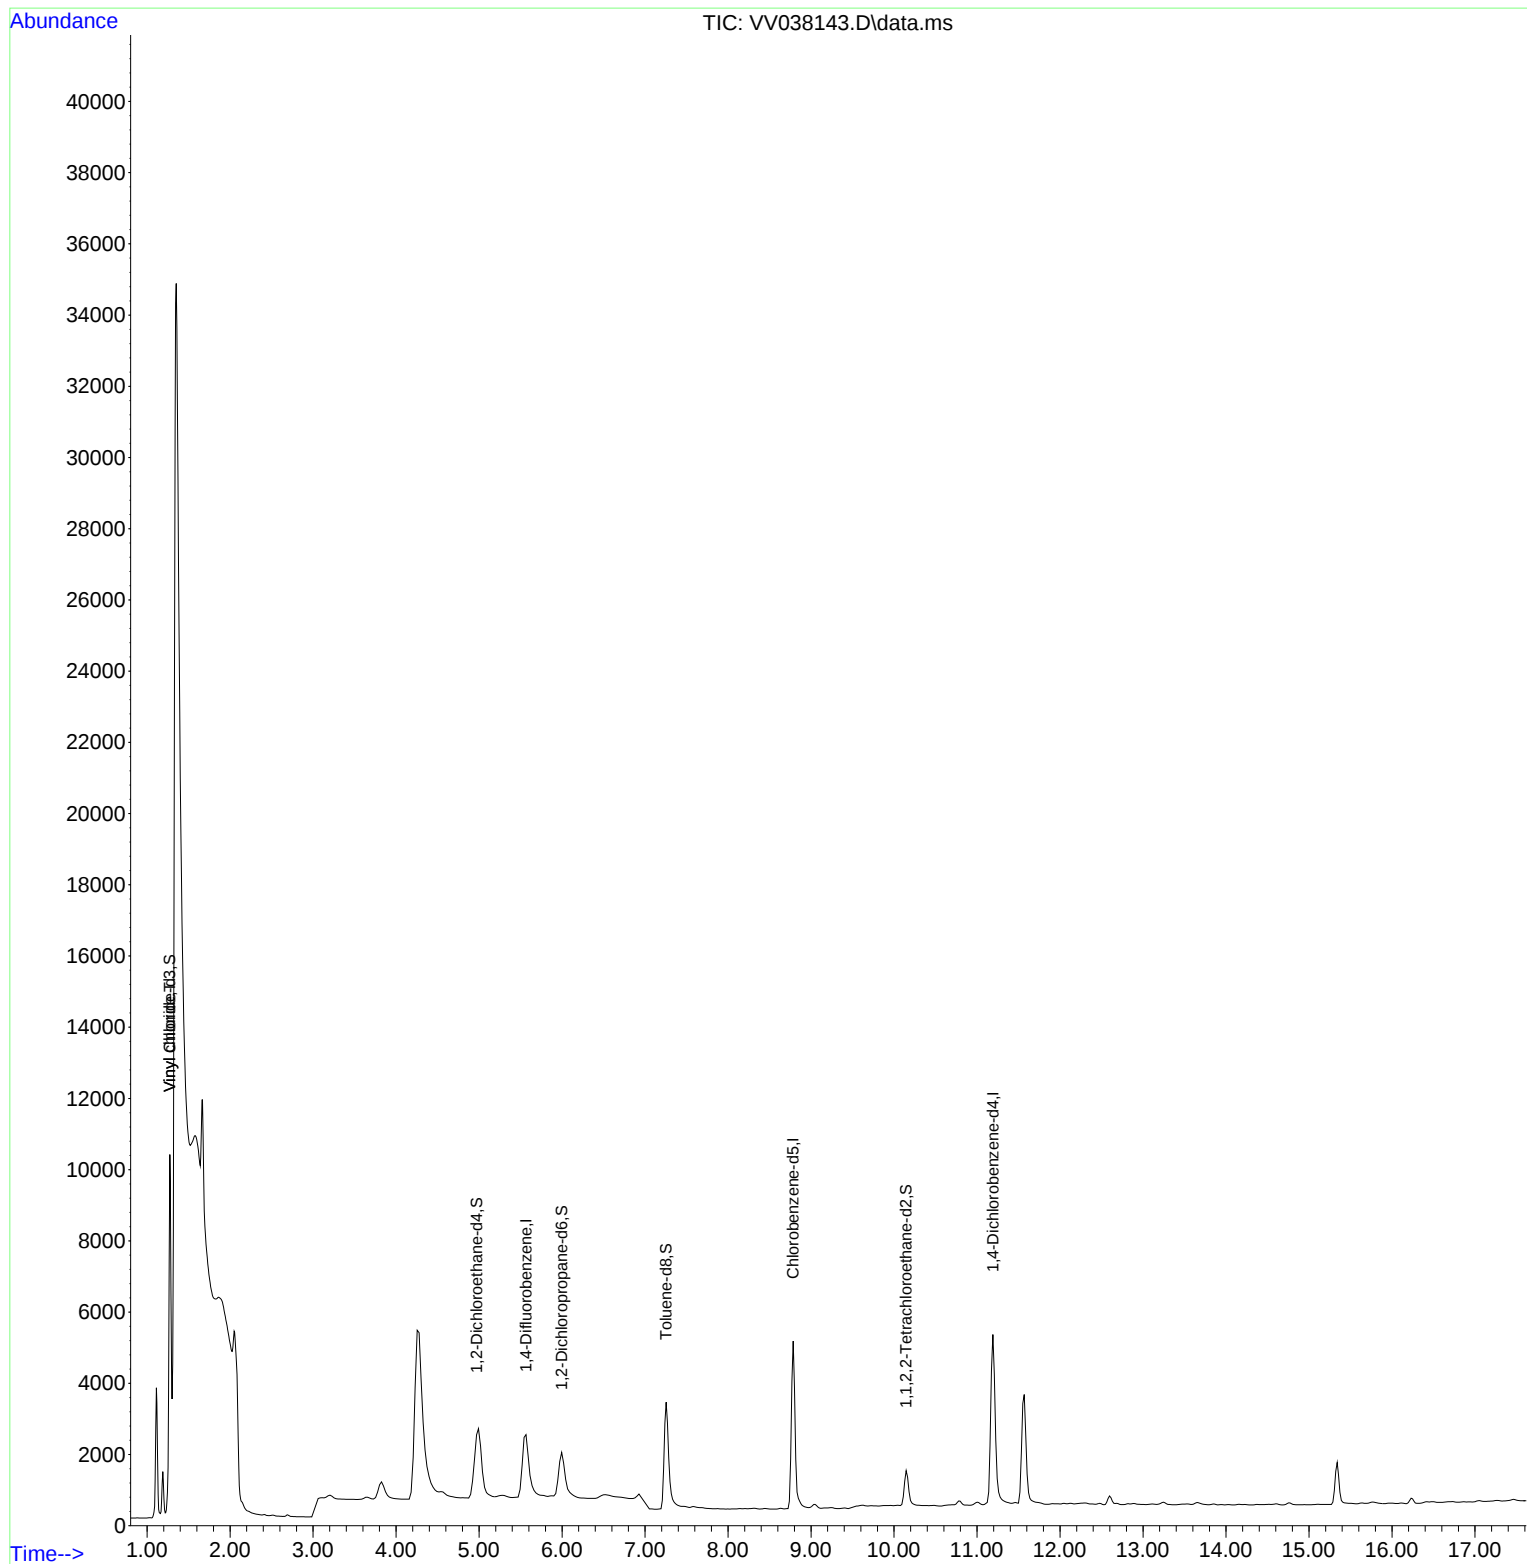

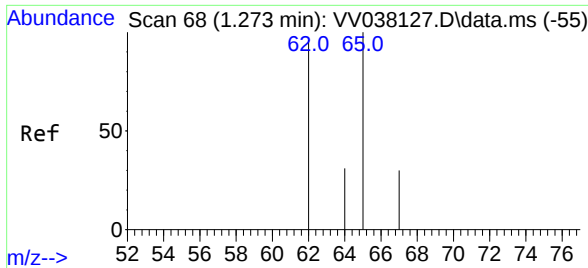

#3
Vinyl chloride
Concen: 0.676 ug/L
RT: 1.273 min Scan# 61
Delta R.T. -0.007 min
Lab File: VV038143.D
Acq: 15 Nov 2024 17:52

Instrument :
MSVOA_V
ClientSampleId :

Tgt Ion: 62 Resp: 5574
Ion Ratio Lower Upper
62 100
64 87.2 25.3 47.1#

