

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV111524\  
 Data File : VV038145.D  
 Acq On : 15 Nov 2024 18:40  
 Operator : SY/MD  
 Sample : P4803-20RE 2X  
 Misc : 25mL/MSVOA\_V/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :

Quant Time: Nov 15 22:12:01 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVSIM111424.M  
 Quant Title : TRACE VOA SOM01.0  
 QLast Update : Fri Nov 15 00:15:53 2024  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon  | Response | Conc     | Units | Dev(Min)     |
|-------------------------------|--------|-------|----------|----------|-------|--------------|
| -----                         |        |       |          |          |       |              |
| Internal Standards            |        |       |          |          |       |              |
| 1) 1,4-Difluorobenzene        | 5.542  | 114   | 11343    | 0.500    | ug/L  | -0.02        |
| 5) Chlorobenzene-d5           | 8.784  | 117   | 11459    | 0.500    | ug/L  | -0.02        |
| 11) 1,4-Dichlorobenzene-d4    | 11.191 | 152   | 6081     | 0.500    | ug/L  | 0.00         |
| System Monitoring Compounds   |        |       |          |          |       |              |
| 2) Vinyl Chloride-d3          | 1.273  | 65    | 5726     | 0.487    | ug/L  | 0.00         |
| Spiked Amount                 | 0.500  | Range | 40 - 130 | Recovery | =     | 98.000%      |
| 4) 1,2-Dichloroethane-d4      | 4.945  | 65    | 3508     | 0.493    | ug/L  | -0.02        |
| Spiked Amount                 | 0.500  | Range | 70 - 130 | Recovery | =     | 98.000%      |
| 7) 1,2-Dichloropropane-d6     | 5.995  | 67    | 4531     | 0.488    | ug/L  | 0.00         |
| Spiked Amount                 | 0.500  | Range | 60 - 140 | Recovery | =     | 98.000%      |
| 8) Toluene-d8                 | 7.253  | 98    | 11671    | 0.491    | ug/L  | 0.00         |
| Spiked Amount                 | 0.500  | Range | 70 - 130 | Recovery | =     | 98.000%      |
| 10) 1,1,2,2-Tetrachloroeth... | 10.145 | 84    | 4370     | 0.589    | ug/L  | 0.00         |
| Spiked Amount                 | 0.500  | Range | 65 - 120 | Recovery | =     | 118.000%     |
| Target Compounds              |        |       |          |          |       |              |
| 3) Vinyl chloride             | 1.097  | 62    | 517      | 0.044    | ug/L  | Qvalue<br>82 |
| -----                         |        |       |          |          |       |              |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV111524\  
Data File : VV038145.D  
Acq On : 15 Nov 2024 18:40  
Operator : SY/MD  
Sample : P4803-20RE 2X  
Misc : 25mL/MSVOA\_V/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :


Quant Time: Nov 15 22:12:01 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVSIM111424.M  
Quant Title : TRACE VOA SOM01.0  
QLast Update : Fri Nov 15 00:15:53 2024  
Response via : Initial Calibration

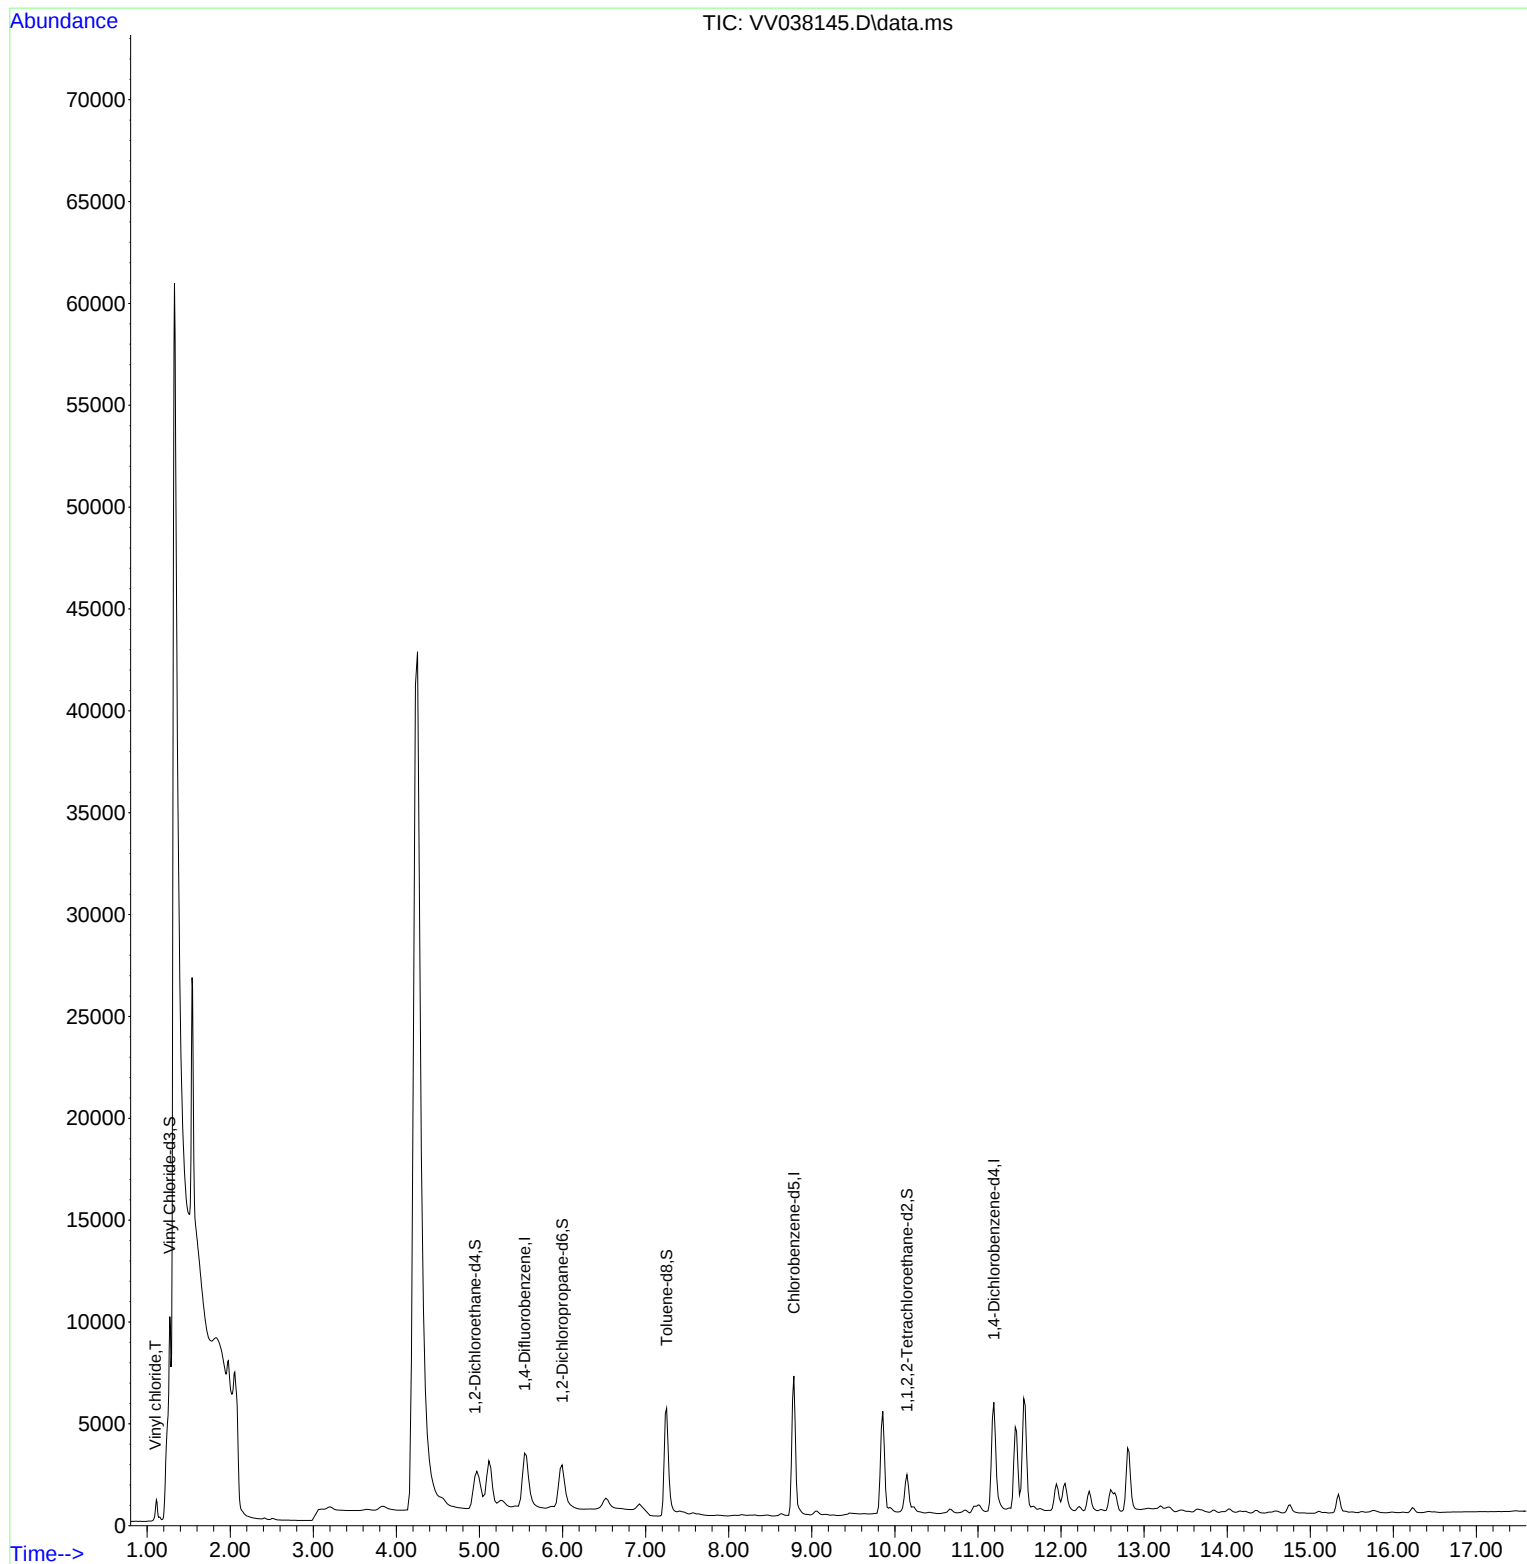

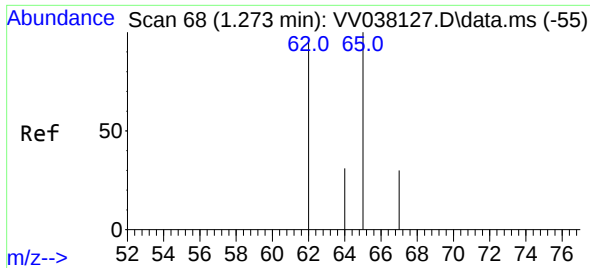

#3  
Vinyl chloride  
Concen: 0.044 ug/L  
RT: 1.097 min Scan# 41  
Delta R.T. -0.183 min  
Lab File: VV038145.D  
Acq: 15 Nov 2024 18:40

Instrument :  
MSVOA\_V  
ClientSampleId :

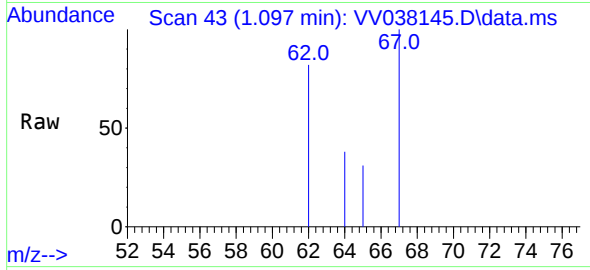

Tgt Ion: 62 Resp: 517  
Ion Ratio Lower Upper  
62 100  
64 46.8 25.3 47.1

