

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111524\
 Data File : VV038132.D
 Acq On : 15 Nov 2024 12:33
 Operator : SY/MD
 Sample : P4847-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A0AT5

Quant Time: Nov 15 22:10:59 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 00:15:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	9524	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.785	117	10201	0.500	ug/L	-0.02
11) 1,4-Dichlorobenzene-d4	11.191	152	7321	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.273	65	5342	0.541	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	108.000%
4) 1,2-Dichloroethane-d4	4.970	65	3374	0.565	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	112.000%
7) 1,2-Dichloropropane-d6	5.996	67	4555	0.551	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	110.000%
8) Toluene-d8	7.254	98	10627	0.502	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	100.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	4387	0.664	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	132.000%#
Target Compounds						
						Qvalue
3) Vinyl chloride	1.273	62	492	0.050	ug/L #	59
6) Trichloroethene	5.852	95	338	0.045	ug/L #	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111524\
Data File : VV038132.D
Acq On : 15 Nov 2024 12:33
Operator : SY/MD
Sample : P4847-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A0AT5

Quant Time: Nov 15 22:10:59 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

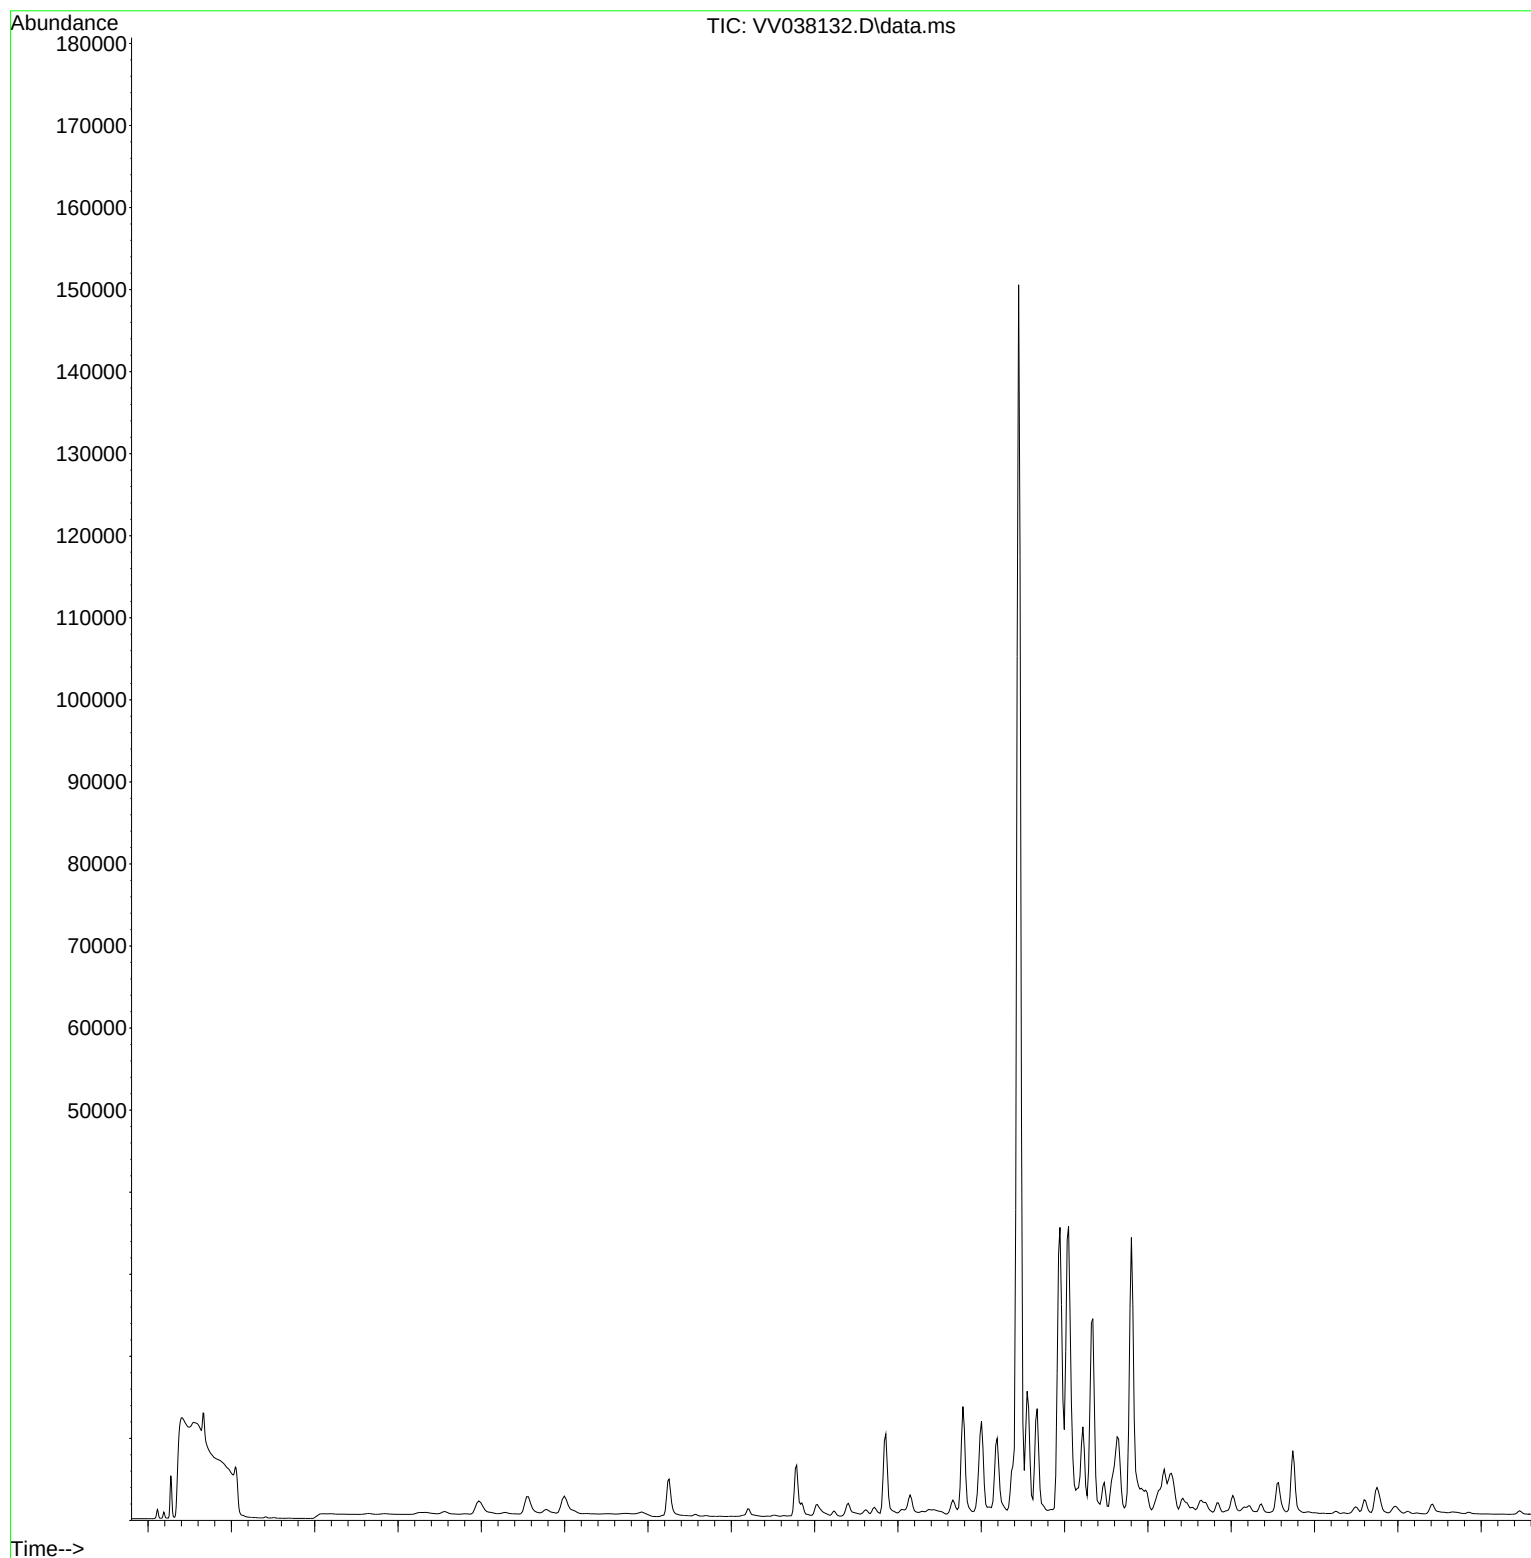

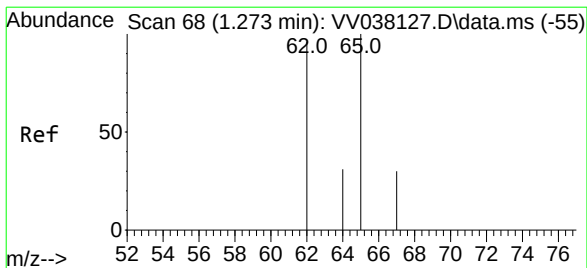

#3

Vinyl chloride

Concen: 0.050 ug/L

RT: 1.273 min Scan# 68

Delta R.T. -0.007 min

Lab File: VV038132.D

Acq: 15 Nov 2024 12:33

Instrument :

MSVOA_V

ClientSampleId :





A0AT5

Tgt Ion: 62 Resp: 492

Ion Ratio Lower Upper

62 100

64 60.6 25.3 47.1#

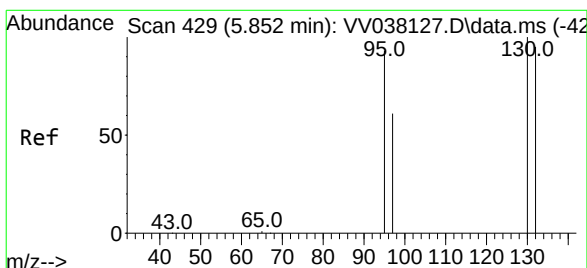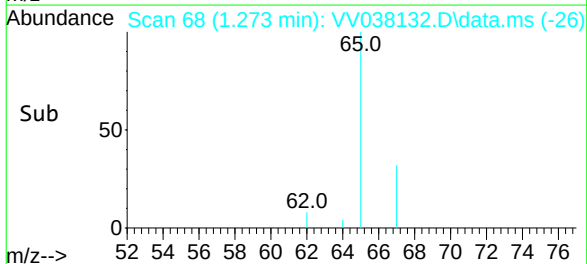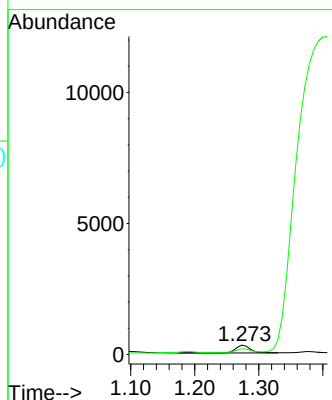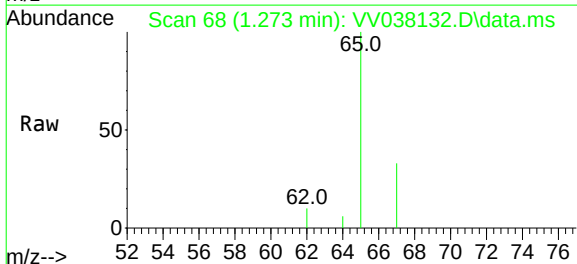

#6

Trichloroethene

Concen: 0.045 ug/L

RT: 5.852 min Scan# 429

Delta R.T. 0.000 min

Lab File: VV038132.D

Acq: 15 Nov 2024 12:33

Tgt Ion: 95 Resp: 338

Ion Ratio Lower Upper

95 100

97 102.1 46.5 86.5#

132 90.5 70.3 130.7

130 92.6 73.4 136.4

