

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111524\
 Data File : VV038134.D
 Acq On : 15 Nov 2024 14:10
 Operator : SY/MD
 Sample : P4847-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A0AT5

Quant Time: Nov 15 22:11:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 00:15:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	10717	0.500	ug/L	-0.02
5) Chlorobenzene-d5	8.785	117	11534	0.500	ug/L	-0.02
11) 1,4-Dichlorobenzene-d4	11.174	152	8175	0.500	ug/L	-0.02
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.273	65	5865	0.528	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	106.000%
4) 1,2-Dichloroethane-d4	4.946	65	3317	0.493	ug/L	-0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	98.000%
7) 1,2-Dichloropropane-d6	5.995	67	4919	0.526	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	106.000%
8) Toluene-d8	7.238	98	11763	0.492	ug/L	-0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	98.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	4177	0.559	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	112.000%
Target Compounds						
6) Trichloroethene	5.852	95	378	0.045	ug/L	Qvalue # 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111524\
Data File : VV038134.D
Acq On : 15 Nov 2024 14:10
Operator : SY/MD
Sample : P4847-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A0AT5

Quant Time: Nov 15 22:11:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

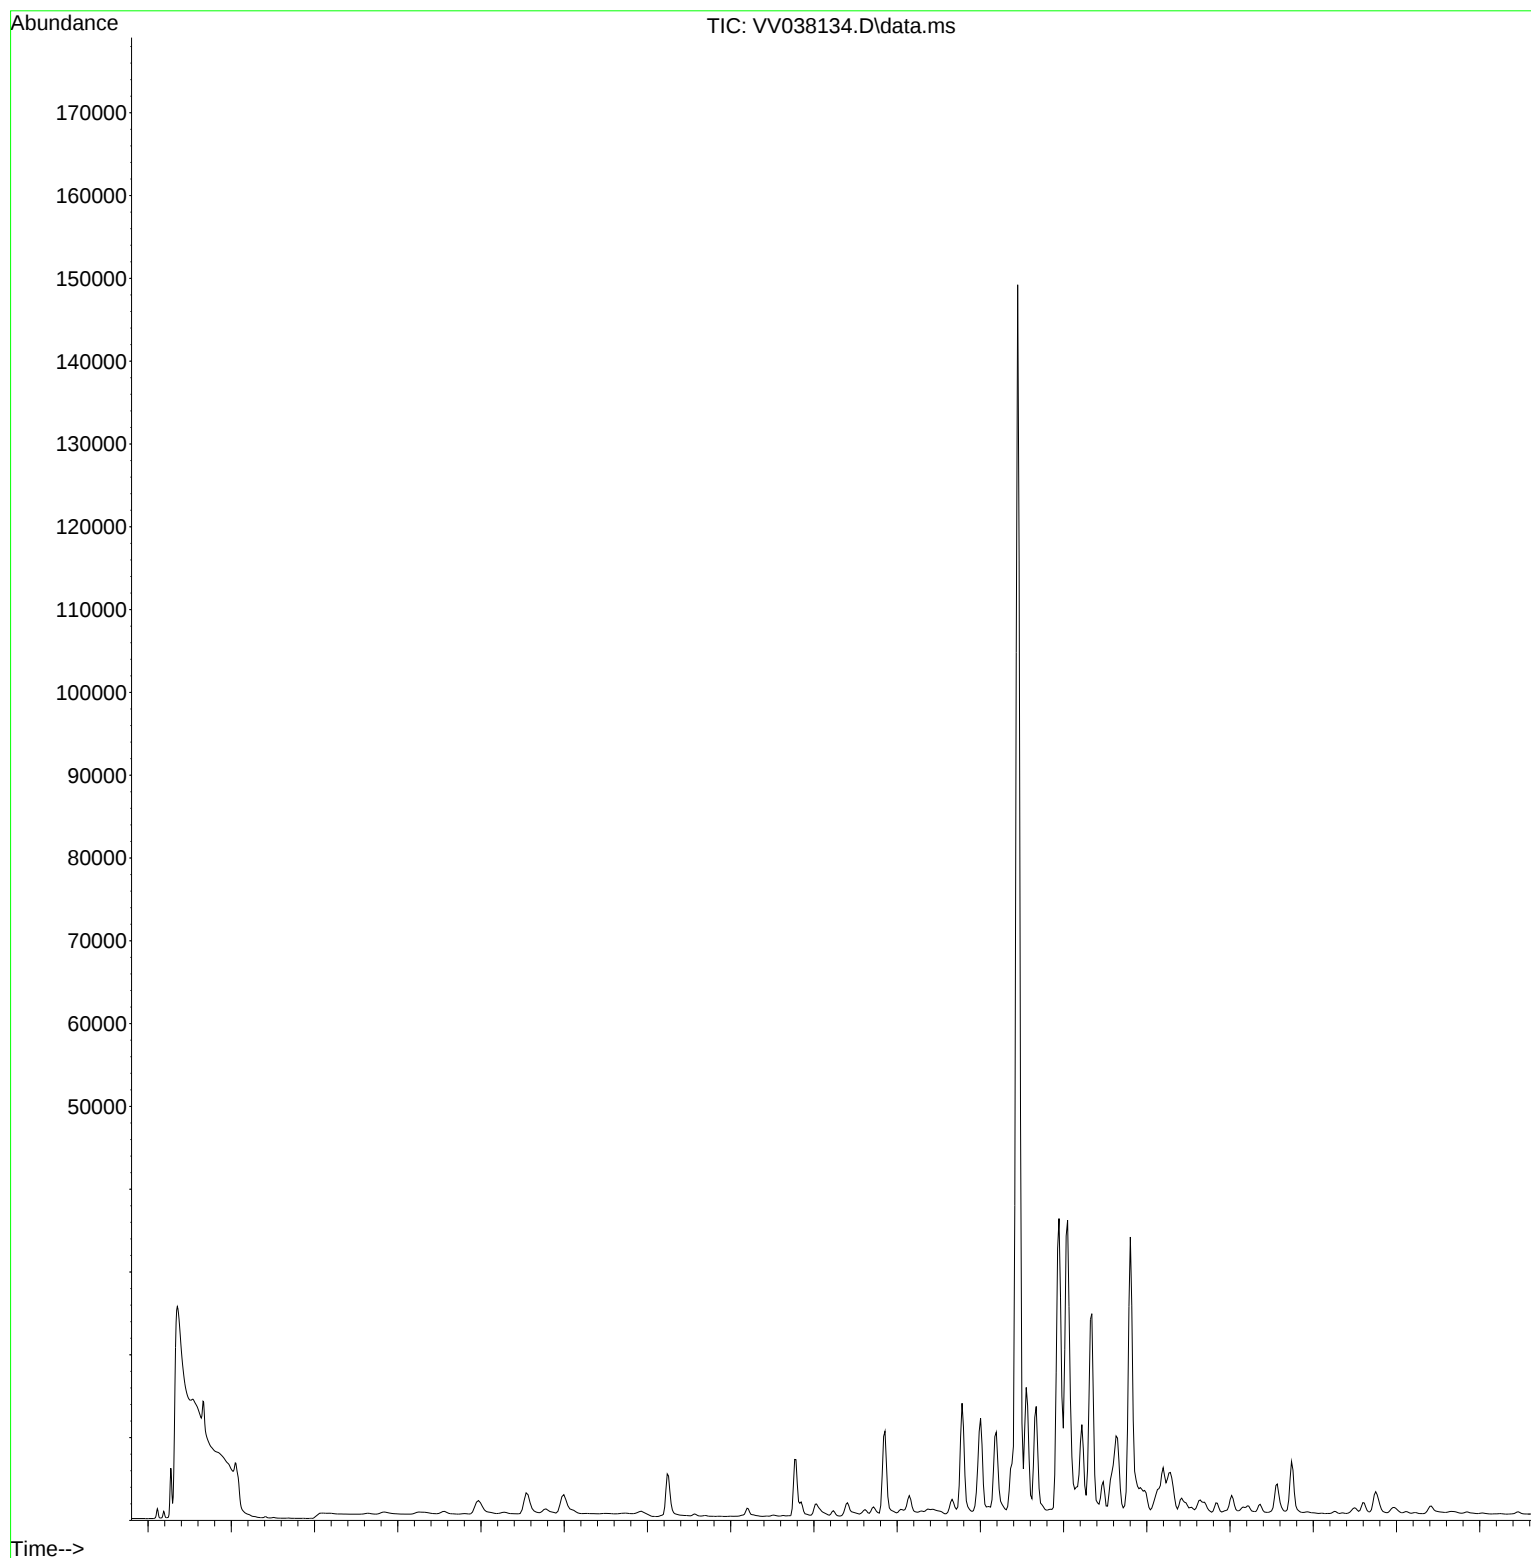

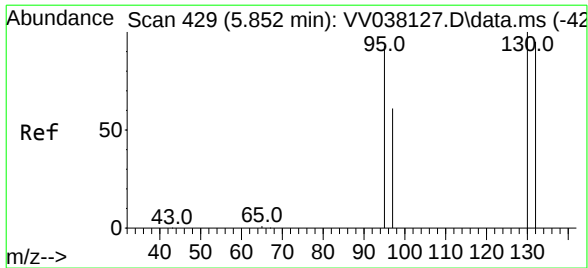

Trichloroethene

Concen: 0.045 ug/L

RT: 5.852 min Scan# 42

Delta R.T. 0.000 min

Lab File: VV038134.D


Acq: 15 Nov 2024 14:10

Instrument :

MSVOA_V

ClientSampleId :

A0AT5

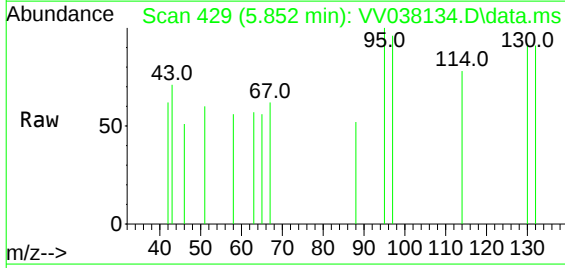

Tgt Ion: 95 Resp: 378

Ion Ratio Lower Upper

95 100

97 96.1 46.5 86.5#

132 91.3 70.3 130.7

130 92.2 73.4 136.4

