

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111623\
 Data File : VV032964.D
 Acq On : 16 Nov 2023 09:51
 Operator : SY/MD
 Sample : VV1116WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 17 00:56:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 17 00:55:52 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	446061	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	447151	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	220663	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	150510	39.895	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	79.800%	
7) Chloroethane-d5	1.532	69	133448	42.693	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	85.380%	
11) 1,1-Dichloroethene-d2	2.060	65	69051	42.009	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	84.020%	
21) 2-Butanone-d5	3.783	46	141285	87.368	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	87.370%	
24) Chloroform-d	4.249	84	283729	43.533	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	87.060%	
26) 1,2-Dichloroethane-d4	4.941	65	174813	44.081	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	88.160%	
32) Benzene-d6	4.960	84	540382	44.310	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	88.620%	
36) 1,2-Dichloropropane-d6	5.989	67	160357	45.236	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	90.480%	
41) Toluene-d8	7.243	98	488092	43.410	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	86.820%	
43) trans-1,3-Dichloroprop...	7.551	79	81873	43.505	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	87.000%	
47) 2-Hexanone-d5	8.024	63	119556	92.059	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	92.060%	
56) 1,1,2,2-Tetrachloroeth...	10.153	84	232769	44.824	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	89.640%	
66) 1,2-Dichlorobenzene-d4	11.561	152	207203	48.325	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	96.640%	
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.555	75	3846	0.785	ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111623\
Data File : VV032964.D
Acq On : 16 Nov 2023 09:51
Operator : SY/MD
Sample : VV1116WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Nov 17 00:56:37 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 17 00:55:52 2023
Response via : Initial Calibration

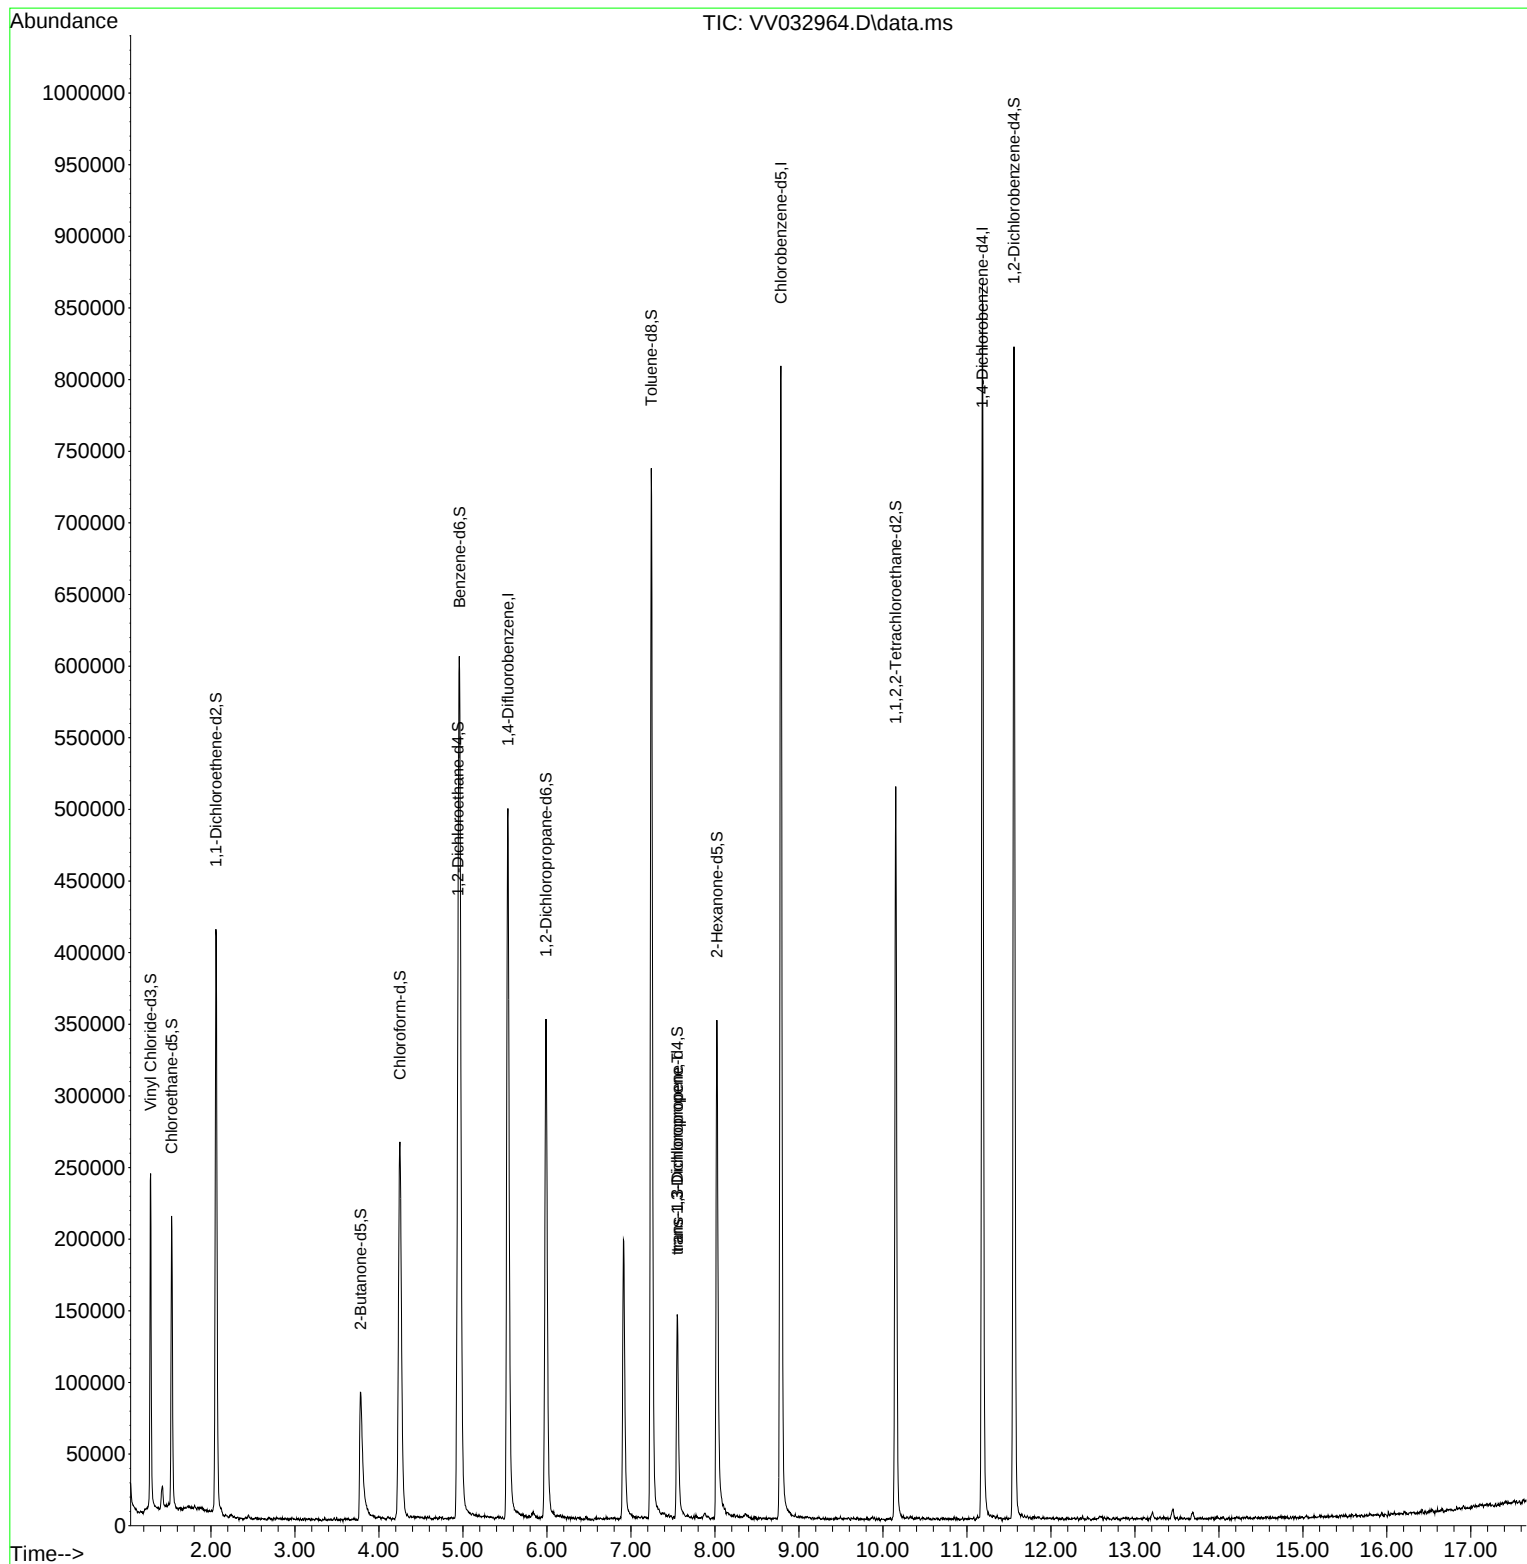

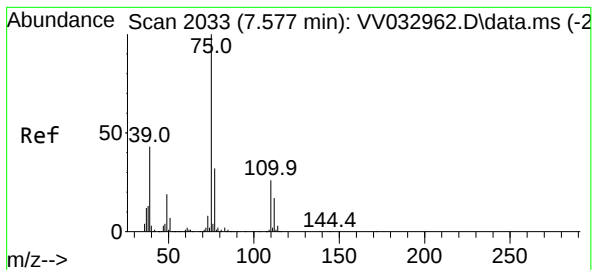

#44
 trans-1,3-Dichloropropene
 Concen: 0.785 ug/L
 RT: 7.555 min Scan# 20
 Delta R.T. -0.023 min
 Lab File: VV032964.D
 Acq: 16 Nov 2023 09:51

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 3846
 Ion Ratio Lower Upper
 75 100
 77 40.5 22.3 41.3

