

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111623\
 Data File : VV032965.D
 Acq On : 16 Nov 2023 10:38
 Operator : SY/MD
 Sample : 05416-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 17 00:56:51 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 17 00:55:52 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	431205	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	430835	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	212345	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	145771	39.970	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	79.940%		
7) Chloroethane-d5	1.532	69	126461	41.851	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	83.700%		
11) 1,1-Dichloroethene-d2	2.060	65	67755	42.641	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	85.280%		
21) 2-Butanone-d5	3.780	46	112908	72.226	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	72.230%		
24) Chloroform-d	4.246	84	265787	42.185	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	84.380%		
26) 1,2-Dichloroethane-d4	4.937	65	164166	42.822	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.640%		
32) Benzene-d6	4.957	84	509915	43.395	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.780%		
36) 1,2-Dichloropropane-d6	5.985	67	150235	43.985	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	87.980%		
41) Toluene-d8	7.243	98	446907	41.252	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	82.500%		
43) trans-1,3-Dichloroprop...	7.551	79	71601	39.488	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	78.980%		
47) 2-Hexanone-d5	8.024	63	97055	77.563	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	77.560%		
56) 1,1,2,2-Tetrachloroeth...	10.153	84	200681	40.109	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	80.220%		
66) 1,2-Dichlorobenzene-d4	11.561	152	190589	46.191	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	92.380%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.908	75	5050	1.039	ug/L	# 68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111623\
Data File : VV032965.D
Acq On : 16 Nov 2023 10:38
Operator : SY/MD
Sample : 05416-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Nov 17 00:56:51 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 17 00:55:52 2023
Response via : Initial Calibration

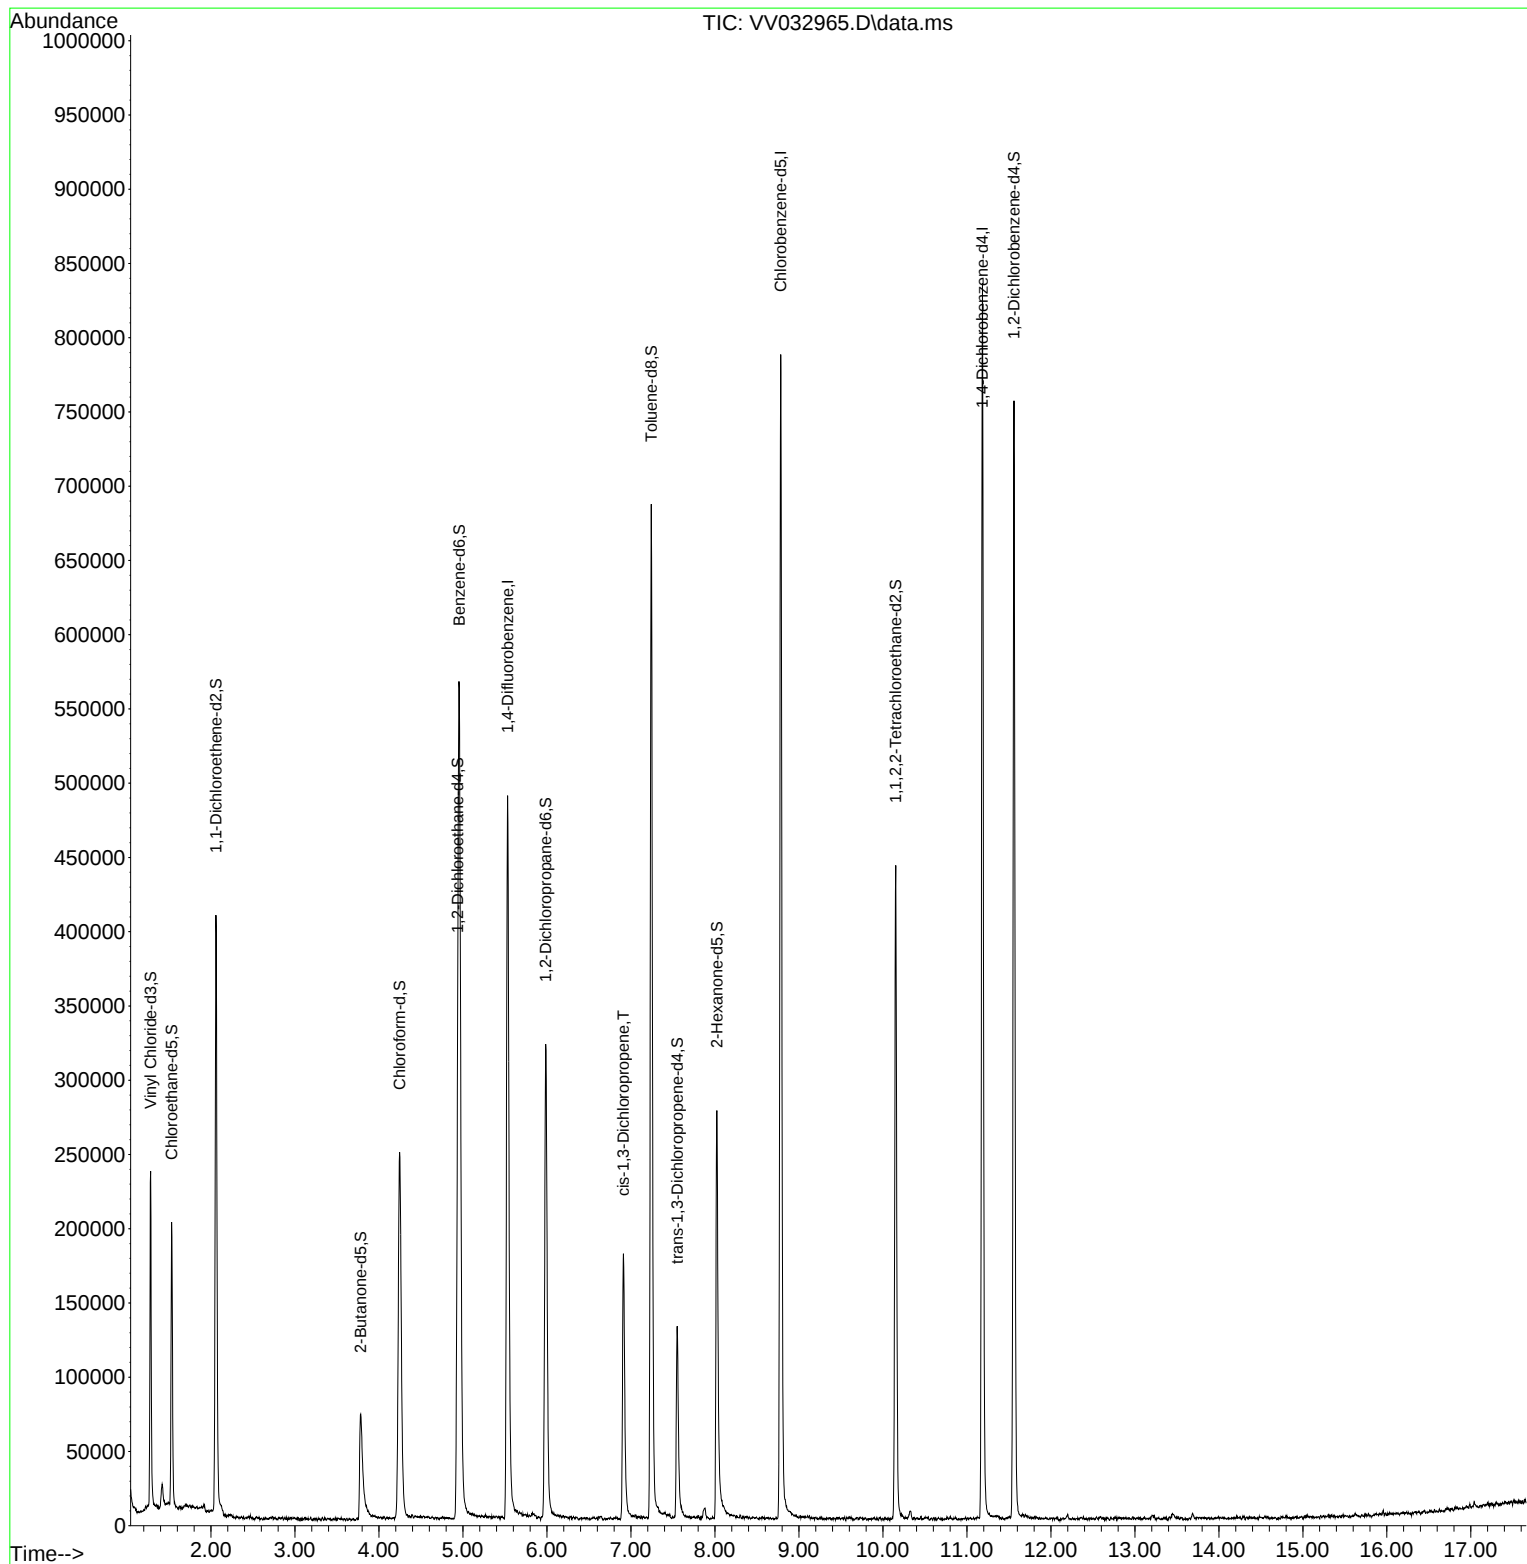

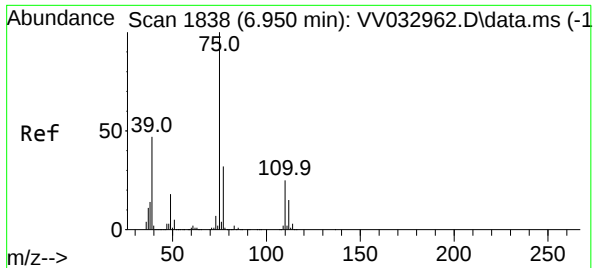

#39
 cis-1,3-Dichloropropene
 Concen: 1.039 ug/L
 RT: 6.908 min Scan# 11
 Delta R.T. -0.042 min
 Lab File: VV032965.D
 Acq: 16 Nov 2023 10:38

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 5050
 Ion Ratio Lower Upper
 75 100
 77 48.7 21.8 40.6#

