

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111623\
 Data File : VV032964.D
 Acq On : 16 Nov 2023 09:51
 Operator : SY/MD
 Sample : VV1116WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK219

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M

Title : VOC Analysis

Signal : TIC: VV032964.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	98	rVB	233327	253623	15.97%	2.010%
2	1.532	147	153	170	rVB	204323	246030	15.49%	1.950%
3	2.060	309	317	343	rVB	409157	620356	39.07%	4.917%
4	2.339	402	404	405	rBV2	1442	639	0.04%	0.005%
5	2.744	528	530	531	rBV2	1569	683	0.04%	0.005%
6	2.777	537	540	542	rBV4	1727	914	0.06%	0.007%
7	2.851	562	563	565	rVB2	1444	417	0.03%	0.003%
8	2.944	588	592	593	rBV3	1338	895	0.06%	0.007%
9	2.963	596	598	600	rBV3	1411	781	0.05%	0.006%
10	3.018	613	615	617	rVB2	1182	366	0.02%	0.003%
11	3.063	626	629	631	rBV4	1516	738	0.05%	0.006%
12	3.095	635	639	642	rBV6	1604	1082	0.07%	0.009%
13	3.117	642	646	649	rBV6	1803	1435	0.09%	0.011%
14	3.195	668	670	673	rBV4	1685	910	0.06%	0.007%
15	3.214	673	676	677	rBV2	1012	571	0.04%	0.005%
16	3.246	683	686	687	rBV3	1102	693	0.04%	0.005%
17	3.281	695	697	698	rVB2	1419	428	0.03%	0.003%
18	3.291	698	700	705	rBV7	969	722	0.05%	0.006%
19	3.330	709	712	715	rBV5	1385	988	0.06%	0.008%
20	3.355	718	720	726	rVB7	2195	1408	0.09%	0.011%
21	3.436	742	745	747	rVB3	1076	474	0.03%	0.004%
22	3.497	761	764	768	rVB5	2242	1373	0.09%	0.011%
23	3.519	768	771	774	rBV5	860	589	0.04%	0.005%
24	3.587	787	792	794	rBV5	1666	1891	0.12%	0.015%
25	3.597	794	795	797	rVB2	1518	552	0.03%	0.004%
26	3.632	803	806	808	rBV3	1325	568	0.04%	0.005%
27	3.699	825	827	828	rBV2	1165	577	0.04%	0.005%
28	3.735	836	838	842	rVB5	961	470	0.03%	0.004%
29	3.780	842	852	874	rBV	89464	233452	14.70%	1.850%
30	4.249	979	998	1023	rBV	263757	676754	42.62%	5.364%
31	4.654	1122	1124	1126	rBV3	1237	709	0.04%	0.006%
32	4.722	1142	1145	1146	rBV3	1609	814	0.05%	0.006%
33	4.831	1177	1179	1183	rBV4	1608	1115	0.07%	0.009%
34	4.957	1202	1218	1251	rBV3	600966	1588008	100.00%	12.586%
35	5.535	1384	1398	1422	rBV	496034	1024381	64.51%	8.119%
36	5.924	1517	1519	1521	rBV3	1394	808	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111623\
 Data File : VV032964.D
 Acq On : 16 Nov 2023 09:51
 Operator : SY/MD
 Sample : VV1116WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK219

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

37	5.989	1527	1539	1561	rBV	346926	707232	44.54%	5.605%
38	6.265	1623	1625	1627	rBV3	1355	764	0.05%	0.006%
39	6.468	1683	1688	1690	rBV6	2101	1834	0.12%	0.015%
40	6.529	1706	1707	1709	rBV2	910	469	0.03%	0.004%
41	6.564	1715	1718	1720	rBV4	1744	1231	0.08%	0.010%
42	6.587	1723	1725	1726	rVB2	2162	713	0.04%	0.006%
43	6.600	1726	1729	1730	rBV3	722	394	0.02%	0.003%
44	6.706	1761	1762	1765	rBV3	1537	585	0.04%	0.005%
45	6.912	1816	1826	1849	rVV	194703	359087	22.61%	2.846%
46	7.243	1918	1929	1951	rBV	732752	1274618	80.27%	10.102%
47	7.551	2016	2025	2047	rBV	142200	254928	16.05%	2.021%
48	8.024	2162	2172	2193	rBV	348296	607243	38.24%	4.813%
49	8.471	2309	2311	2314	rBV4	2400	1666	0.10%	0.013%
50	8.516	2323	2325	2327	rVV3	1422	616	0.04%	0.005%
51	8.609	2352	2354	2357	rVB4	1733	711	0.04%	0.006%
52	8.786	2398	2409	2434	rBV	802807	1310153	82.50%	10.384%
53	9.317	2572	2574	2578	rBV4	1581	964	0.06%	0.008%
54	9.368	2588	2590	2592	rBV3	1010	422	0.03%	0.003%
55	9.432	2606	2610	2611	rBV3	1690	883	0.06%	0.007%
56	9.461	2617	2619	2623	rBV5	992	698	0.04%	0.006%
57	9.622	2666	2669	2671	rBV4	1877	1091	0.07%	0.009%
58	9.651	2676	2678	2681	rVV3	1438	663	0.04%	0.005%
59	9.686	2687	2689	2691	rBV3	1398	588	0.04%	0.005%
60	9.718	2697	2699	2700	rBV3	1175	383	0.02%	0.003%
61	9.738	2704	2705	2708	rVB3	1228	517	0.03%	0.004%
62	9.805	2724	2726	2727	rBV2	1303	481	0.03%	0.004%
63	9.837	2734	2736	2738	rBV3	905	433	0.03%	0.003%
64	9.921	2759	2762	2764	rBV3	1543	791	0.05%	0.006%
65	9.947	2768	2770	2773	rVV5	1255	665	0.04%	0.005%
66	9.985	2777	2782	2784	rBV6	1493	1402	0.09%	0.011%
67	10.037	2796	2798	2799	rBV2	1295	611	0.04%	0.005%
68	10.153	2823	2834	2855	rBV	510008	793424	49.96%	6.289%
69	10.661	2989	2992	2994	rVB3	1210	515	0.03%	0.004%
70	10.686	2997	3000	3002	rBV4	1490	868	0.05%	0.007%
71	10.879	3058	3060	3064	rVB4	1777	1088	0.07%	0.009%
72	10.931	3072	3076	3078	rBV4	833	702	0.04%	0.006%
73	10.972	3086	3089	3090	rBV3	1142	653	0.04%	0.005%
74	11.107	3129	3131	3132	rBV2	1100	504	0.03%	0.004%
75	11.185	3145	3155	3176	rBV	861068	1314234	82.76%	10.416%
76	11.429	3228	3231	3234	rBV4	2047	1770	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111623\
 Data File : VV032964.D
 Acq On : 16 Nov 2023 09:51
 Operator : SY/MD
 Sample : VV1116WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK219

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

77	11.561	3261	3272	3290	rBV	817344	1270876	80.03%	10.073%
78	11.776	3336	3339	3340	rBV3	1481	908	0.06%	0.007%
79	12.027	3415	3417	3419	rVB3	1503	561	0.04%	0.004%
80	12.156	3456	3457	3462	rBV5	940	592	0.04%	0.005%
81	12.378	3522	3526	3529	rBV5	2495	1651	0.10%	0.013%
82	12.406	3533	3535	3538	rBV3	1073	538	0.03%	0.004%
83	12.513	3565	3568	3570	rBV4	1084	661	0.04%	0.005%
84	12.632	3602	3605	3606	rBV2	2174	1281	0.08%	0.010%
85	12.670	3615	3617	3620	rBV4	1558	863	0.05%	0.007%
86	12.837	3666	3669	3672	rBV6	1557	1278	0.08%	0.010%
87	12.956	3699	3706	3708	rBV6	1423	1811	0.11%	0.014%
88	13.165	3769	3771	3772	rBV2	1064	526	0.03%	0.004%
89	13.455	3851	3861	3866	rBV3	6797	11276	0.71%	0.089%
90	13.490	3870	3872	3873	rBV2	1081	466	0.03%	0.004%
91	13.545	3887	3889	3890	rBV2	1332	411	0.03%	0.003%
92	13.651	3920	3922	3923	rBV3	1230	489	0.03%	0.004%
93	13.680	3926	3931	3932	rBV5	3947	3399	0.21%	0.027%
94	13.750	3950	3953	3957	rBV5	1837	1520	0.10%	0.012%
95	13.908	4000	4002	4003	rBV2	1374	481	0.03%	0.004%
96	13.963	4017	4019	4022	rBV3	1507	1047	0.07%	0.008%
97	14.133	4070	4072	4076	rVB4	1492	1225	0.08%	0.010%
98	14.152	4076	4078	4079	rBV	2278	855	0.05%	0.007%
99	14.474	4174	4178	4179	rBV4	1193	717	0.05%	0.006%
100	14.956	4326	4328	4332	rBV5	1434	663	0.04%	0.005%




Sum of corrected areas: 12616903

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111623\
Data File : VV032964.D
Acq On : 16 Nov 2023 09:51
Operator : SY/MD
Sample : VV1116WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK219

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

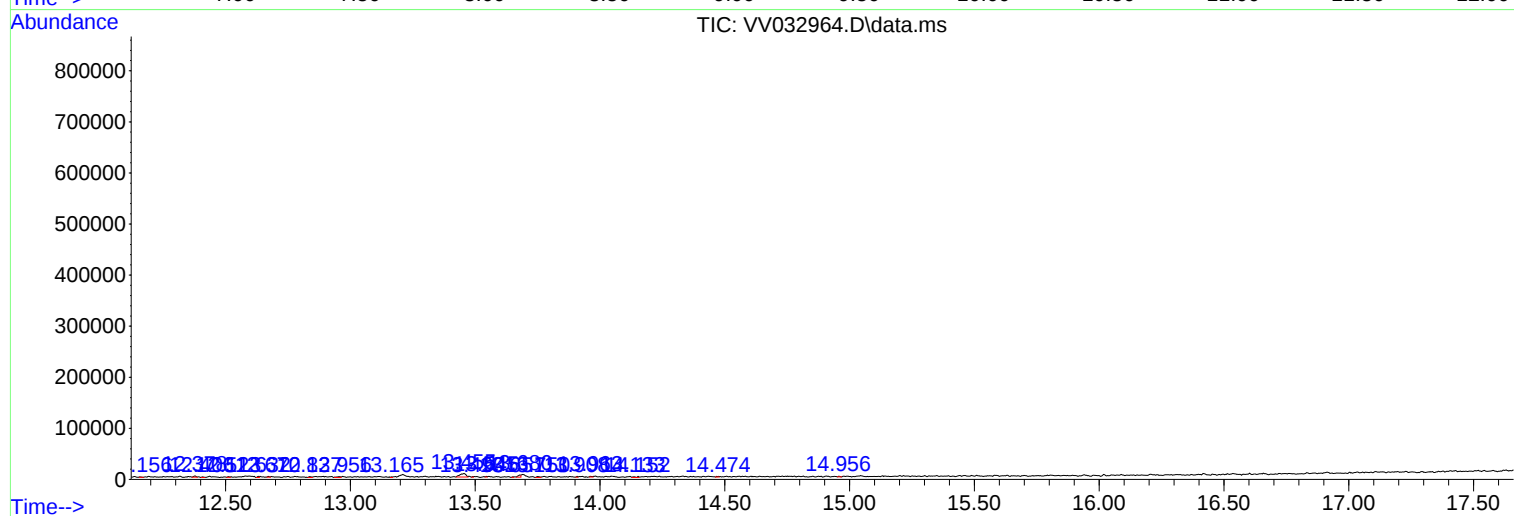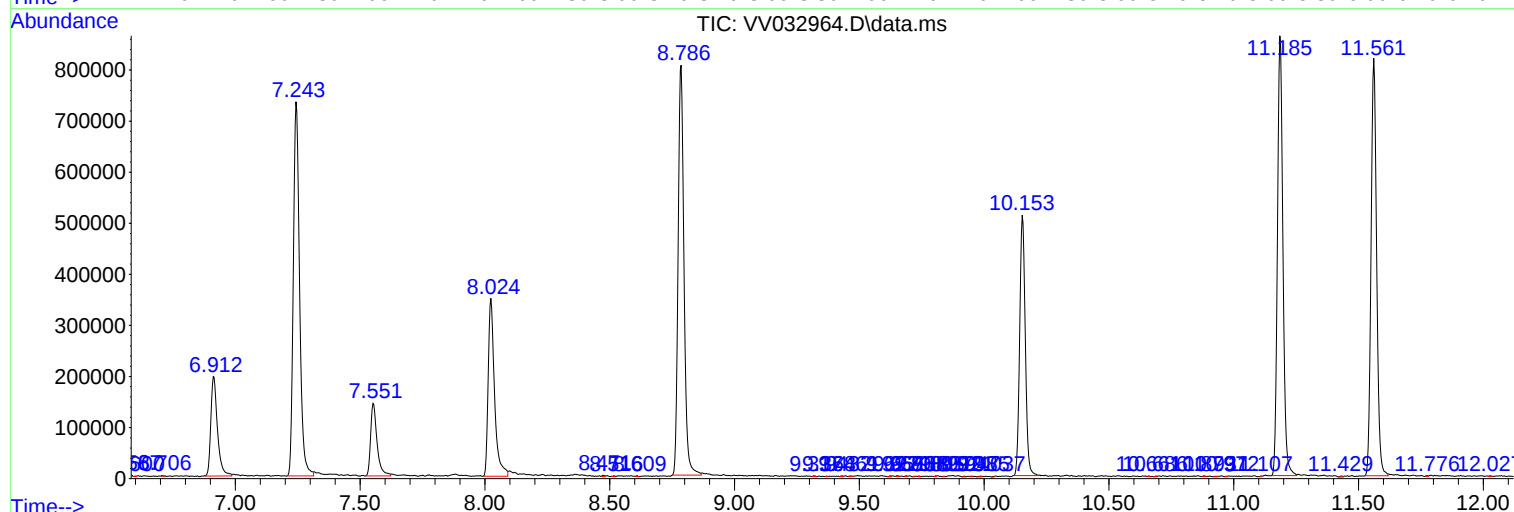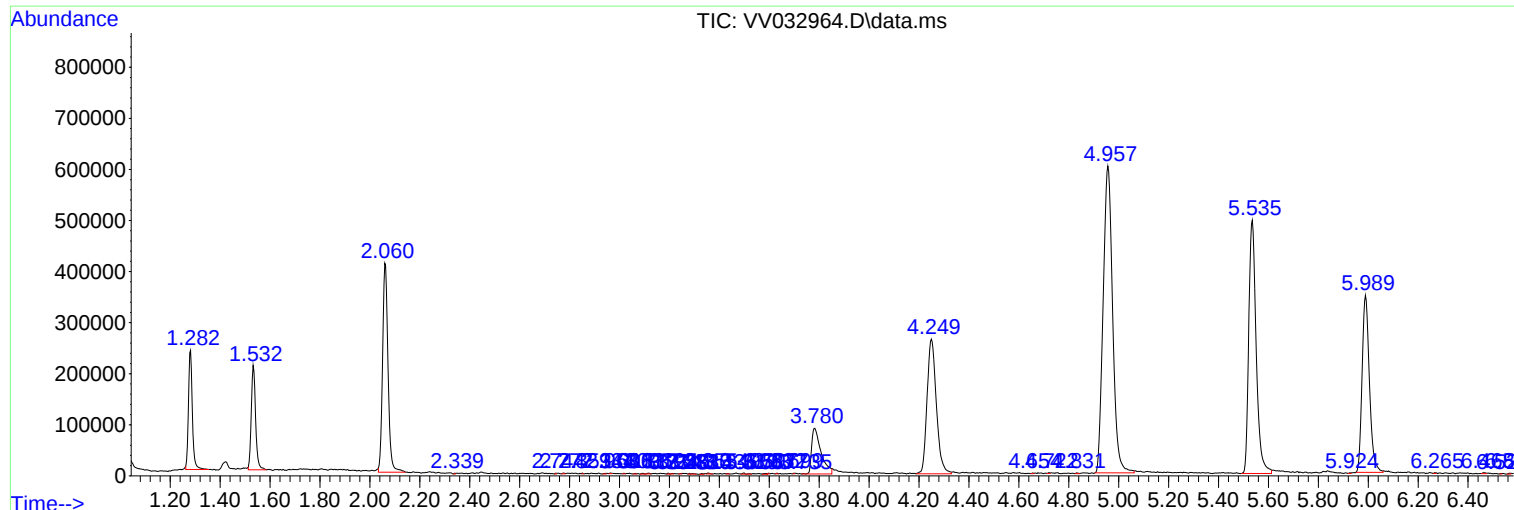

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111623\
Data File : VV032964.D
Acq On : 16 Nov 2023 09:51
Operator : SY/MD
Sample : VV1116WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK219

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111623\
Data File : VV032964.D
Acq On : 16 Nov 2023 09:51
Operator : SY/MD
Sample : VV1116WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK219

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
