

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111623\
 Data File : VV032965.D
 Acq On : 16 Nov 2023 10:38
 Operator : SY/MD
 Sample : 05416-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COALO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M

Title : VOC Analysis

Signal : TIC: VV032965.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	88	rVB	224712	238342	16.27%	2.024%
2	1.532	147	153	169	rVB	191952	228131	15.57%	1.937%
3	2.060	308	317	333	rBV	399687	582261	39.75%	4.945%
4	2.388	417	419	423	rVB5	1891	1096	0.07%	0.009%
5	2.468	442	444	446	rBV3	2067	954	0.07%	0.008%
6	2.812	547	551	553	rBV5	1405	1123	0.08%	0.010%
7	2.902	576	579	582	rVB4	2060	1262	0.09%	0.011%
8	2.925	582	586	587	rBV4	1659	911	0.06%	0.008%
9	2.941	587	591	595	rVV7	1609	1281	0.09%	0.011%
10	2.963	595	598	600	rBV4	1517	865	0.06%	0.007%
11	3.037	619	621	625	rVB5	2239	1450	0.10%	0.012%
12	3.060	625	628	630	rBV4	1456	875	0.06%	0.007%
13	3.072	630	632	635	rVB4	1878	891	0.06%	0.008%
14	3.252	685	688	692	rVB4	2067	1546	0.11%	0.013%
15	3.272	692	694	696	rBV3	1349	808	0.06%	0.007%
16	3.326	706	711	715	rBV5	2148	2087	0.14%	0.018%
17	3.352	715	719	721	rVV3	1838	1072	0.07%	0.009%
18	3.365	721	723	727	rVV5	1431	790	0.05%	0.007%
19	3.388	727	730	733	rVV5	1493	1351	0.09%	0.011%
20	3.420	737	740	744	rVB6	1555	1073	0.07%	0.009%
21	3.458	750	752	756	rBV5	1329	984	0.07%	0.008%
22	3.481	756	759	762	rVB5	1814	934	0.06%	0.008%
23	3.513	766	769	771	rBV4	1774	1385	0.09%	0.012%
24	3.616	798	801	805	rVB7	1785	1353	0.09%	0.011%
25	3.741	833	840	843	rBV7	1805	1820	0.12%	0.015%
26	3.783	843	853	873	rBV	71119	187726	12.82%	1.594%
27	4.088	945	948	950	rBV5	1373	992	0.07%	0.008%
28	4.246	984	997	1022	rVB2	244463	615090	41.99%	5.224%
29	4.953	1202	1217	1243	rBV2	561489	1464792	100.00%	12.440%
30	5.452	1369	1372	1374	rBV4	2042	1574	0.11%	0.013%
31	5.532	1385	1397	1425	rBV	487297	999111	68.21%	8.485%
32	5.934	1519	1522	1524	rBV4	2277	1737	0.12%	0.015%
33	5.985	1527	1538	1561	rVV	318417	659567	45.03%	5.601%
34	6.346	1648	1650	1653	rBV4	1141	839	0.06%	0.007%
35	6.484	1691	1693	1699	rVB7	1643	1501	0.10%	0.013%
36	6.616	1731	1734	1738	rBV5	2398	2152	0.15%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111623\
 Data File : VW032965.D
 Acq On : 16 Nov 2023 10:38
 Operator : SY/MD
 Sample : 05416-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COALO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

37	6.712	1760	1764	1766	rBV4	984	830	0.06%	0.007%
38	6.757	1774	1778	1781	rVV7	1461	1027	0.07%	0.009%
39	6.912	1814	1826	1849	rBV2	179333	340867	23.27%	2.895%
40	7.121	1889	1891	1895	rVB5	1965	1250	0.09%	0.011%
41	7.243	1918	1929	1953	rBV	682657	1187305	81.06%	10.083%
42	7.551	2016	2025	2040	rBV	128546	223498	15.26%	1.898%
43	7.831	2110	2112	2115	rBV4	2113	1164	0.08%	0.010%
44	7.883	2115	2128	2134	rVV3	7330	15381	1.05%	0.131%
45	8.024	2162	2172	2194	rBV	274925	494295	33.75%	4.198%
46	8.535	2326	2331	2335	rBV8	1344	1405	0.10%	0.012%
47	8.783	2397	2408	2434	rBV	783622	1287818	87.92%	10.937%
48	9.194	2533	2536	2538	rBV4	1853	1332	0.09%	0.011%
49	9.252	2552	2554	2557	rVB4	1803	858	0.06%	0.007%
50	9.272	2557	2560	2563	rVB5	1994	1183	0.08%	0.010%
51	9.416	2602	2605	2611	rVB7	1440	1651	0.11%	0.014%
52	9.445	2611	2614	2617	rBV5	1673	1240	0.08%	0.011%
53	9.464	2617	2620	2622	rBV3	1299	833	0.06%	0.007%
54	9.545	2641	2645	2649	rVB7	2451	2113	0.14%	0.018%
55	9.571	2649	2653	2655	rBV4	2335	1798	0.12%	0.015%
56	9.645	2674	2676	2679	rVB3	1292	871	0.06%	0.007%
57	9.667	2679	2683	2684	rBV4	1006	725	0.05%	0.006%
58	9.731	2699	2703	2705	rBV5	1430	1187	0.08%	0.010%
59	9.870	2744	2746	2749	rBV4	1440	882	0.06%	0.007%
60	9.927	2761	2764	2768	rBV6	1810	1164	0.08%	0.010%
61	9.953	2771	2772	2774	rBV2	1516	815	0.06%	0.007%
62	9.995	2780	2785	2787	rBV6	1249	1027	0.07%	0.009%
63	10.017	2790	2792	2795	rBV3	1534	897	0.06%	0.008%
64	10.091	2811	2815	2818	rBV5	1643	1229	0.08%	0.010%
65	10.153	2823	2834	2853	rBV	439899	695482	47.48%	5.906%
66	10.455	2925	2928	2930	rVB4	2424	1436	0.10%	0.012%
67	10.609	2971	2976	2979	rBV7	1952	1673	0.11%	0.014%
68	10.625	2979	2981	2984	rBV4	1451	809	0.06%	0.007%
69	10.763	3022	3024	3030	rBV6	1821	1501	0.10%	0.013%
70	10.937	3075	3078	3080	rBV4	1154	777	0.05%	0.007%
71	11.011	3096	3101	3103	rBV5	1713	1491	0.10%	0.013%
72	11.024	3103	3105	3109	rBV5	1295	1025	0.07%	0.009%
73	11.185	3144	3155	3178	rBV	831549	1280395	87.41%	10.874%
74	11.561	3260	3272	3296	rBV	751959	1170137	79.88%	9.937%
75	11.821	3350	3353	3357	rBV5	1956	1444	0.10%	0.012%
76	12.033	3415	3419	3422	rVB5	1524	1102	0.08%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111623\
 Data File : VV032965.D
 Acq On : 16 Nov 2023 10:38
 Operator : SY/MD
 Sample : 05416-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COALO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

77	12.053	3422	3425	3428	rBV4	1308	1169	0.08%	0.010%
78	12.117	3442	3445	3447	rBV4	1924	1272	0.09%	0.011%
79	12.310	3499	3505	3507	rBV7	977	1119	0.08%	0.010%
80	12.329	3509	3511	3514	rBV4	986	724	0.05%	0.006%
81	12.387	3527	3529	3532	rBV4	1771	814	0.06%	0.007%
82	12.545	3573	3578	3584	rVB8	1872	2146	0.15%	0.018%
83	12.632	3603	3605	3608	rVB4	2229	1161	0.08%	0.010%
84	12.654	3608	3612	3613	rBV3	1647	960	0.07%	0.008%
85	12.715	3626	3631	3634	rBV7	2210	1973	0.13%	0.017%
86	12.799	3653	3657	3659	rBV5	2065	1592	0.11%	0.014%
87	12.972	3708	3711	3714	rBV4	1892	1507	0.10%	0.013%
88	13.021	3723	3726	3727	rBV3	1140	722	0.05%	0.006%
89	13.204	3778	3783	3788	rBV8	2967	4209	0.29%	0.036%
90	13.262	3800	3801	3804	rBV3	1318	735	0.05%	0.006%
91	13.397	3840	3843	3844	rBV3	1361	767	0.05%	0.007%
92	13.413	3844	3848	3851	rBV6	1722	1708	0.12%	0.015%
93	13.599	3904	3906	3908	rVB2	1660	785	0.05%	0.007%
94	13.738	3946	3949	3955	rBV7	1637	1894	0.13%	0.016%
95	14.326	4128	4132	4134	rBV5	1792	1655	0.11%	0.014%
96	14.480	4178	4180	4184	rBV5	1716	1174	0.08%	0.010%
97	14.715	4250	4253	4255	rBV4	1450	1049	0.07%	0.009%
98	14.934	4319	4321	4325	rBV5	1312	726	0.05%	0.006%
99	15.021	4344	4348	4349	rBV4	1695	1191	0.08%	0.010%
100	15.213	4404	4408	4412	rBV6	2340	2441	0.17%	0.021%




Sum of corrected areas: 11775136

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111623\
Data File : VV032965.D
Acq On : 16 Nov 2023 10:38
Operator : SY/MD
Sample : 05416-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COALO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

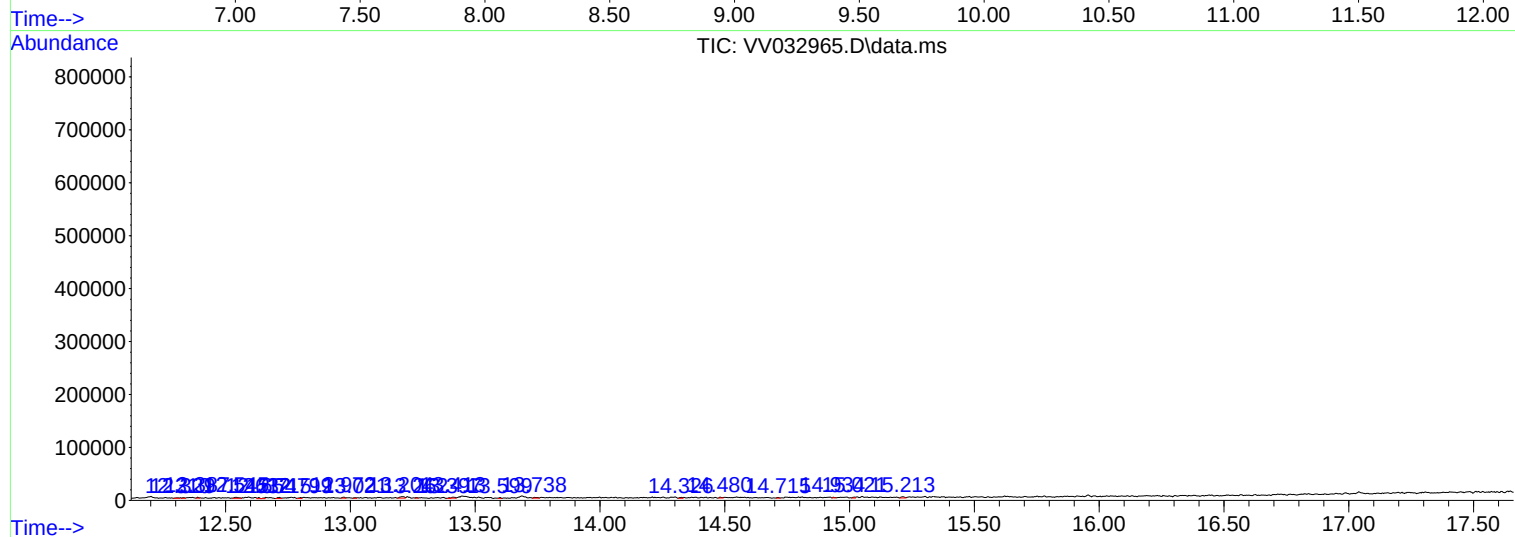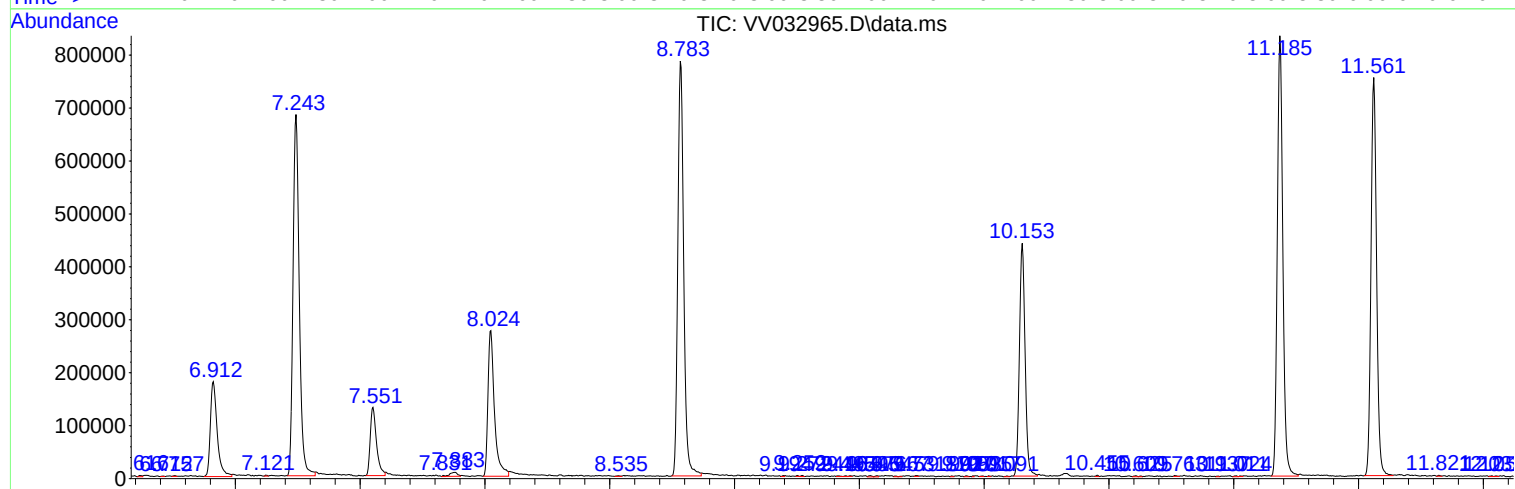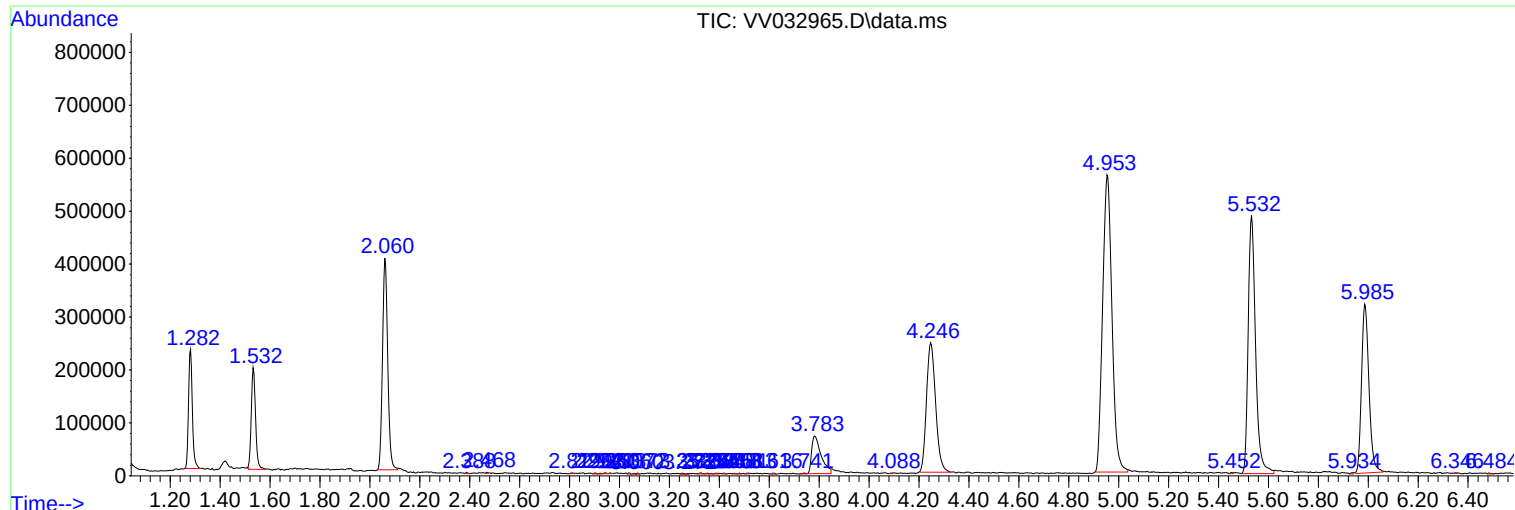

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111623\
Data File : VV032965.D
Acq On : 16 Nov 2023 10:38
Operator : SY/MD
Sample : 05416-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AL0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111623\
Data File : VV032965.D
Acq On : 16 Nov 2023 10:38
Operator : SY/MD
Sample : 05416-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AL0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc