

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111623\
 Data File : VV032966.D
 Acq On : 16 Nov 2023 11:01
 Operator : SY/MD
 Sample : 05416-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032966.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	220383	227673	15.57%	2.007%
2	1.532	146	153	167	rVB	188666	226492	15.49%	1.997%
3	2.059	309	317	330	rVB	383710	546980	37.42%	4.823%
4	2.622	490	492	493	rBV2	823	436	0.03%	0.004%
5	2.680	507	510	511	rBV2	1416	819	0.06%	0.007%
6	2.757	531	534	535	rBV2	1253	663	0.05%	0.006%
7	2.902	576	579	582	rVB5	2637	1777	0.12%	0.016%
8	2.918	582	584	585	rBV2	1730	658	0.05%	0.006%
9	2.953	593	595	596	rBV2	1340	386	0.03%	0.003%
10	3.005	609	611	614	rBV4	1336	654	0.04%	0.006%
11	3.034	617	620	622	rBV3	1481	1105	0.08%	0.010%
12	3.066	628	630	634	rBV4	1466	1027	0.07%	0.009%
13	3.137	648	652	653	rBV3	1285	683	0.05%	0.006%
14	3.169	657	662	666	rBV8	1452	1368	0.09%	0.012%
15	3.217	672	677	681	rVB6	2244	2551	0.17%	0.022%
16	3.239	681	684	685	rBV3	811	474	0.03%	0.004%
17	3.256	685	689	690	rBV4	1111	749	0.05%	0.007%
18	3.265	690	692	696	rBV6	1326	760	0.05%	0.007%
19	3.313	705	707	709	rBV3	1126	519	0.04%	0.005%
20	3.429	741	743	748	rVB6	1650	1103	0.08%	0.010%
21	3.487	757	761	764	rVV6	1281	928	0.06%	0.008%
22	3.532	771	775	780	rBV6	1356	1309	0.09%	0.012%
23	3.593	792	794	796	rVV3	1558	606	0.04%	0.005%
24	3.657	812	814	815	rBV2	954	399	0.03%	0.004%
25	3.783	845	853	877	rBV	76773	201806	13.80%	1.779%
26	4.249	984	998	1024	rBV2	238285	609392	41.69%	5.373%
27	4.645	1118	1121	1123	rBV3	940	516	0.04%	0.005%
28	4.673	1126	1130	1131	rBV4	1221	959	0.07%	0.008%
29	4.760	1155	1157	1158	rBV2	1822	821	0.06%	0.007%
30	4.850	1183	1185	1188	rBV4	1162	705	0.05%	0.006%
31	4.956	1202	1218	1247	rBV2	549753	1461879	100.00%	12.890%
32	5.207	1294	1296	1301	rBV5	2012	1407	0.10%	0.012%
33	5.535	1386	1398	1423	rBV	439179	907627	62.09%	8.003%
34	5.989	1527	1539	1564	rBV	317003	652736	44.65%	5.755%
35	6.381	1657	1661	1662	rBV4	1433	931	0.06%	0.008%
36	6.432	1673	1677	1683	rVB7	2444	2504	0.17%	0.022%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111623\
 Data File : VV032966.D
 Acq On : 16 Nov 2023 11:01
 Operator : SY/MD
 Sample : 05416-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

37	6.461	1683	1686	1687	rBV3	1030	728	0.05%	0.006%
38	6.596	1726	1728	1730	rBV3	1149	750	0.05%	0.007%
39	6.628	1736	1738	1741	rVB3	1529	560	0.04%	0.005%
40	6.648	1742	1744	1751	rVB7	2043	1983	0.14%	0.017%
41	6.680	1751	1754	1758	rBV6	2475	2192	0.15%	0.019%
42	6.815	1793	1796	1802	rBV8	1361	1547	0.11%	0.014%
43	6.841	1802	1804	1805	rBV2	1001	357	0.02%	0.003%
44	6.915	1817	1827	1845	rBV	174419	320431	21.92%	2.825%
45	7.243	1918	1929	1955	rBV	656720	1165204	79.71%	10.274%
46	7.554	2016	2026	2043	rBV	127905	230585	15.77%	2.033%
47	7.870	2119	2124	2126	rBV5	3651	3534	0.24%	0.031%
48	7.966	2147	2154	2156	rBV7	2173	2384	0.16%	0.021%
49	8.024	2163	2172	2192	rBV	305825	527933	36.11%	4.655%
50	8.387	2282	2285	2288	rBV4	1480	1004	0.07%	0.009%
51	8.519	2324	2326	2328	rBV3	1069	576	0.04%	0.005%
52	8.558	2335	2338	2341	rBV5	1732	1200	0.08%	0.011%
53	8.606	2351	2353	2355	rBV3	1590	1089	0.07%	0.010%
54	8.657	2368	2369	2371	rBV2	1155	481	0.03%	0.004%
55	8.786	2398	2409	2428	rBV	707996	1174250	80.32%	10.353%
56	9.140	2516	2519	2521	rBV4	1860	1226	0.08%	0.011%
57	9.284	2559	2564	2566	rBV5	2633	2379	0.16%	0.021%
58	9.336	2575	2580	2583	rBV8	1307	1207	0.08%	0.011%
59	9.365	2587	2589	2591	rVB3	1532	574	0.04%	0.005%
60	9.461	2617	2619	2622	rBV4	1009	624	0.04%	0.006%
61	9.529	2637	2640	2642	rBV3	1345	734	0.05%	0.006%
62	9.702	2691	2694	2697	rBV4	1462	1036	0.07%	0.009%
63	9.963	2773	2775	2780	rBV6	1689	1288	0.09%	0.011%
64	10.069	2806	2808	2809	rBV2	933	479	0.03%	0.004%
65	10.152	2823	2834	2856	rBV	447944	709448	48.53%	6.255%
66	10.320	2883	2886	2896	rVB7	2708	3921	0.27%	0.035%
67	10.390	2904	2908	2912	rBV6	1941	1757	0.12%	0.015%
68	10.410	2912	2914	2916	rBV4	1448	686	0.05%	0.006%
69	10.577	2963	2966	2968	rBV3	1707	1015	0.07%	0.009%
70	10.599	2971	2973	2976	rVV4	1098	546	0.04%	0.005%
71	10.660	2990	2992	2995	rVB4	1364	774	0.05%	0.007%
72	10.676	2995	2997	2999	rBV3	1242	723	0.05%	0.006%
73	10.831	3040	3045	3046	rBV5	1532	1328	0.09%	0.012%
74	10.995	3093	3096	3097	rBV3	1170	644	0.04%	0.006%
75	11.040	3108	3110	3113	rBV4	1212	750	0.05%	0.007%
76	11.184	3144	3155	3180	rBV	736526	1153488	78.90%	10.170%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111623\
 Data File : VV032966.D
 Acq On : 16 Nov 2023 11:01
 Operator : SY/MD
 Sample : 05416-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

77	11.400	3220	3222	3223	rBV2	1594	610	0.04%	0.005%
78	11.490	3248	3250	3252	rBV3	1456	738	0.05%	0.007%
79	11.561	3261	3272	3293	rBV	736745	1138124	77.85%	10.035%
80	12.062	3426	3428	3429	rBV2	1489	510	0.03%	0.004%
81	12.152	3454	3456	3459	rVB4	1897	859	0.06%	0.008%
82	12.265	3488	3491	3494	rBV5	1778	1101	0.08%	0.010%
83	12.307	3502	3504	3509	rVB6	1546	860	0.06%	0.008%
84	12.377	3524	3526	3528	rBV3	1233	665	0.05%	0.006%
85	12.471	3550	3555	3557	rBV7	2041	1782	0.12%	0.016%
86	12.551	3579	3580	3585	rBV4	1385	836	0.06%	0.007%
87	12.734	3635	3637	3640	rBV5	1238	541	0.04%	0.005%
88	12.844	3669	3671	3677	rVB6	1634	1340	0.09%	0.012%
89	12.879	3681	3682	3685	rBV3	1055	581	0.04%	0.005%
90	12.966	3706	3709	3710	rBV2	1180	625	0.04%	0.006%
91	13.200	3776	3782	3783	rBV4	2224	2149	0.15%	0.019%
92	13.274	3802	3805	3806	rBV3	1044	537	0.04%	0.005%
93	13.284	3806	3808	3811	rVB4	1732	731	0.05%	0.006%
94	13.390	3837	3841	3842	rBV4	1781	1204	0.08%	0.011%
95	13.506	3875	3877	3880	rVB3	987	374	0.03%	0.003%
96	13.545	3887	3889	3892	rBV4	1059	542	0.04%	0.005%
97	13.667	3923	3927	3928	rBV3	1658	1194	0.08%	0.011%
98	14.287	4118	4120	4121	rBV2	1441	655	0.04%	0.006%
99	14.467	4172	4176	4179	rBV6	1444	1351	0.09%	0.012%
100	15.438	4476	4478	4480	rBV3	1888	869	0.06%	0.008%




Sum of corrected areas: 11341595

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111623\
Data File : VV032966.D
Acq On : 16 Nov 2023 11:01
Operator : SY/MD
Sample : 05416-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COAL3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

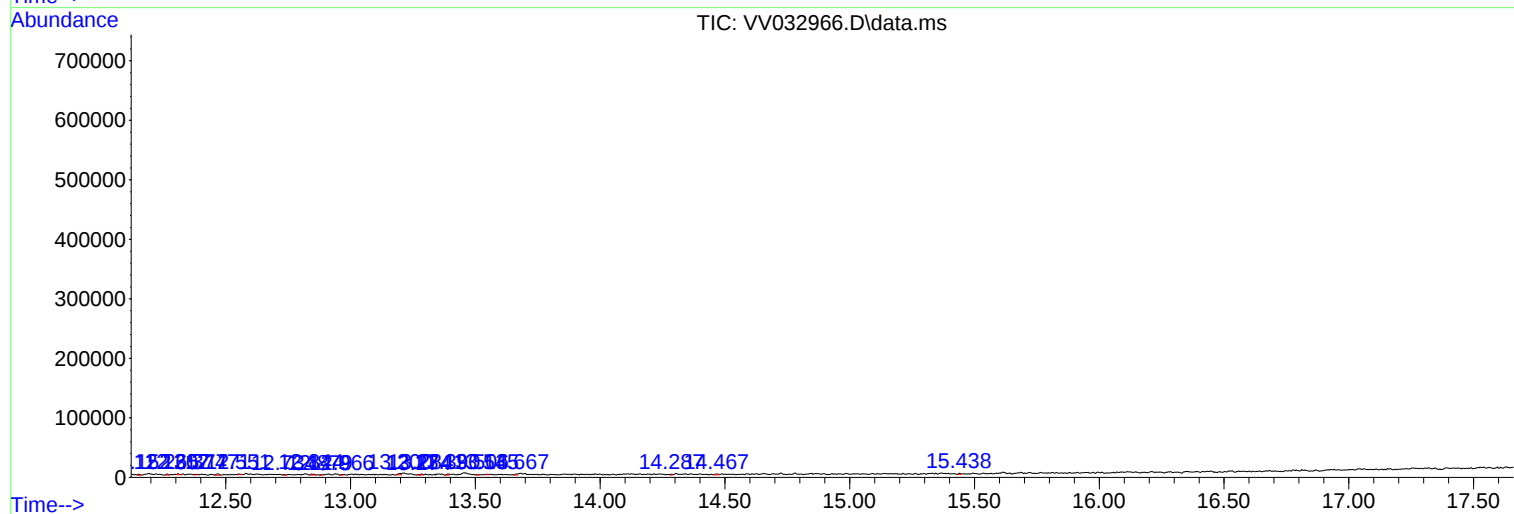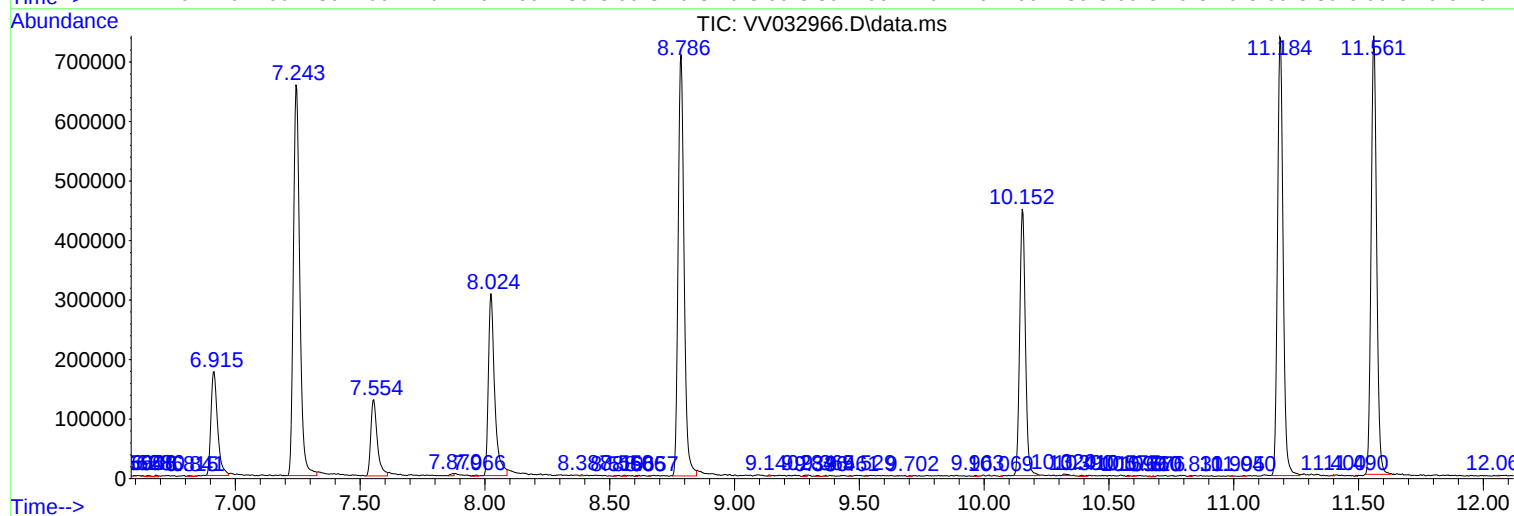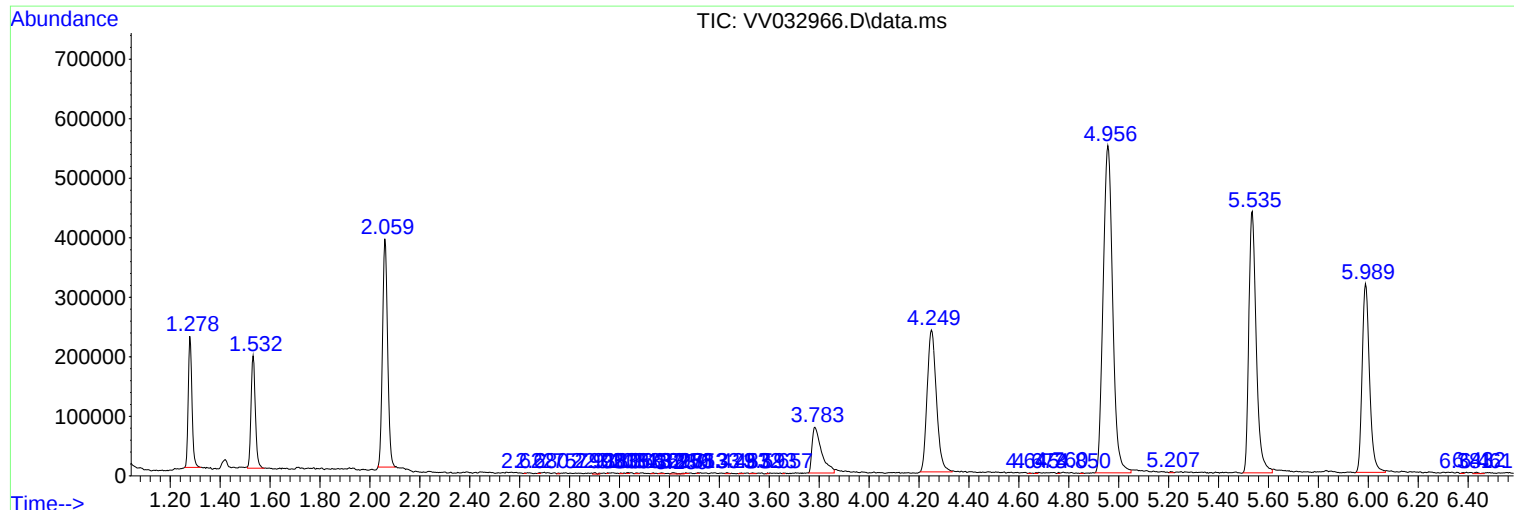

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111623\
Data File : VV032966.D
Acq On : 16 Nov 2023 11:01
Operator : SY/MD
Sample : 05416-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AL3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111623\
Data File : VV032966.D
Acq On : 16 Nov 2023 11:01
Operator : SY/MD
Sample : 05416-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AL3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc