

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111623\
 Data File : VV032967.D
 Acq On : 16 Nov 2023 12:52
 Operator : SY/MD
 Sample : 05416-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032967.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	85	rVB	229258	235324	15.56%	1.982%
2	1.532	146	153	164	rVB	194950	230519	15.24%	1.941%
3	2.060	308	317	339	rVB	400771	589480	38.98%	4.965%
4	2.410	424	426	428	rBV3	1323	656	0.04%	0.006%
5	2.481	446	448	450	rBV3	1574	908	0.06%	0.008%
6	2.867	566	568	569	rBV2	1034	482	0.03%	0.004%
7	2.944	590	592	595	rBV4	1131	712	0.05%	0.006%
8	3.031	617	619	622	rVB4	1257	542	0.04%	0.005%
9	3.182	662	666	667	rBV4	1317	957	0.06%	0.008%
10	3.207	672	674	676	rBV3	1004	573	0.04%	0.005%
11	3.294	694	701	703	rBV6	2397	2277	0.15%	0.019%
12	3.410	733	737	738	rBV4	1432	883	0.06%	0.007%
13	3.445	743	748	752	rBV8	1655	1585	0.10%	0.013%
14	3.465	752	754	755	rBV2	1237	485	0.03%	0.004%
15	3.490	760	762	763	rBV2	811	265	0.02%	0.002%
16	3.500	763	765	767	rBV2	1554	849	0.06%	0.007%
17	3.677	816	820	824	rBV7	1859	1536	0.10%	0.013%
18	3.719	831	833	836	rBV3	1480	685	0.05%	0.006%
19	3.741	836	840	843	rBV7	1444	1413	0.09%	0.012%
20	3.776	843	851	884	rVV2	77134	212518	14.05%	1.790%
21	4.146	964	966	970	rVB4	2668	1458	0.10%	0.012%
22	4.178	974	976	979	rBV4	1488	969	0.06%	0.008%
23	4.243	982	996	1020	rVV	248726	635692	42.03%	5.354%
24	4.857	1181	1187	1189	rBV7	1425	1171	0.08%	0.010%
25	4.895	1195	1199	1200	rBV4	2215	1576	0.10%	0.013%
26	4.953	1201	1217	1245	rVV2	568048	1512309	100.00%	12.737%
27	5.532	1385	1397	1423	rBV	466126	961007	63.55%	8.094%
28	5.985	1526	1538	1562	rBV	331273	680733	45.01%	5.733%
29	6.577	1718	1722	1723	rBV5	1493	1182	0.08%	0.010%
30	6.857	1808	1809	1812	rBV3	691	270	0.02%	0.002%
31	6.911	1815	1826	1848	rBV	183114	339739	22.46%	2.861%
32	7.243	1918	1929	1951	rBV	687149	1202497	79.51%	10.127%
33	7.551	2014	2025	2044	rBV	131150	234606	15.51%	1.976%
34	7.799	2099	2102	2105	rVB4	2200	1403	0.09%	0.012%
35	7.972	2153	2156	2160	rBV5	1678	1299	0.09%	0.011%
36	8.021	2162	2171	2197	rBV	301807	536552	35.48%	4.519%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111623\
 Data File : VV032967.D
 Acq On : 16 Nov 2023 12:52
 Operator : SY/MD
 Sample : 05416-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

37	8.673	2372	2374	2375	rBV2	972	326	0.02%	0.003%
38	8.712	2384	2386	2388	rBV3	2124	1001	0.07%	0.008%
39	8.783	2397	2408	2429	rBV	764748	1256835	83.11%	10.585%
40	9.731	2701	2703	2704	rBV2	1074	381	0.03%	0.003%
41	9.902	2754	2756	2757	rBV2	1246	635	0.04%	0.005%
42	9.927	2762	2764	2767	rVV3	1603	710	0.05%	0.006%
43	9.966	2773	2776	2778	rBV4	1566	841	0.06%	0.007%
44	9.982	2778	2781	2783	rBV4	1617	1075	0.07%	0.009%
45	10.050	2800	2802	2806	rVB5	1968	1076	0.07%	0.009%
46	10.069	2806	2808	2812	rVB5	2005	1577	0.10%	0.013%
47	10.095	2812	2816	2817	rBV3	907	697	0.05%	0.006%
48	10.152	2821	2834	2856	rBV	460982	743155	49.14%	6.259%
49	10.451	2925	2927	2929	rBV3	1491	529	0.03%	0.004%
50	10.506	2942	2944	2948	rBV4	1423	969	0.06%	0.008%
51	10.525	2948	2950	2952	rVB3	978	356	0.02%	0.003%
52	10.757	3017	3022	3024	rBV5	2016	1488	0.10%	0.013%
53	10.882	3060	3061	3064	rBV3	1175	456	0.03%	0.004%
54	10.956	3081	3084	3085	rBV3	1152	576	0.04%	0.005%
55	10.982	3090	3092	3096	rVB5	1702	982	0.06%	0.008%
56	11.005	3096	3099	3104	rVB7	1506	1375	0.09%	0.012%
57	11.024	3104	3105	3106	rBV	712	203	0.01%	0.002%
58	11.037	3106	3109	3110	rBV3	1312	656	0.04%	0.006%
59	11.101	3127	3129	3131	rBV3	1206	659	0.04%	0.006%
60	11.185	3144	3155	3176	rBV	796617	1234813	81.65%	10.400%
61	11.413	3224	3226	3228	rBV3	2443	1144	0.08%	0.010%
62	11.435	3230	3233	3237	rBV6	1385	1204	0.08%	0.010%
63	11.561	3261	3272	3294	rBV	774157	1191937	78.82%	10.038%
64	11.898	3374	3377	3379	rBV3	1173	727	0.05%	0.006%
65	11.940	3388	3390	3392	rBV3	1345	626	0.04%	0.005%
66	11.953	3392	3394	3397	rVB4	1470	715	0.05%	0.006%
67	12.033	3414	3419	3422	rBV6	2299	2340	0.15%	0.020%
68	12.123	3444	3447	3450	rBV5	1311	995	0.07%	0.008%
69	12.168	3458	3461	3466	rBV6	2201	2236	0.15%	0.019%
70	12.384	3525	3528	3530	rBV5	1389	734	0.05%	0.006%
71	12.426	3539	3541	3543	rBV2	1495	917	0.06%	0.008%
72	12.490	3556	3561	3563	rBV5	1377	1261	0.08%	0.011%
73	12.535	3573	3575	3583	rVB8	1820	1773	0.12%	0.015%
74	12.802	3654	3658	3660	rBV5	3097	2074	0.14%	0.017%
75	13.082	3741	3745	3747	rBV5	1248	950	0.06%	0.008%
76	13.114	3751	3755	3757	rBV4	1034	761	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111623\
 Data File : VV032967.D
 Acq On : 16 Nov 2023 12:52
 Operator : SY/MD
 Sample : 05416-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M

Title : VOC Analysis

77	13.207	3780	3784	3789	rBV8	2725	3271	0.22%	0.028%
78	13.371	3832	3835	3837	rBV4	1364	917	0.06%	0.008%
79	13.445	3853	3858	3863	rBV9	3616	4534	0.30%	0.038%
80	13.644	3918	3920	3923	rBV4	1717	1026	0.07%	0.009%
81	13.840	3979	3981	3982	rBV2	1317	403	0.03%	0.003%
82	14.110	4062	4065	4066	rBV3	1380	852	0.06%	0.007%
83	14.201	4089	4093	4095	rBV4	1472	1294	0.09%	0.011%
84	14.217	4096	4098	4100	rVB3	1663	646	0.04%	0.005%
85	14.673	4235	4240	4243	rBV7	2159	1775	0.12%	0.015%
86	14.860	4295	4298	4300	rBV4	1429	802	0.05%	0.007%
87	14.934	4319	4321	4322	rBV3	1150	486	0.03%	0.004%
88	14.946	4322	4325	4326	rBV3	1541	806	0.05%	0.007%




Sum of corrected areas: 11873689

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111623\
Data File : VV032967.D
Acq On : 16 Nov 2023 12:52
Operator : SY/MD
Sample : 05416-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

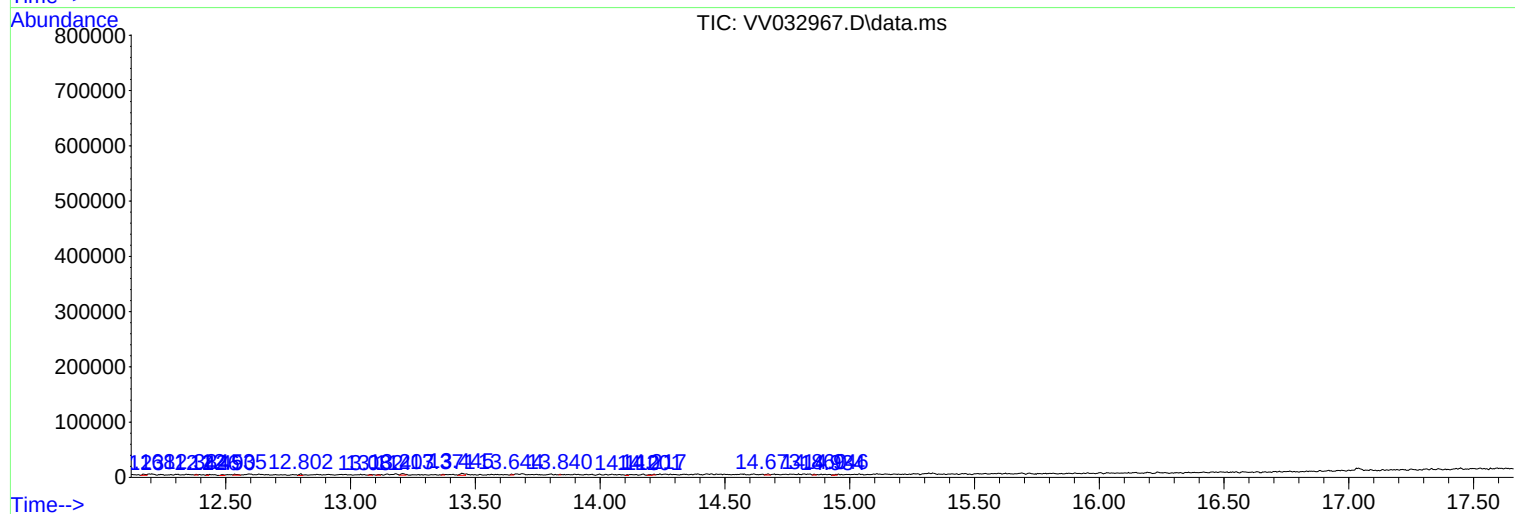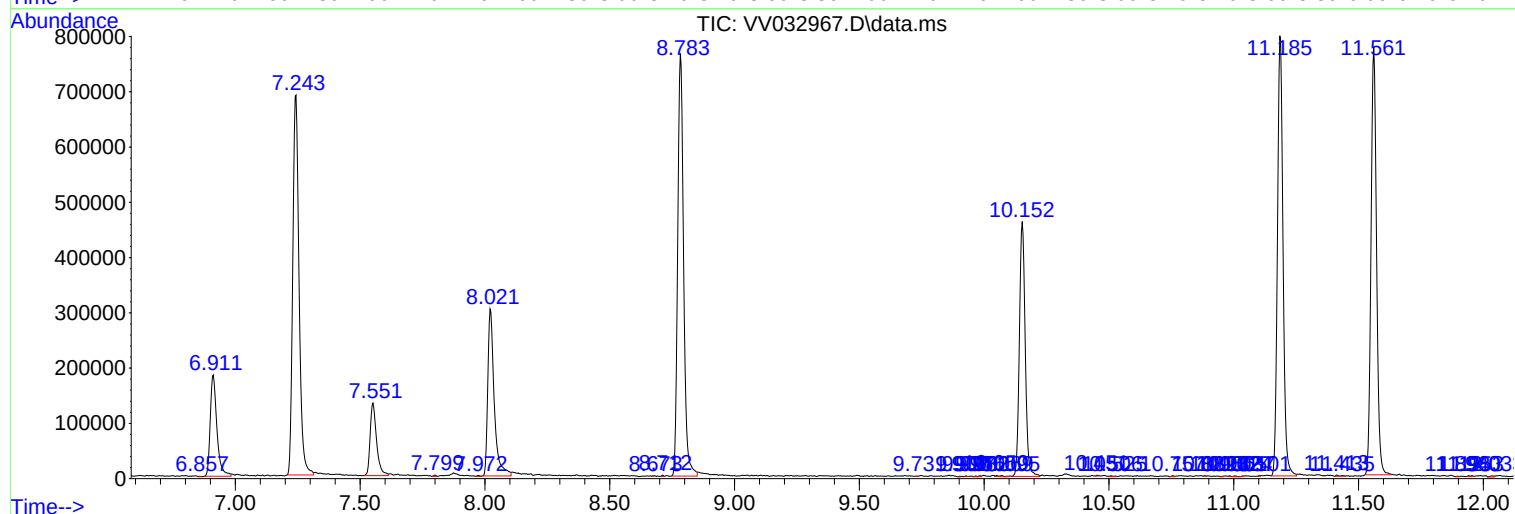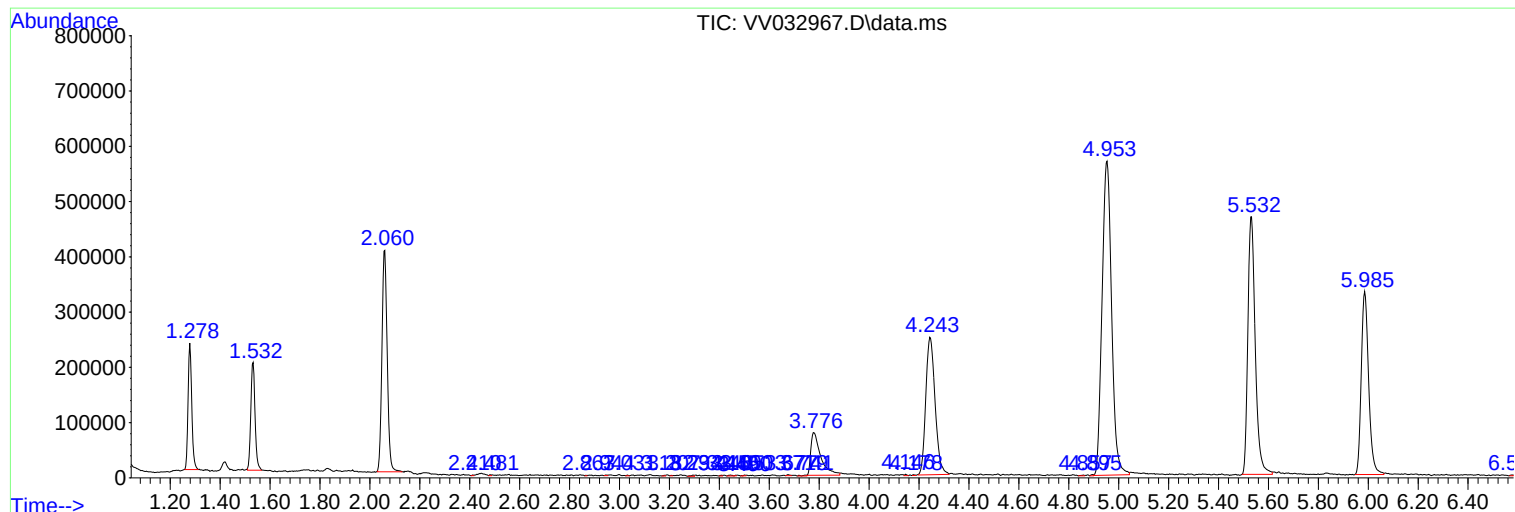

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111623\
Data File : VV032967.D
Acq On : 16 Nov 2023 12:52
Operator : SY/MD
Sample : 05416-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111623\
Data File : VV032967.D
Acq On : 16 Nov 2023 12:52
Operator : SY/MD
Sample : 05416-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------