

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111624\
 Data File : VV038154.D
 Acq On : 16 Nov 2024 10:41
 Operator : SY/MD
 Sample : P4761-15RE 2X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 17 23:35:29 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 00:15:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	13731	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.816	117	11019	0.500	ug/L	0.02
11) 1,4-Dichlorobenzene-d4	11.191	152	5232	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.329	65	6760	0.475	ug/L	0.06
Spiked Amount 0.500	Range 40 - 130		Recovery =	94.000%		
4) 1,2-Dichloroethane-d4	4.969	65	4241	0.492	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	98.000%		
7) 1,2-Dichloropropane-d6	6.067	67	5359	0.600	ug/L	0.07
Spiked Amount 0.500	Range 60 - 140		Recovery =	120.000%		
8) Toluene-d8	7.300	98	13056	0.571	ug/L	0.05
Spiked Amount 0.500	Range 70 - 130		Recovery =	114.000%		
10) 1,1,2,2-Tetrachloroeth...	10.146	84	3824	0.536	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	108.000%		
Target Compounds						Qvalue
13) 1,2-Dibromo-3-chloropr...	12.168	75	48	0.053	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111624\
Data File : VV038154.D
Acq On : 16 Nov 2024 10:41
Operator : SY/MD
Sample : P4761-15RE 2X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Nov 17 23:35:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

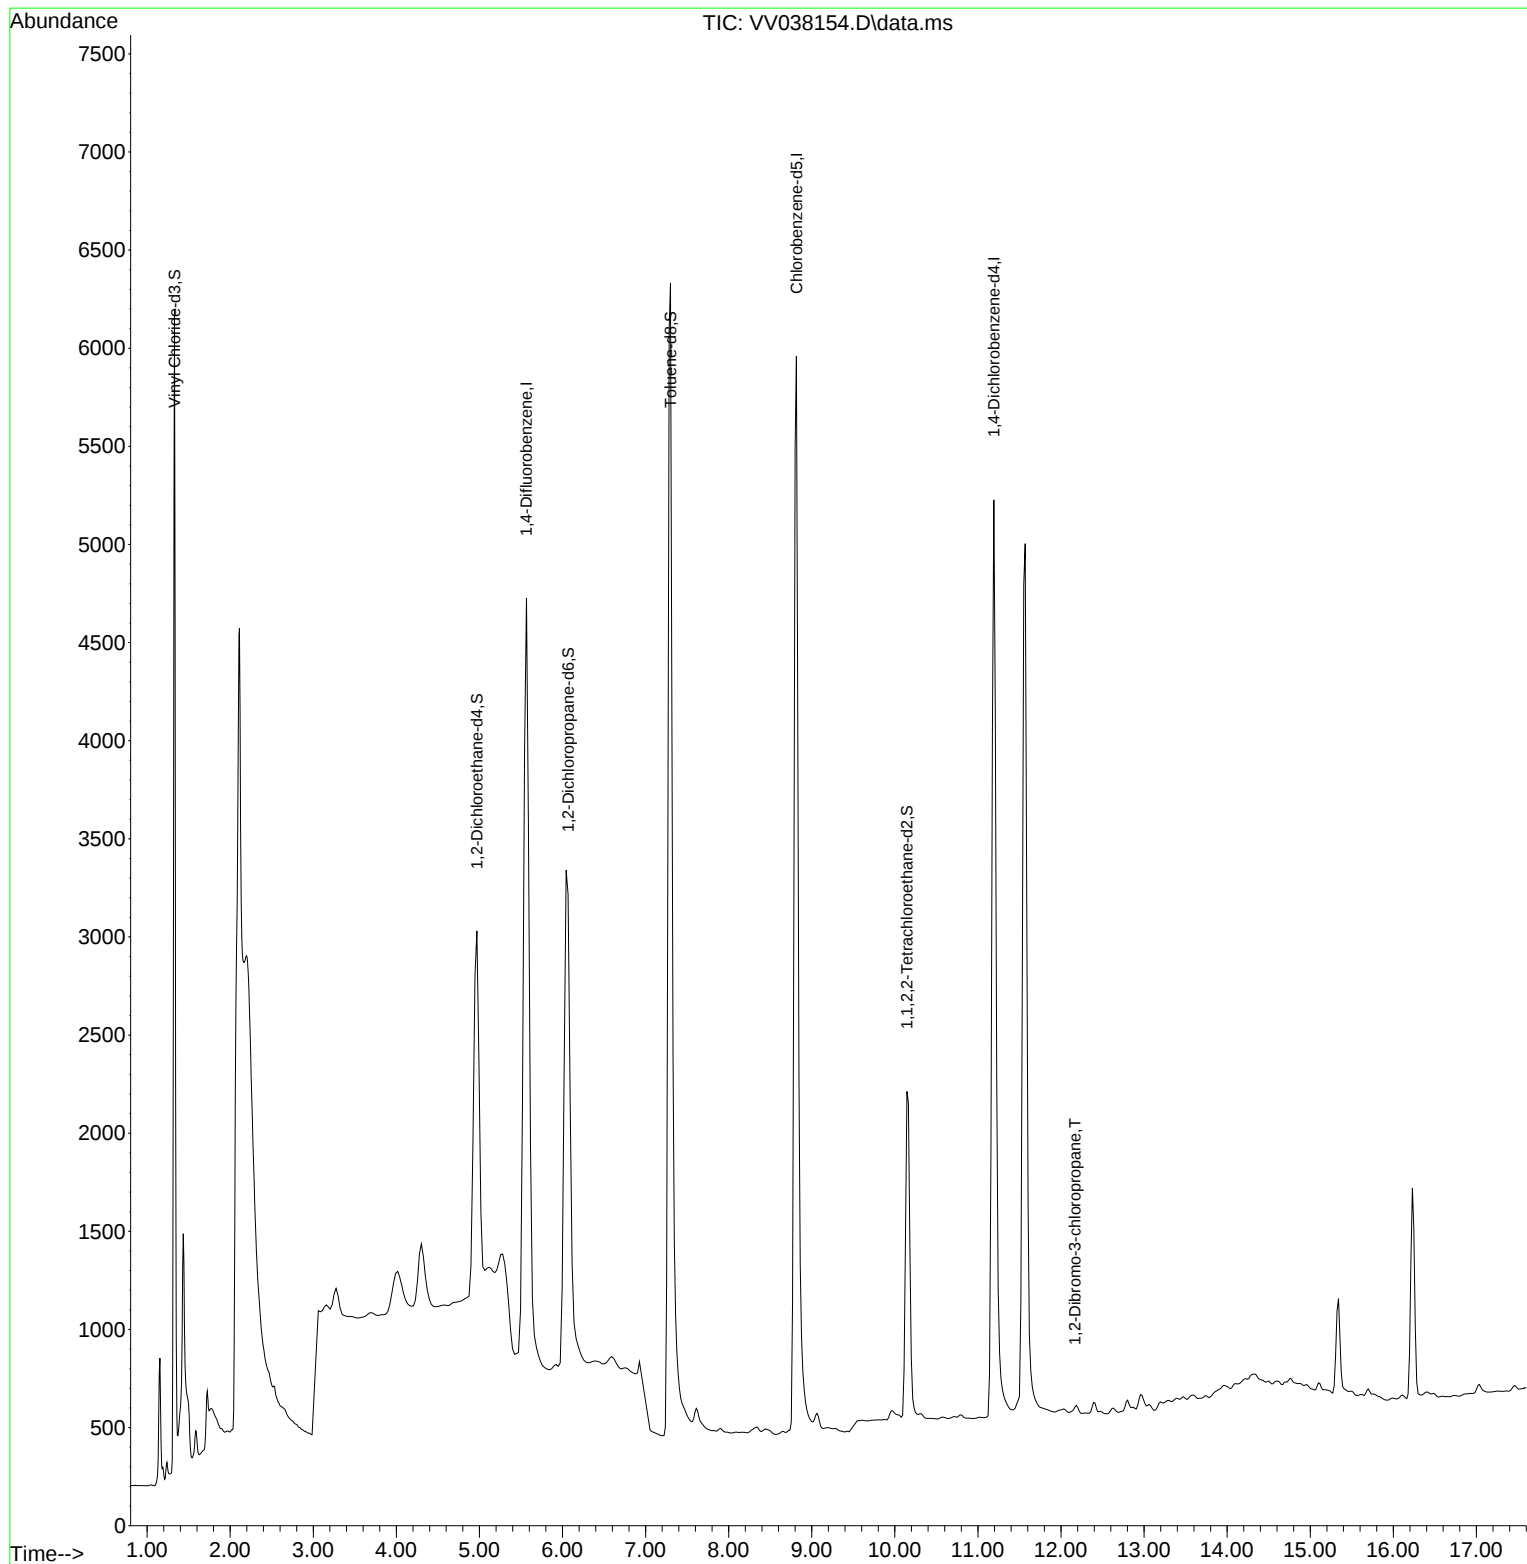

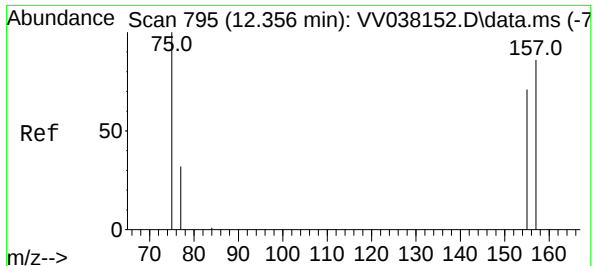

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.053 ug/L
 RT: 12.168 min Scan# 795
 Delta R.T. -0.188 min
 Lab File: VV038154.D
 Acq: 16 Nov 2024 10:41

Instrument :
 MSVOA_V
 ClientSampleId :

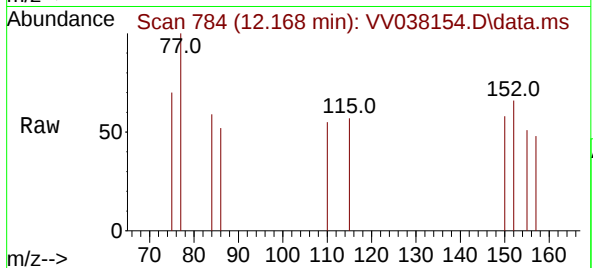

Tgt Ion: 75 Resp: 48

Ion	Ratio	Lower	Upper
75	100		
157	69.6	69.4	104.0
155	72.5	61.3	91.9

