

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111624\
 Data File : VV038158.D
 Acq On : 16 Nov 2024 13:02
 Operator : SY/MD
 Sample : VIBLK
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 17 23:36:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 00:15:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	10418	0.500	ug/L	-0.02
5) Chlorobenzene-d5	8.785	117	10633	0.500	ug/L	-0.02
11) 1,4-Dichlorobenzene-d4	11.191	152	5164	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.273	65	6172	0.572	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	114.000%
4) 1,2-Dichloroethane-d4	4.945	65	3522	0.539	ug/L	-0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	108.000%
7) 1,2-Dichloropropane-d6	5.995	67	4483	0.520	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	104.000%
8) Toluene-d8	7.238	98	11006	0.499	ug/L	-0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	100.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	3441	0.500	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	100.000%
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.168	75	21	0.023	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111624\
Data File : VV038158.D
Acq On : 16 Nov 2024 13:02
Operator : SY/MD
Sample : VIBLK
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Nov 17 23:36:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

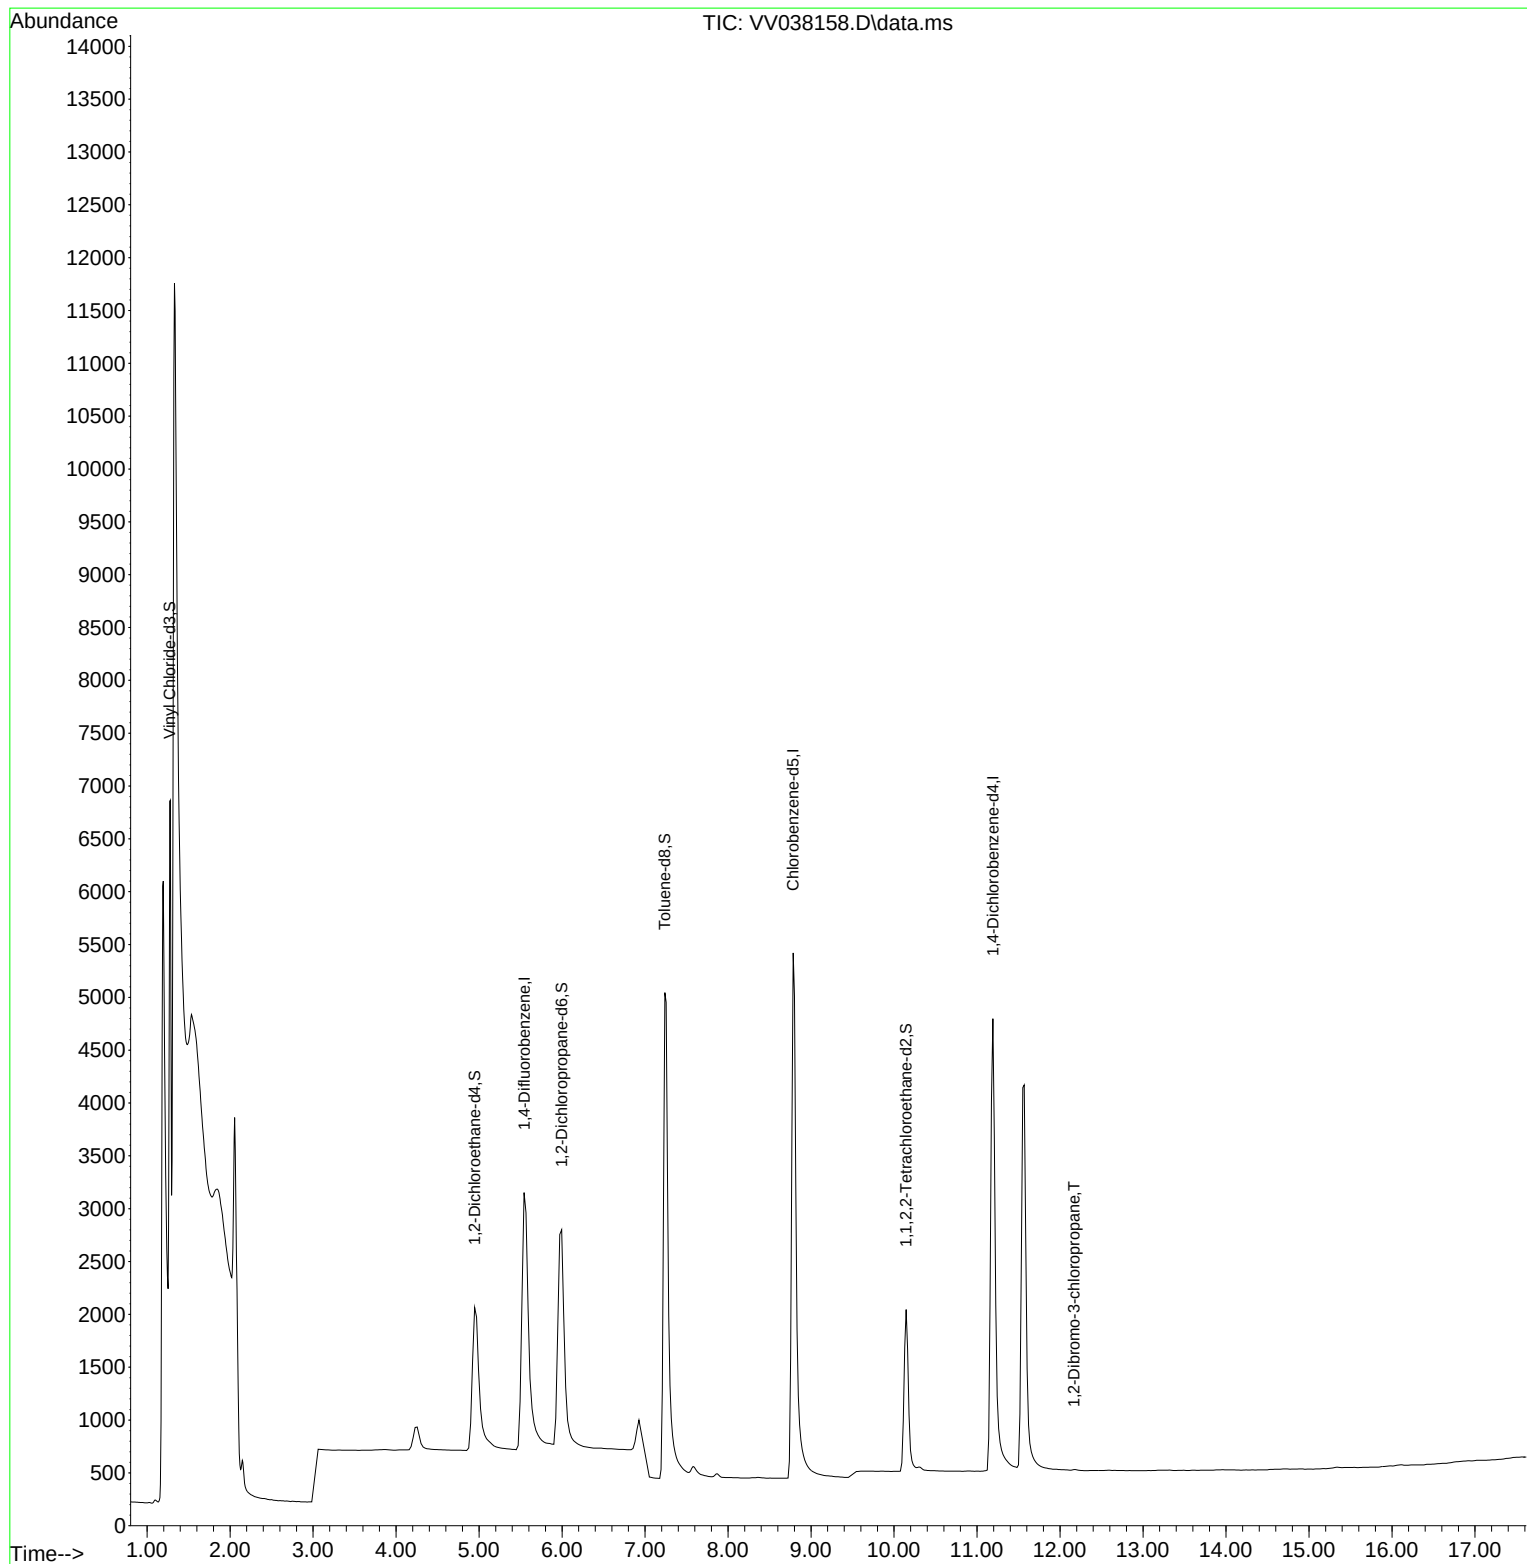

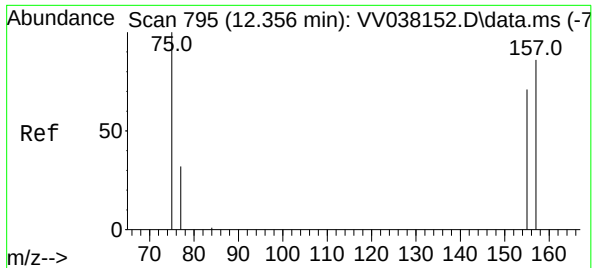

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.023 ug/L
 RT: 12.168 min Scan# 795
 Delta R.T. -0.188 min
 Lab File: VV038158.D
 Acq: 16 Nov 2024 13:02

Instrument :
 MSVOA_V
 ClientSampleId :

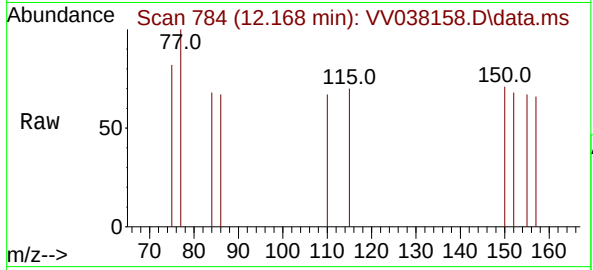

Tgt Ion: 75 Resp: 21

Ion	Ratio	Lower	Upper
75	100		
157	80.0	69.4	104.0
155	81.7	61.3	91.9

