
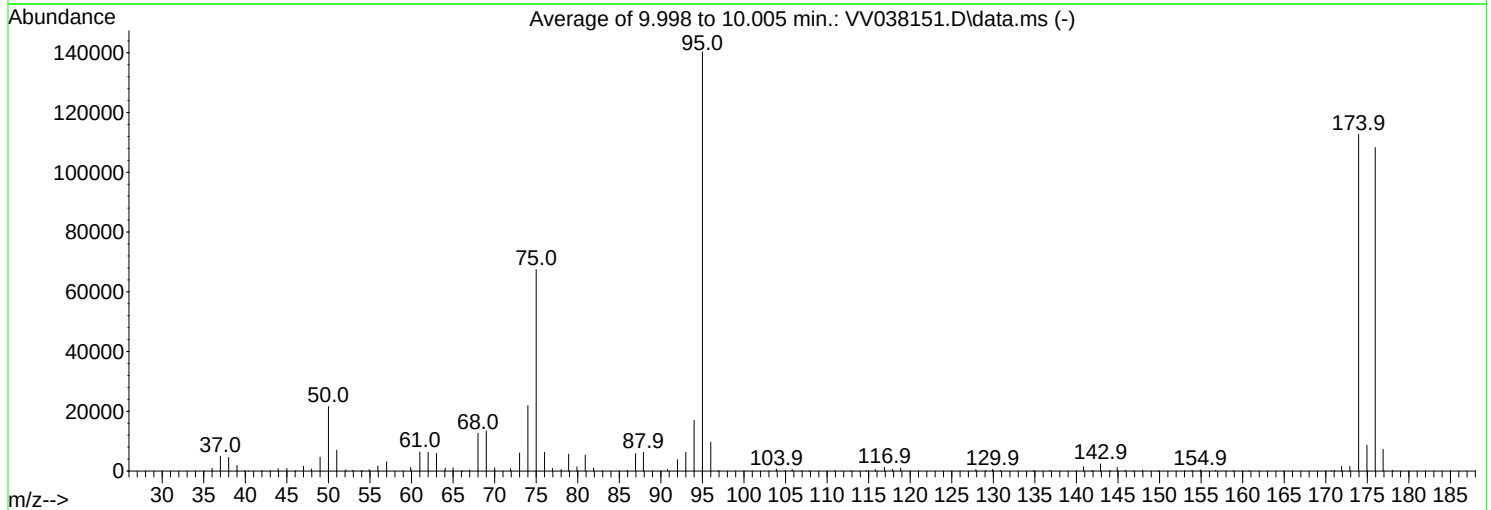


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111624\
Data File : VV038151.D
Acq On : 16 Nov 2024 08:31
Operator : SY/MD
Sample : BFB224
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB224

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Title : TRACE VOA SOM01.0
Last Update : Fri Nov 15 00:15:53 2024

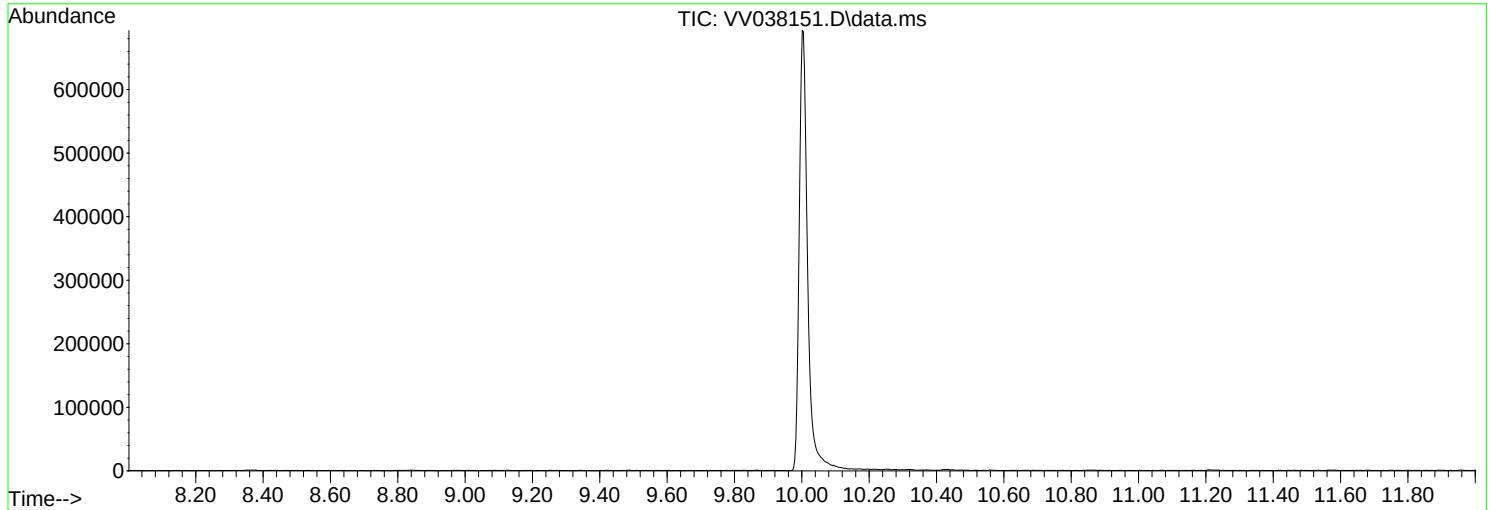

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2775

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	21605	PASS
75	95	30	80	48.1	67467	PASS
95	95	100	100	100.0	140352	PASS
96	95	5	9	6.9	9677	PASS
173	174	0.00	2	1.4	1615	PASS
174	95	50	120	80.3	112656	PASS
175	174	5	9	7.7	8656	PASS
176	174	95	101	96.2	108336	PASS
177	176	5	9	6.7	7286	PASS

m/z	Abundance
39.90	187.0
44.00	252.0

Instrument :
MSVOA_V
ClientSampleId :
BFB224

m/z	Abundance
36.00	998.0
37.00	4435.0
38.00	4364.0
39.00	1872.0
39.90	243.0
42.00	142.0
43.00	117.0
44.00	981.0
45.00	951.0
46.00	140.0
47.00	1669.0
47.90	613.0
49.00	4458.0
50.00	20184.0
51.00	6895.0
52.10	458.0
52.90	227.0
53.90	173.0
54.90	512.0
56.00	1476.0
57.00	3225.0
59.90	1238.0
61.00	6266.0
62.00	5759.0
63.00	5714.0
64.10	1031.0
65.00	1034.0
67.00	405.0
68.00	12283.0
69.00	12840.0
70.00	971.0
71.90	673.0
73.00	5976.0
74.00	20672.0
75.00	64072.0
76.00	6200.0
77.00	834.0
78.00	535.0
78.90	5362.0
79.90	1320.0
80.90	4974.0
81.90	1021.0
86.00	203.0
87.00	5591.0
87.90	6062.0
90.80	491.0
92.00	3587.0
93.00	5641.0
94.00	15731.0
95.00	131392.0
96.00	9074.0
96.90	204.0
103.90	679.0
104.90	278.0
105.80	516.0
107.00	137.0
112.80	125.0
114.70	184.0
115.80	520.0
116.90	1119.0
117.90	572.0
118.90	853.0
127.90	408.0
129.20	192.0
129.90	463.0
130.80	275.0
134.80	209.0
136.80	289.0
140.90	1249.0
141.90	219.0
142.90	2092.0
144.10	120.0
144.90	1189.0
145.90	289.0
146.90	154.0
147.90	285.0
153.00	149.0
153.90	197.0
154.90	450.0
156.70	237.0
158.80	177.0
160.70	182.0
170.70	467.0
171.90	1340.0
172.90	1396.0
173.90	103464.0
175.00	7788.0
176.00	99560.0
176.90	6875.0
178.00	211.0

Instrument :
MSVOA_V
ClientSampleId :
BFB224

m/z	Abundance
36.00	929.0
37.00	5085.0
38.00	4697.0
39.00	1922.0
39.90	249.0
40.40	163.0
42.00	126.0
43.00	116.0
43.90	1065.0
45.00	870.0
46.10	196.0
47.00	1641.0
48.00	711.0
49.00	4779.0
50.00	22344.0
51.00	7238.0
52.10	475.0
53.00	298.0
54.10	194.0
54.90	524.0
55.90	1743.0
57.00	3159.0
59.90	1289.0
61.00	6703.0
62.00	6540.0
63.00	6157.0
64.10	1087.0
65.00	1142.0
66.10	138.0
67.00	366.0
68.00	12912.0
69.00	13948.0
70.00	1136.0
71.90	807.0
73.00	6200.0
74.00	22688.0
75.00	69648.0
76.00	6431.0
76.90	970.0
78.00	533.0
78.90	5856.0
79.90	1449.0
80.90	5394.0
81.90	1000.0
82.90	130.0
85.90	207.0
87.00	6000.0
87.90	6513.0
90.80	534.0
92.00	3889.0
93.00	6503.0
94.00	17632.0
95.00	145472.0
96.00	10121.0
96.90	240.0
103.90	715.0
104.90	295.0
105.80	584.0
106.90	116.0
107.80	126.0
110.90	155.0
112.80	117.0
114.70	194.0
115.80	517.0
116.90	1275.0
117.80	599.0
118.90	993.0
127.90	546.0
129.10	236.0
129.90	576.0
130.80	268.0
134.80	248.0
136.80	283.0
140.90	1499.0
141.90	252.0
142.90	2393.0
144.10	160.0
144.90	1285.0
145.80	330.0
146.80	149.0
148.00	351.0
149.80	135.0
153.00	126.0
153.90	194.0
154.90	466.0
156.70	250.0
158.00	115.0
158.90	181.0
160.80	168.0
171.00	455.0
171.90	1606.0
172.90	1699.0

Instrument :
MSVOA_V
ClientSampleId :
BFB224

173.90	116264.0
174.90	8928.0
176.00	112000.0
176.90	7486.0
178.00	207.0

Instrument :
MSVOA_V
ClientSampleId :
BFB224

m/z	Abundance
36.00	801.0
37.00	5470.0
38.00	4628.0
39.00	1925.0
39.90	272.0
42.00	101.0
43.90	1170.0
45.00	791.0
46.10	195.0
47.00	1539.0
48.00	816.0
49.00	4814.0
50.00	22288.0
51.00	6838.0
52.10	410.0
53.00	292.0
54.10	223.0
54.90	397.0
56.00	1842.0
57.00	2925.0
59.90	1122.0
61.00	6324.0
62.00	6512.0
63.00	5892.0
64.00	1054.0
65.00	1103.0
66.20	186.0
66.90	331.0
68.00	12703.0
69.00	13423.0
70.00	1170.0
71.90	889.0
73.00	5930.0
74.00	22392.0
75.00	68680.0
76.00	6186.0
76.90	906.0
78.00	525.0
78.90	5783.0
79.90	1516.0
80.90	5684.0
81.90	947.0
83.00	199.0
85.90	219.0
86.90	5772.0
87.90	6287.0
90.80	540.0
92.00	3919.0
93.00	6642.0
94.00	17448.0
95.00	144192.0
96.00	9837.0
96.90	259.0
103.90	639.0
105.00	261.0
105.80	601.0
106.90	103.0
107.80	165.0
110.90	199.0
111.70	106.0
112.80	107.0
114.70	175.0
115.80	529.0
116.90	1300.0
117.80	676.0
118.80	1032.0
127.90	625.0
129.00	290.0
129.90	653.0
130.90	221.0
134.80	263.0
136.80	199.0
140.80	1568.0
141.80	256.0
142.90	2666.0
144.10	158.0
144.90	1204.0
145.80	300.0
146.70	146.0
148.00	340.0
149.80	165.0
153.00	125.0
153.90	163.0
154.90	455.0
156.80	271.0
158.00	105.0
158.90	174.0
160.80	172.0
171.10	455.0
171.90	1782.0
172.90	1750.0
174.00	118240.0

Instrument :
MSVOA_V
ClientSampleId :
BFB224

174.90	9253.0
175.90	113448.0
176.90	7498.0
178.10	223.0

Instrument :
MSVOA_V
ClientSampleId :
BFB224