




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028666.D
Acq On : 16 Nov 2023 16:23
Operator : MA/JU
Sample : 05338-19
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5210

Manual IntegrationsAPPROVED

Quant Time: Nov 16 18:05:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 14:20:35 2023
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/20/2023
Supervised By :Semsettin Yesilyurt 11/20/2023

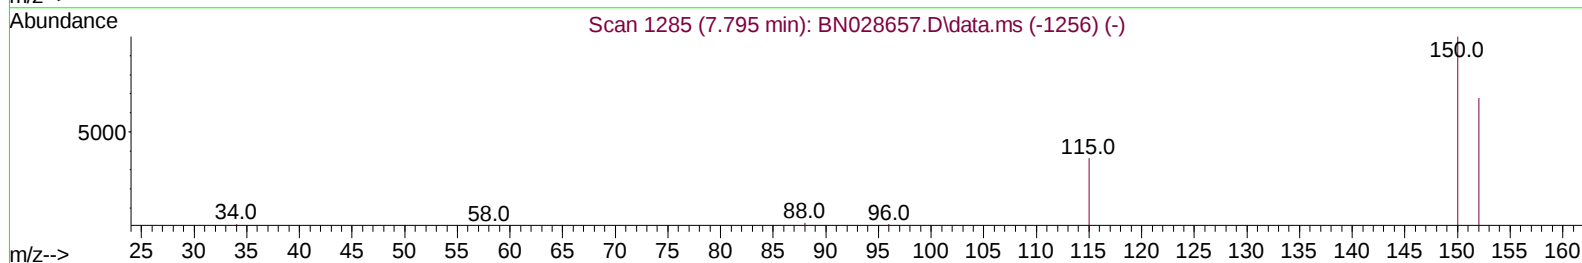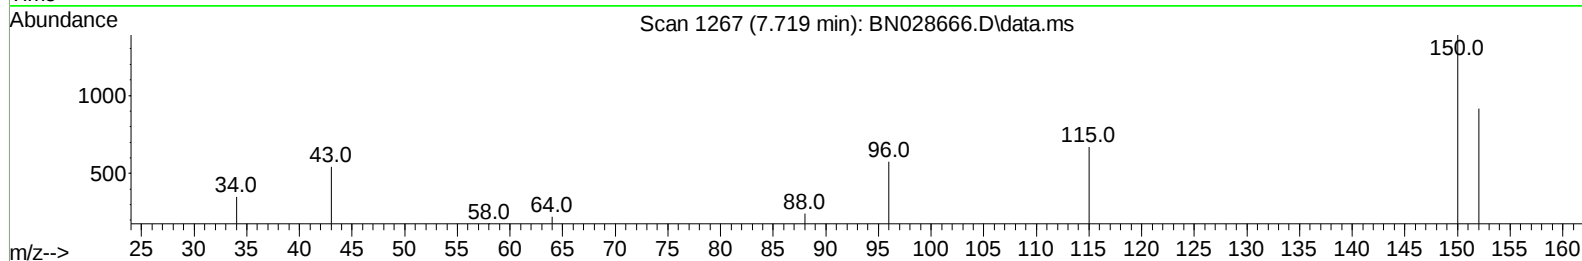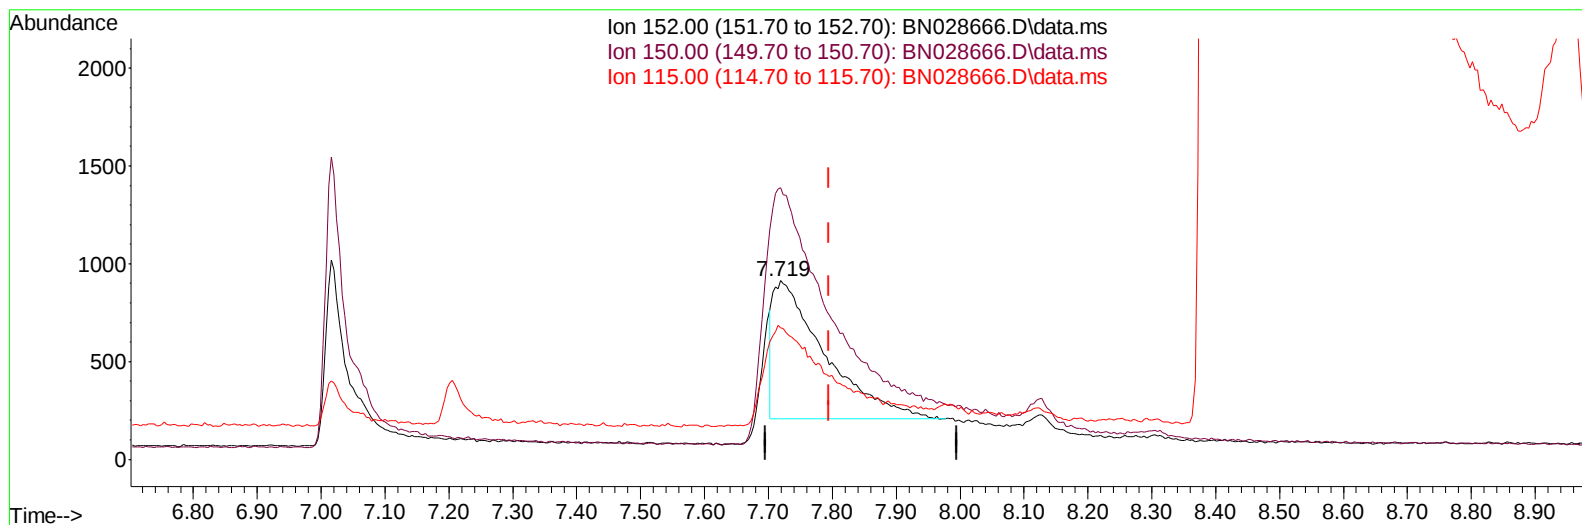

TIC: BN028666.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.719min (-0.076) 0.40 ng/u1

response 3987

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	151.86
115.00	62.20	73.41
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028666.D
Acq On : 16 Nov 2023 16:23
Operator : MA/JU
Sample : 05338-19
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5210

Manual IntegrationsAPPROVED

Quant Time: Nov 16 18:05:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 14:20:35 2023
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/20/2023
Supervised By :Semsettin Yesilyurt 11/20/2023

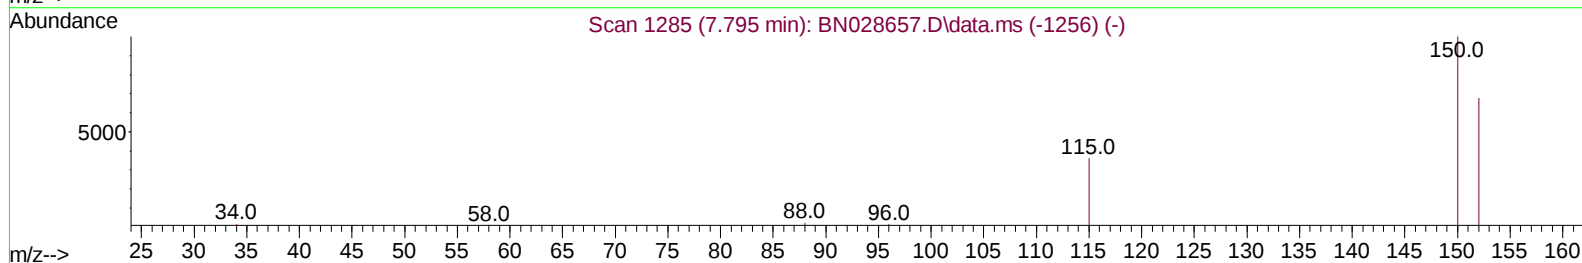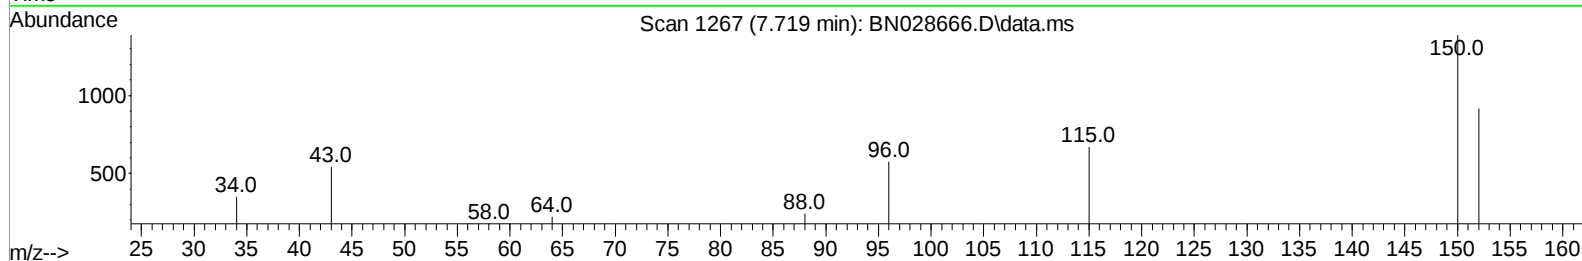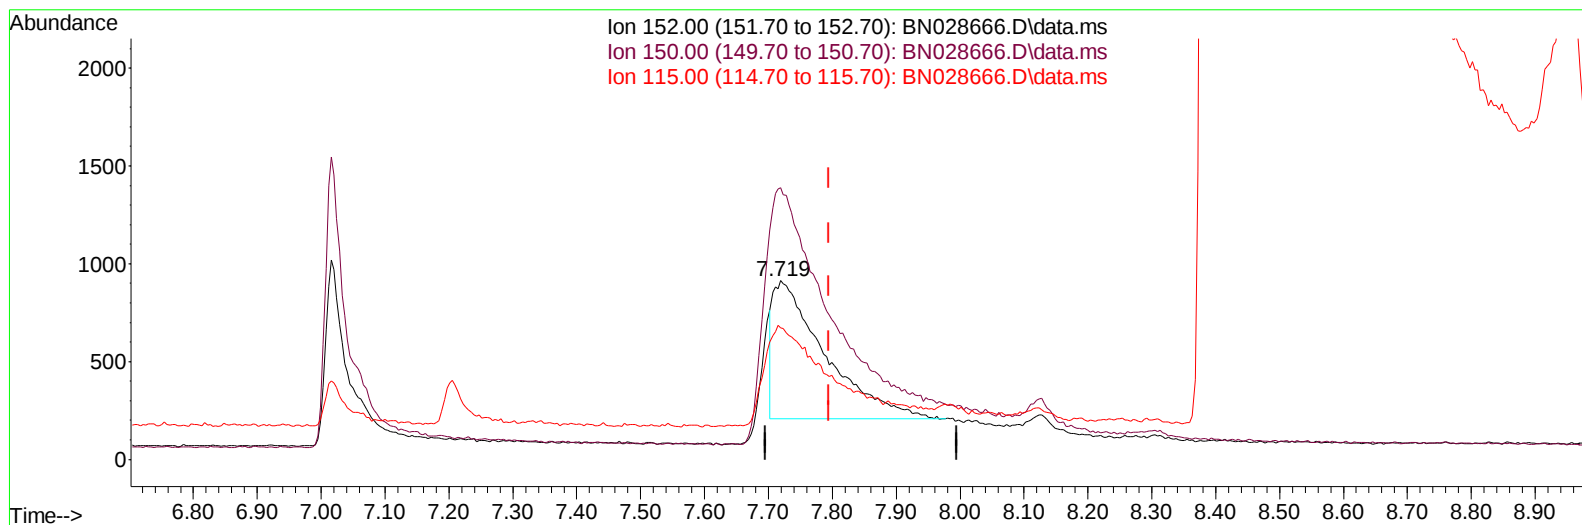

TIC: BN028666.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.719min (-0.076) 0.40 ng/u1

response 3987

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	151.86
115.00	62.20	73.41
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028666.D
Acq On : 16 Nov 2023 16:23
Operator : MA/JU
Sample : 05338-19
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5210

Manual IntegrationsAPPROVED

Quant Time: Nov 16 18:05:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 14:20:35 2023
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/20/2023
Supervised By :Semsettin Yesilyurt 11/20/2023

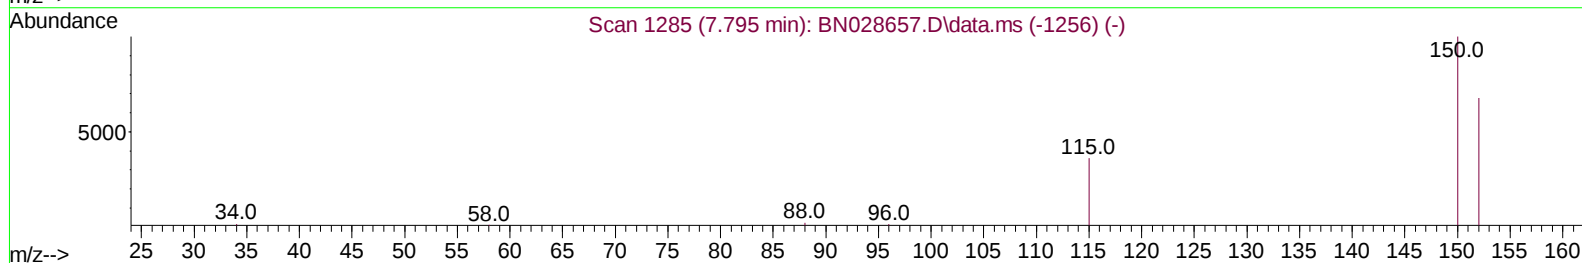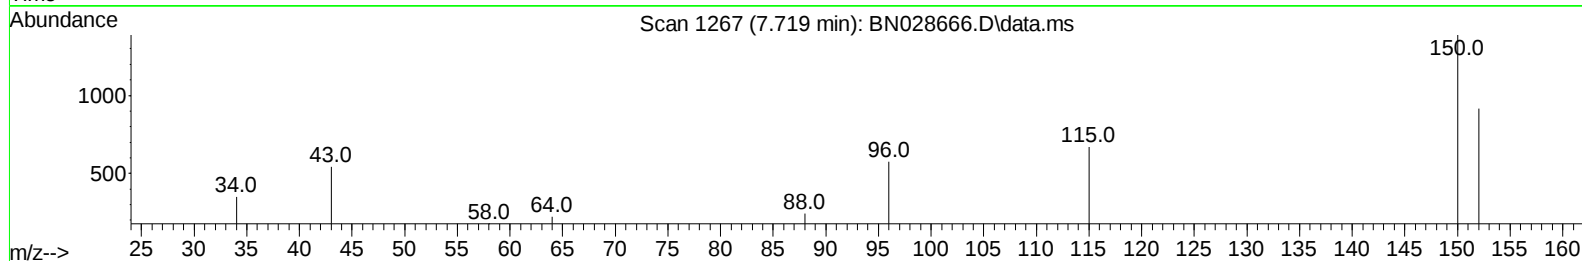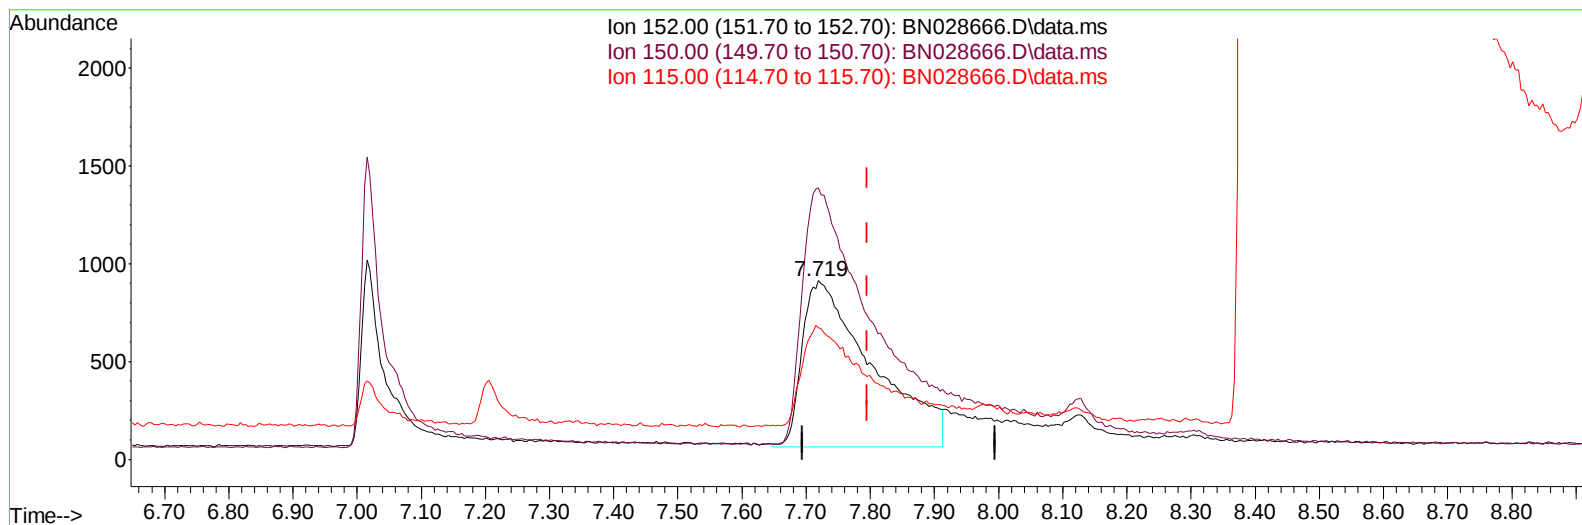

TIC: BN028666.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.719min (-0.076) 0.40 ng/ul m

response 6496

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	155.30	151.86
115.00	62.20	73.41
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111523\
Data File : BN028666.D
Acq On : 16 Nov 2023 16:23
Operator : MA/JU
Sample : 05338-19
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5210

Manual IntegrationsAPPROVED

Quant Time: Nov 16 18:05:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 14:20:35 2023
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/20/2023
Supervised By :Semsettin Yesilyurt 11/20/2023

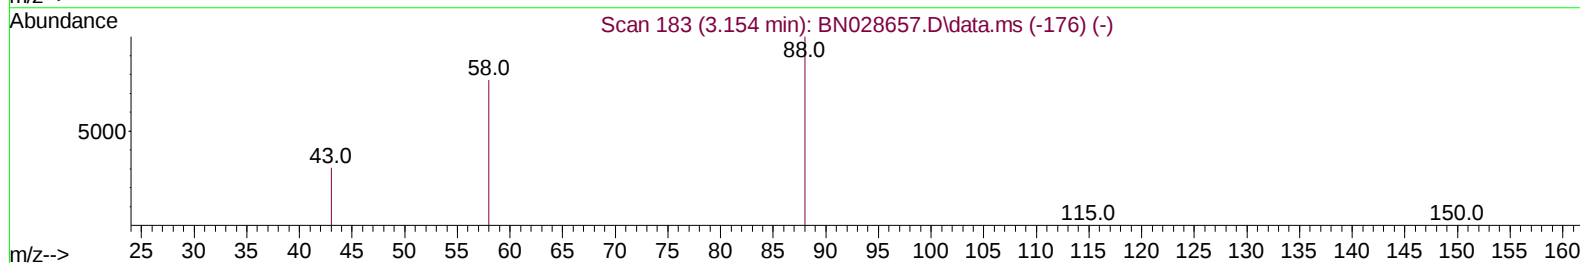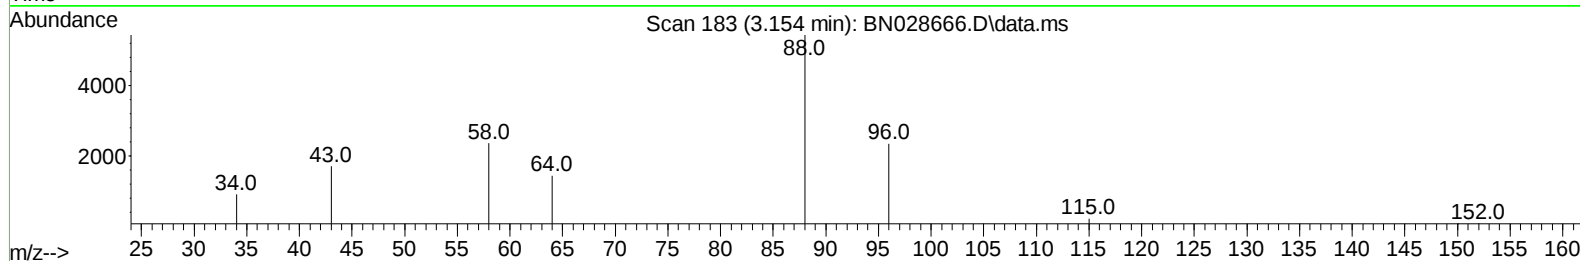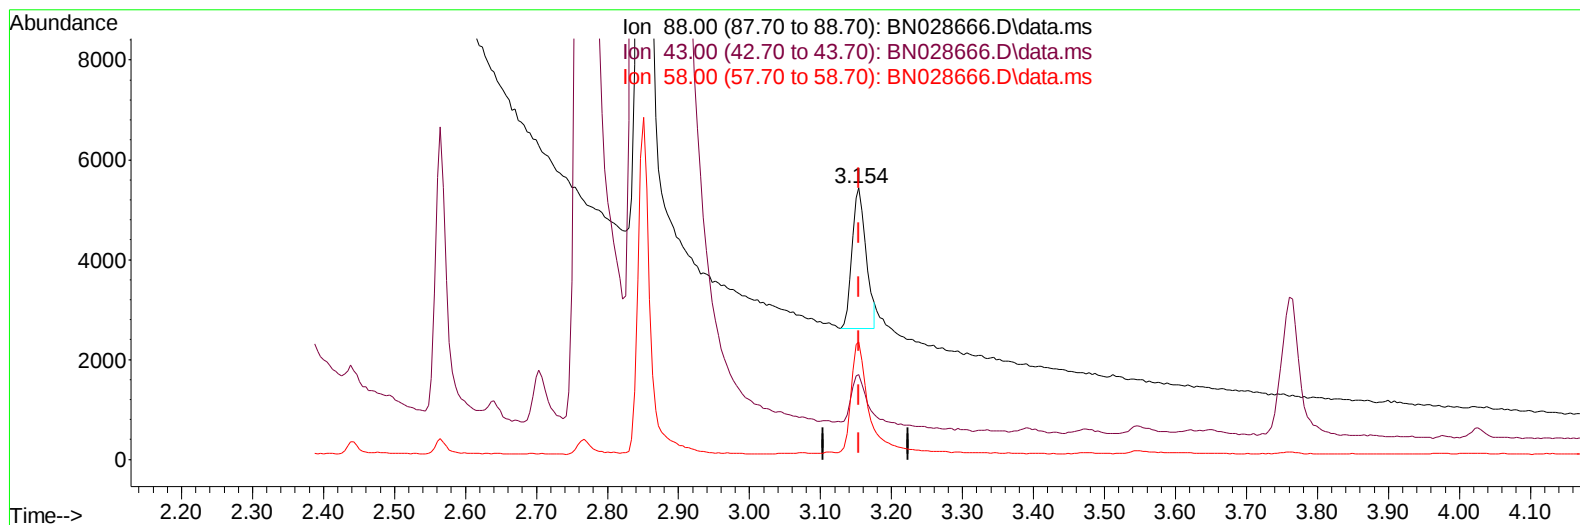

TIC: BN028666.D\data.ms

(2) 1,4-Dioxane

3.154min (+ 0.000) 0.48 ng/u1

response 3847

Ion	Exp%	Act%
88.00	100.00	100.00
43.00	41.10	31.28#
58.00	52.30	43.32
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111723\
 Data File : VV032970.D
 Acq On : 16 Nov 2023 17:36
 Operator : SY/MD
 Sample : VSTD0.510
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5210

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 11/20/2023
 Supervised By :Semsettin Yesilyurt 11/20/2023

Quant Time: Nov 17 00:30:12 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 17 00:29:50 2023
 Response via : Initial Calibration

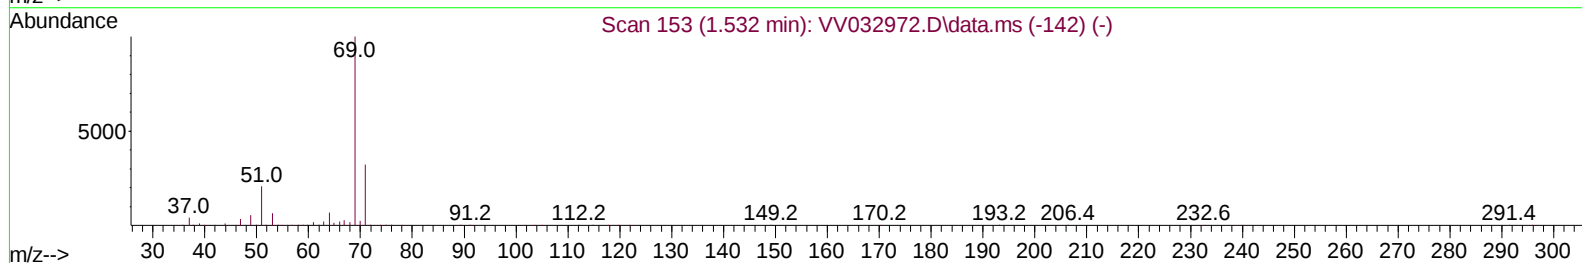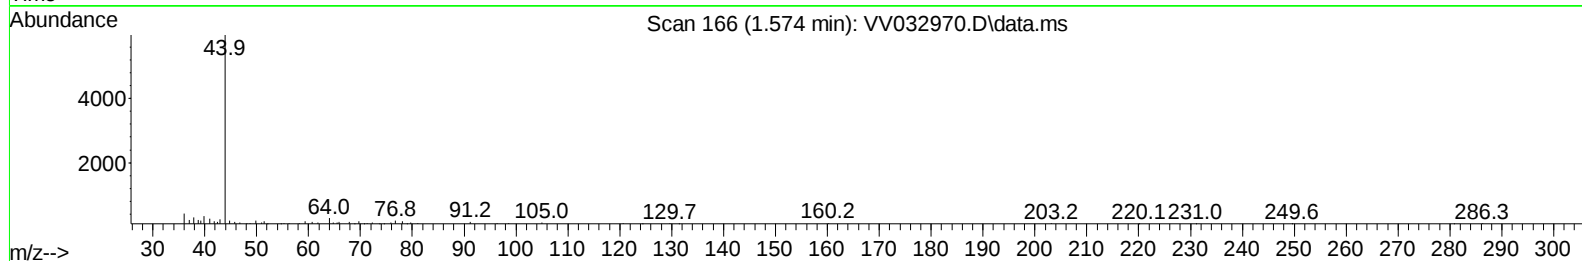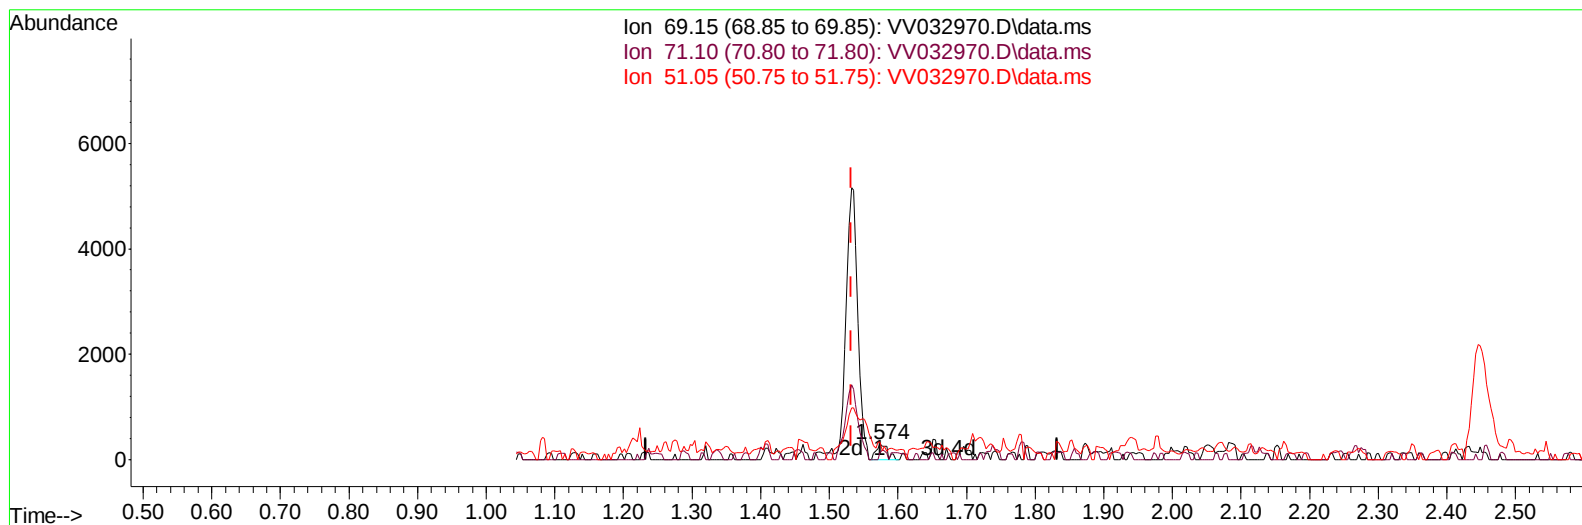

TIC: VV032970.D\data.ms

(7) Chloroethane-d5 (S)

1.574min (+ 0.042) 0.02 ug/L

response 337

Ion	Exp%	Act%
69.15	100.00	100.00
71.10	30.90	34.12
51.05	26.10	26.71
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111723\
 Data File : VV032970.D
 Acq On : 16 Nov 2023 17:36
 Operator : SY/MD
 Sample : VSTD0.510
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5210

Manual IntegrationsAPPROVED

Quant Time: Nov 17 00:30:12 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 17 00:29:50 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/20/2023
 Supervised By :Semsettin Yesilyurt 11/20/2023

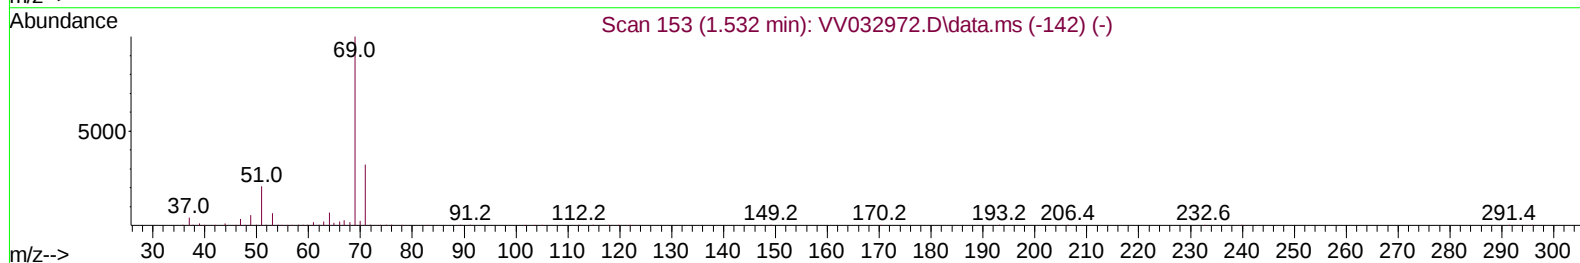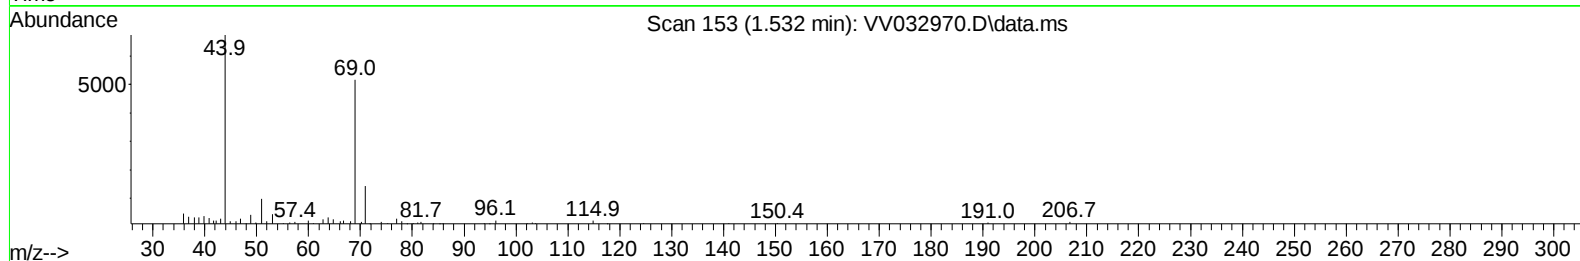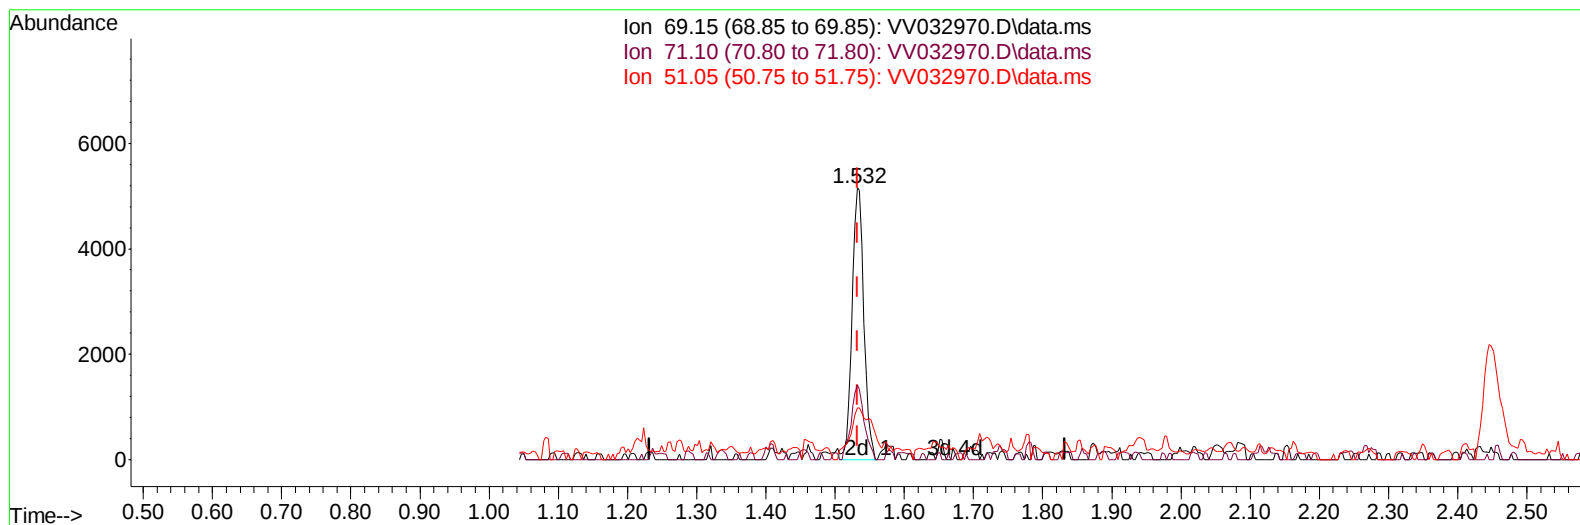

TIC: VV032970.D\data.ms

(7) Chloroethane-d5 (S)

1.532min (-0.000) 0.45 ug/L m

response 6121

Ion	Exp%	Act%
69.15	100.00	100.00
71.10	30.90	1.88#
51.05	26.10	1.47#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111723\
 Data File : VV032970.D
 Acq On : 16 Nov 2023 17:36
 Operator : SY/MD
 Sample : VSTD0.510
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5210

Manual IntegrationsAPPROVED

Quant Time: Nov 17 00:30:12 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 17 00:29:50 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/20/2023
 Supervised By :Semsettin Yesilyurt 11/20/2023

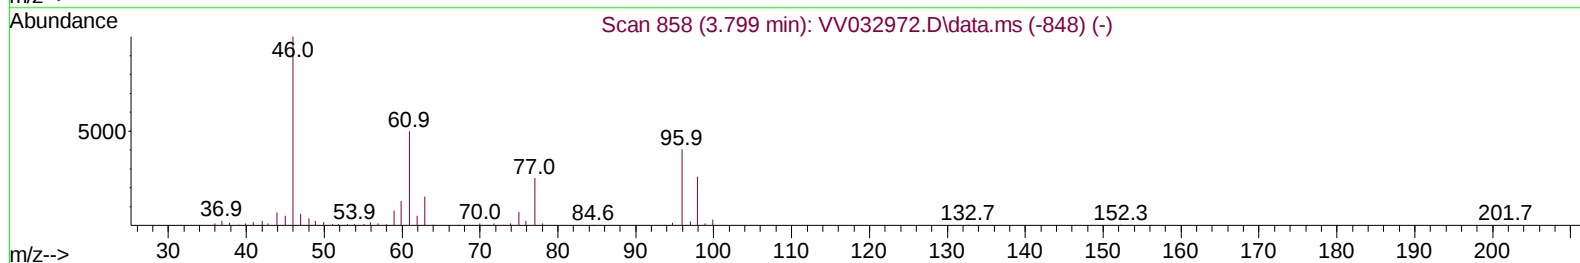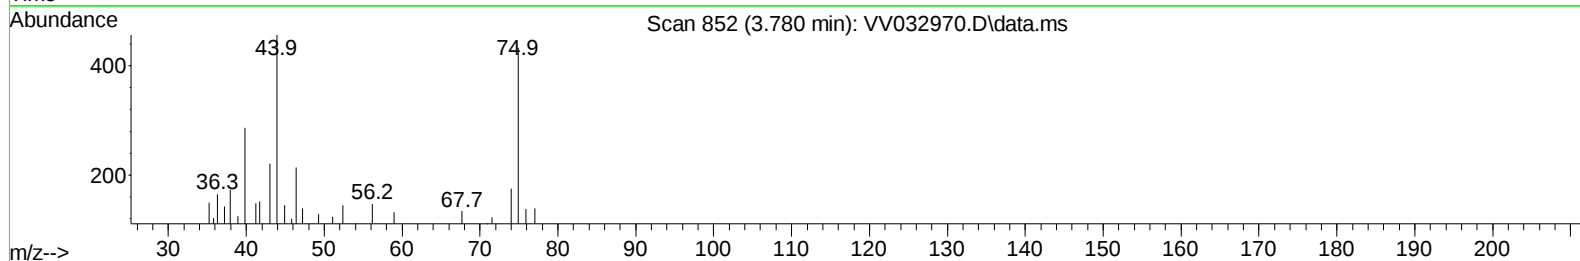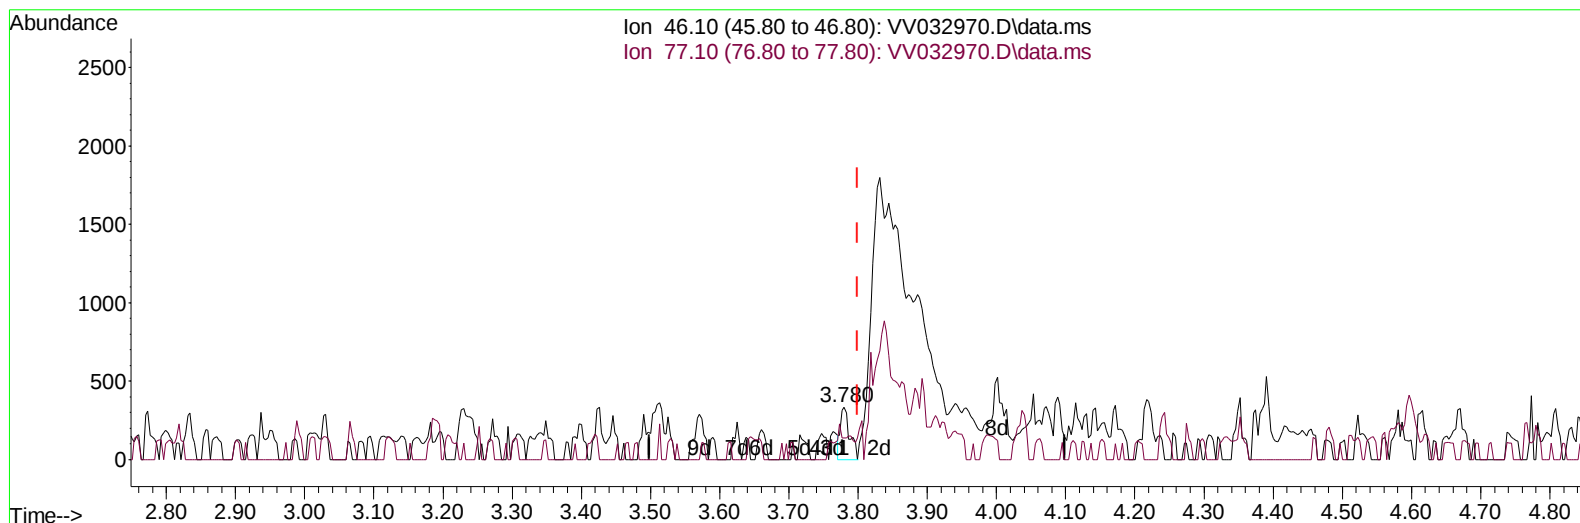

TIC: VV032970.D\data.ms

(20) 2-Butanone-d5 (S)

3.780min (-0.019) 0.16 ug/L

response 310

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	25.90	36.13#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111723\
 Data File : VV032970.D
 Acq On : 16 Nov 2023 17:36
 Operator : SY/MD
 Sample : VSTD0.510
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5210

Manual IntegrationsAPPROVED

Quant Time: Nov 17 00:30:12 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 17 00:29:50 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/20/2023
 Supervised By :Semsettin Yesilyurt 11/20/2023

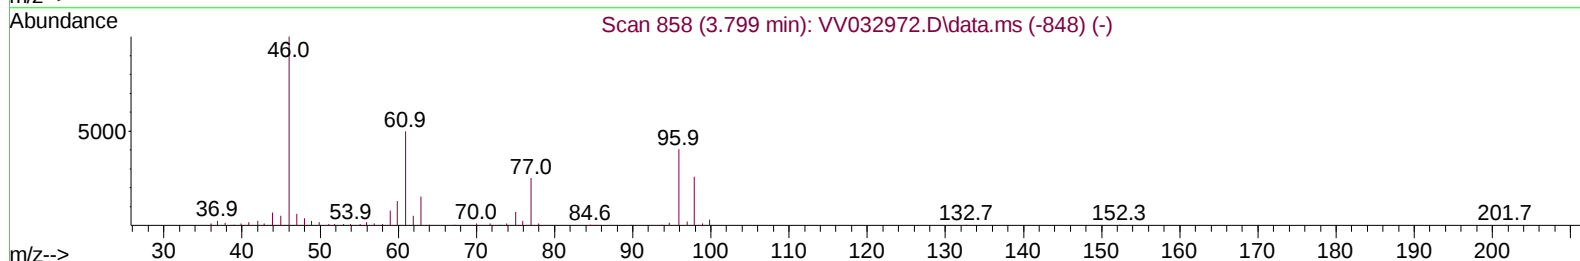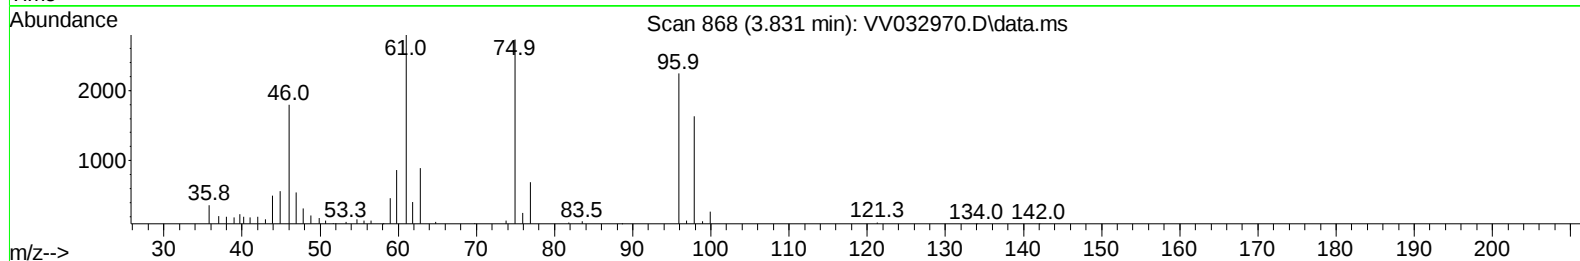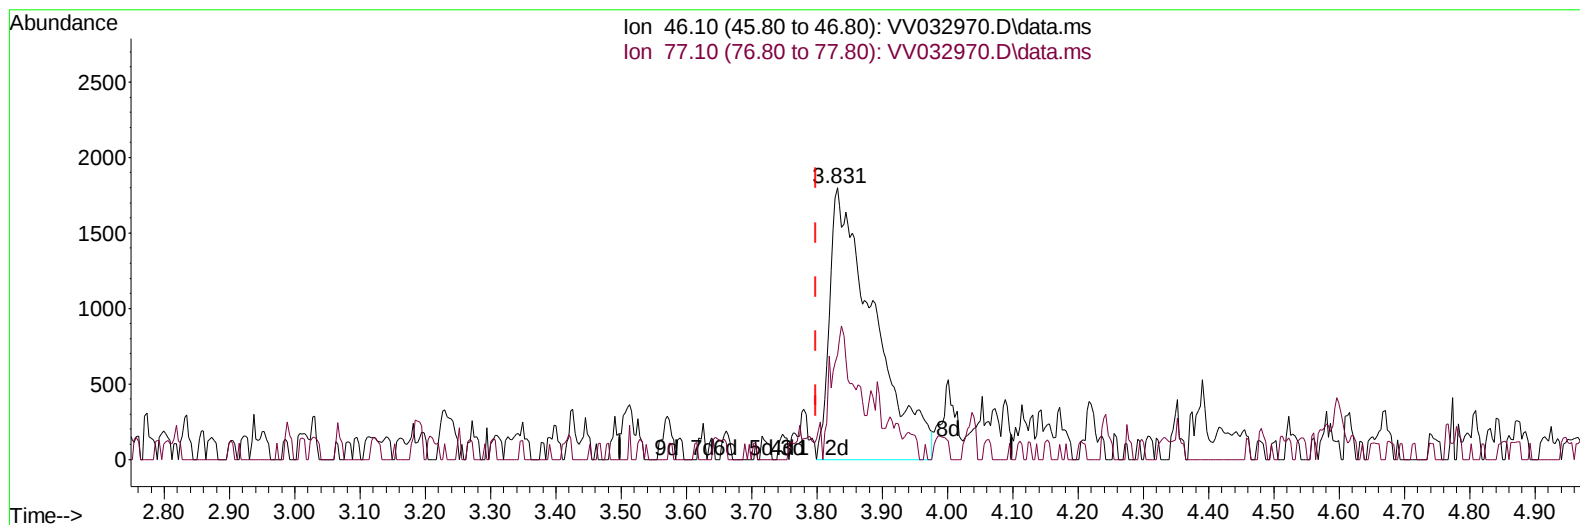

TIC: VV032970.D\data.ms

(20) 2-Butanone-d5 (S)

3.831min (+ 0.032) 4.44 ug/L m

response 8412

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	25.90	1.33#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111723\
Data File : VV032970.D
Acq On : 16 Nov 2023 17:36
Operator : SY/MD
Sample : VSTD0.510
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5210

Manual IntegrationsAPPROVED

Quant Time: Nov 17 00:30:12 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 17 00:29:50 2023
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/20/2023
Supervised By :Semsettin Yesilyurt 11/20/2023

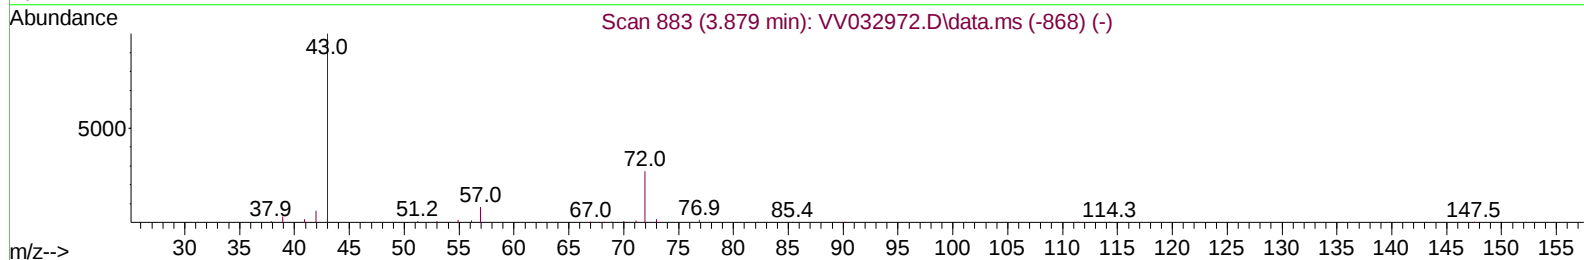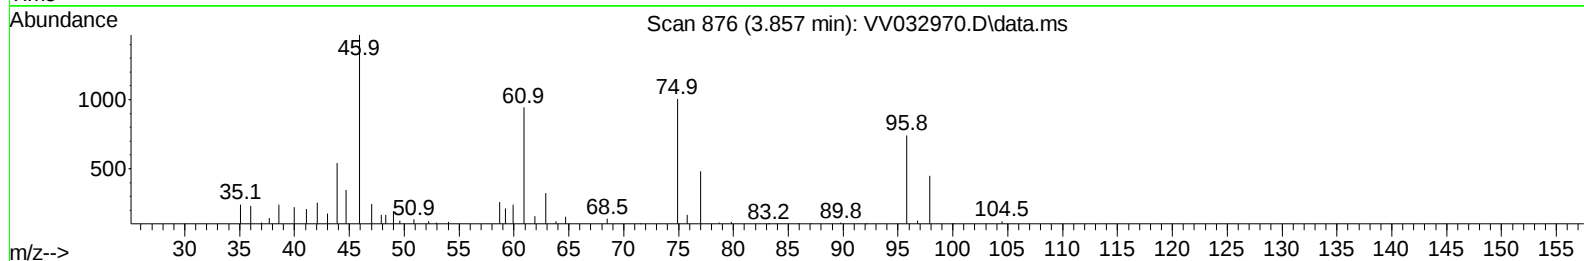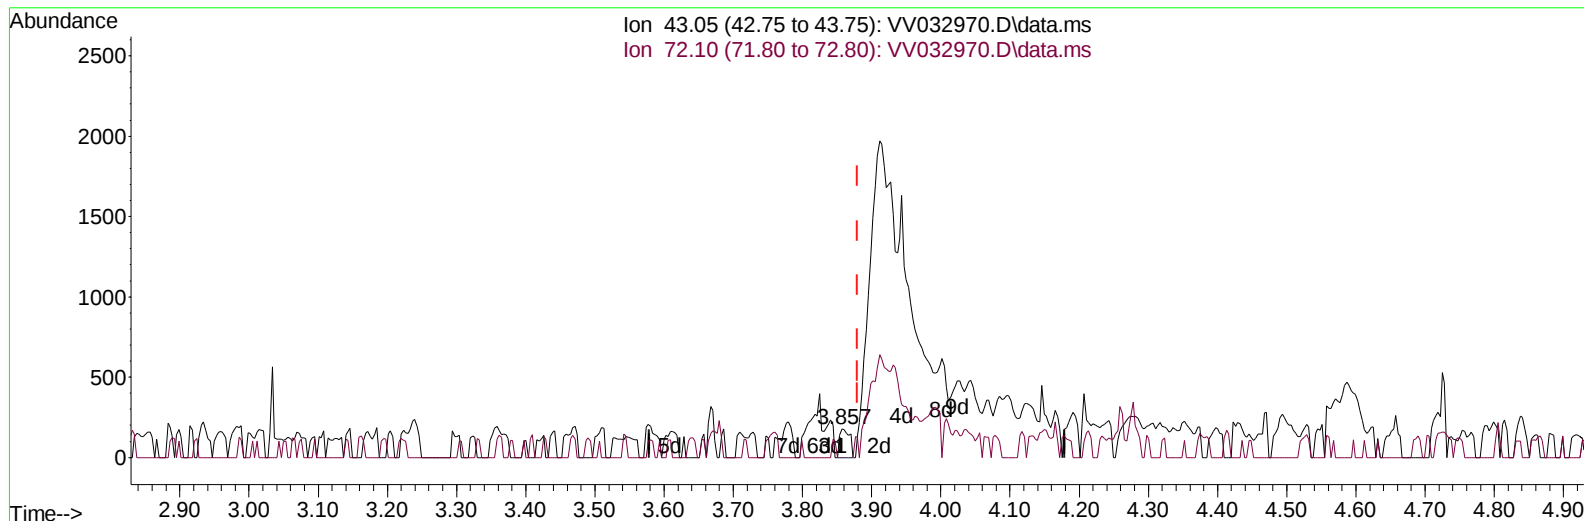

TIC: VV032970.D\data.ms

(21) 2-Butanone (T)

3.857min (-0.023) 0.08 ug/L

response 178

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	26.70	27.53
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111723\
 Data File : VV032970.D
 Acq On : 16 Nov 2023 17:36
 Operator : SY/MD
 Sample : VSTD0.510
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5210

Manual IntegrationsAPPROVED

Quant Time: Nov 17 00:30:12 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 17 00:29:50 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/20/2023
 Supervised By :Semsettin Yesilyurt 11/20/2023

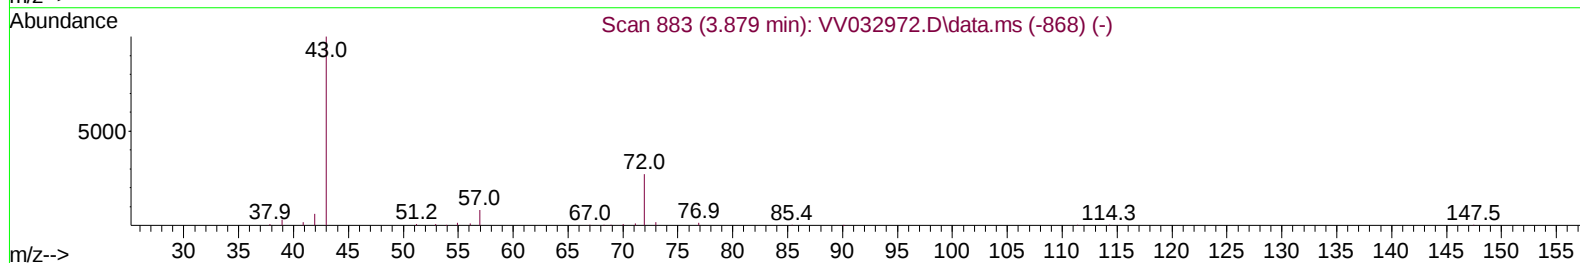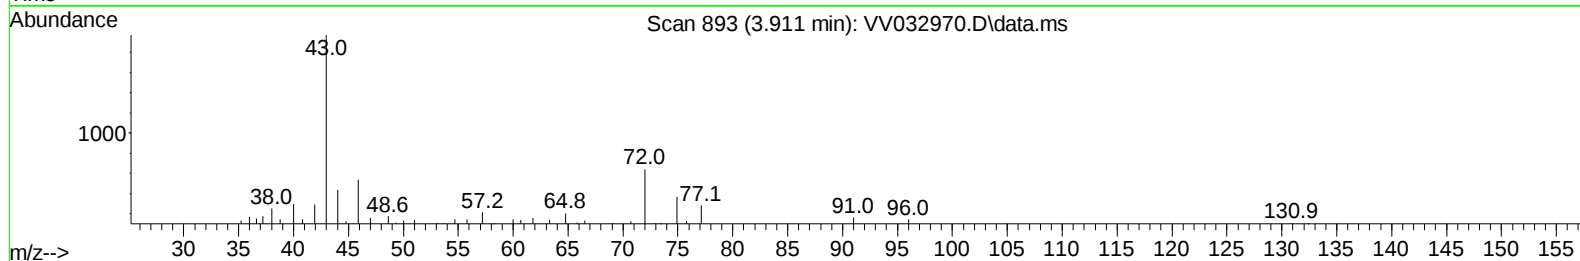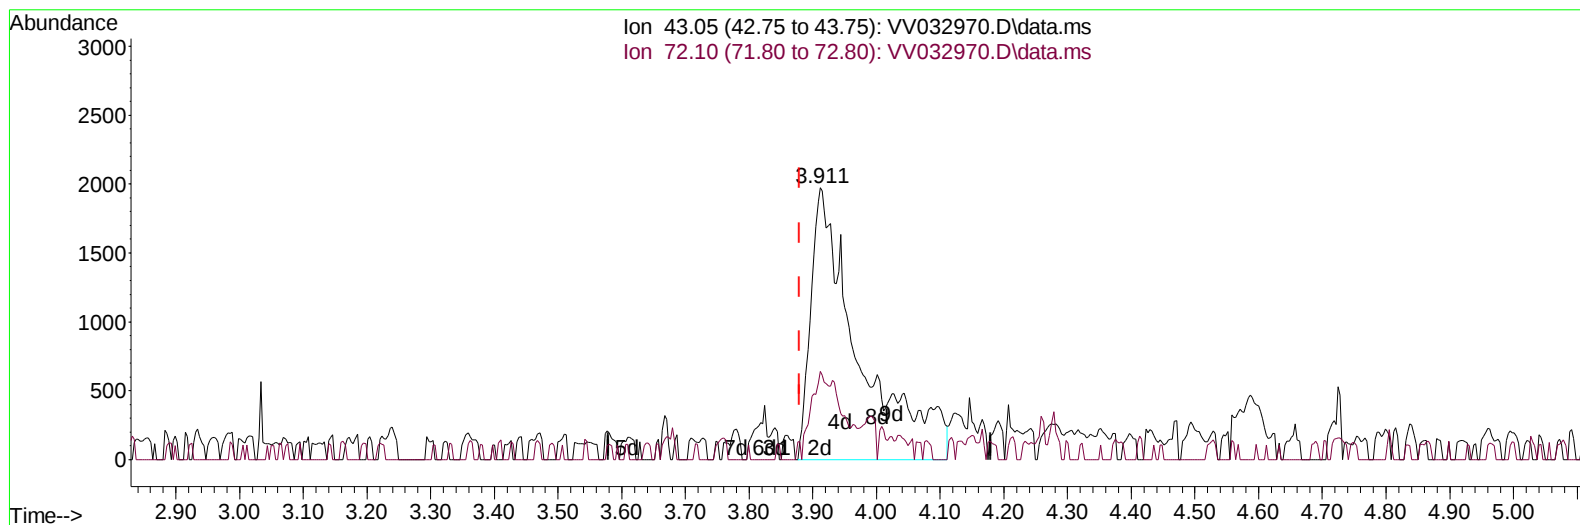

TIC: VV032970.D\data.ms

(21) 2-Butanone (T)

3.911min (+ 0.032) 4.87 ug/L m

response 10299

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	26.70	0.48#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111723\
 Data File : VV032970.D
 Acq On : 16 Nov 2023 17:36
 Operator : SY/MD
 Sample : VSTD0.510
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5210

Manual IntegrationsAPPROVED

Quant Time: Nov 17 00:30:12 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 17 00:29:50 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/20/2023
 Supervised By :Semsettin Yesilyurt 11/20/2023

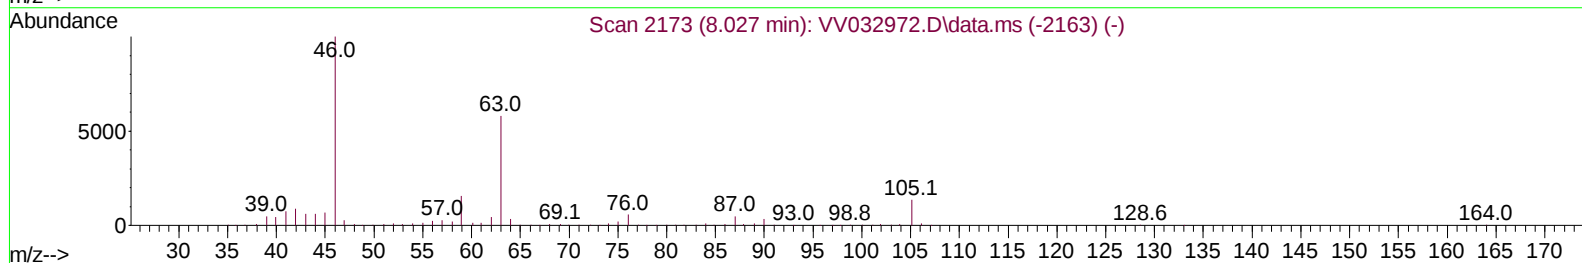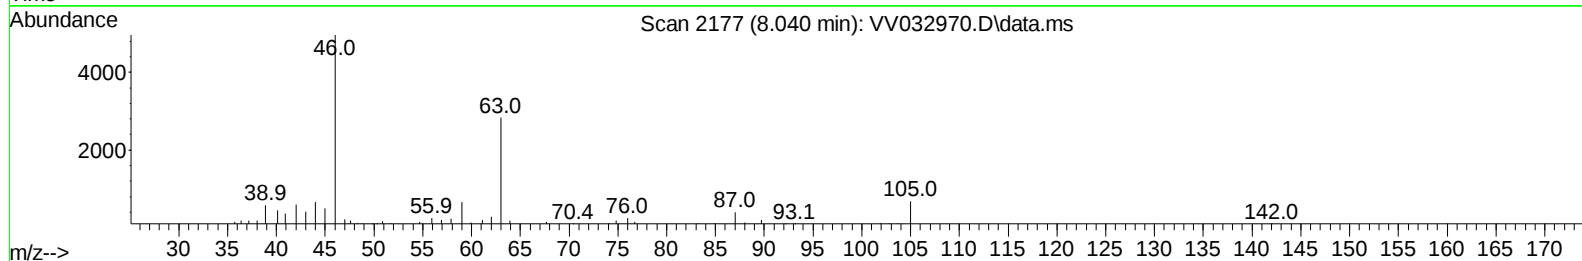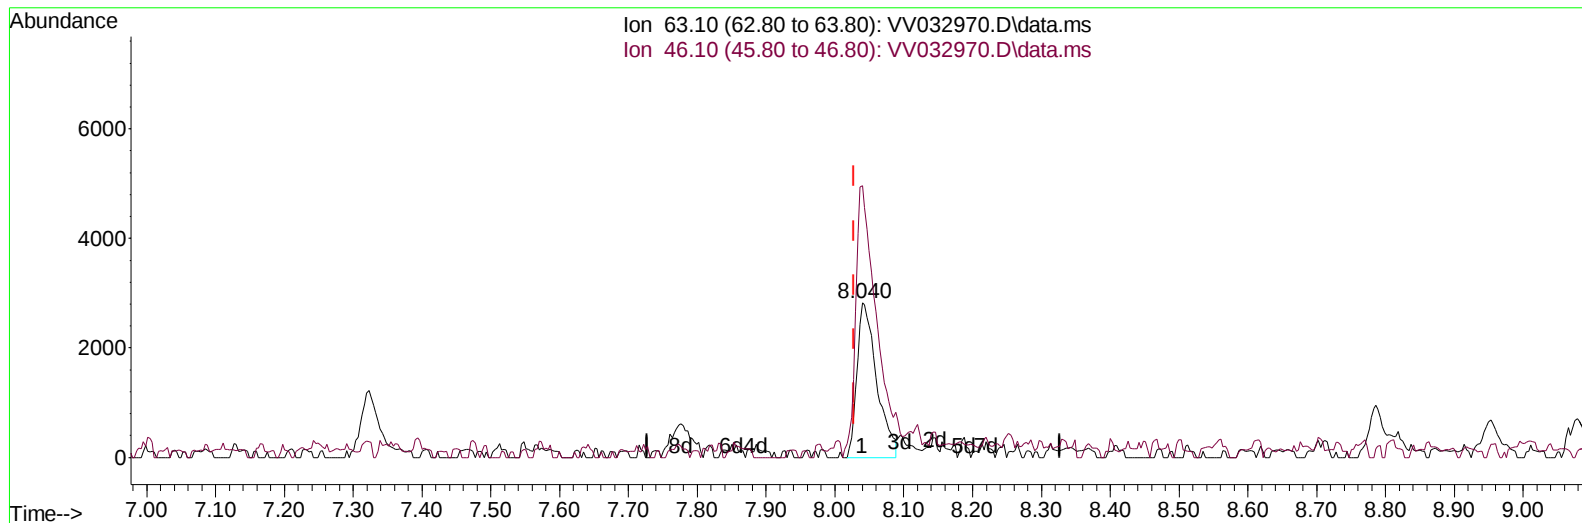

TIC: VV032970.D\data.ms

(46) 2-Hexanone-d5 (S)

8.040min (+ 0.013) 3.34 ug/L

response 5600

Ion	Exp%	Act%
63.10	100.00	100.00
46.10	177.30	188.16
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111723\
 Data File : VV032970.D
 Acq On : 16 Nov 2023 17:36
 Operator : SY/MD
 Sample : VSTD0.510
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5210

Manual IntegrationsAPPROVED

Quant Time: Nov 17 00:30:12 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 17 00:29:50 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/20/2023
 Supervised By :Semsettin Yesilyurt 11/20/2023

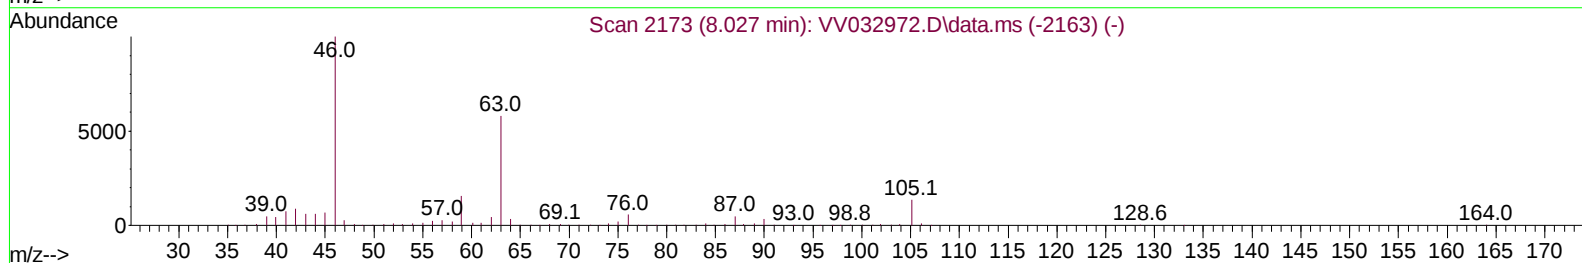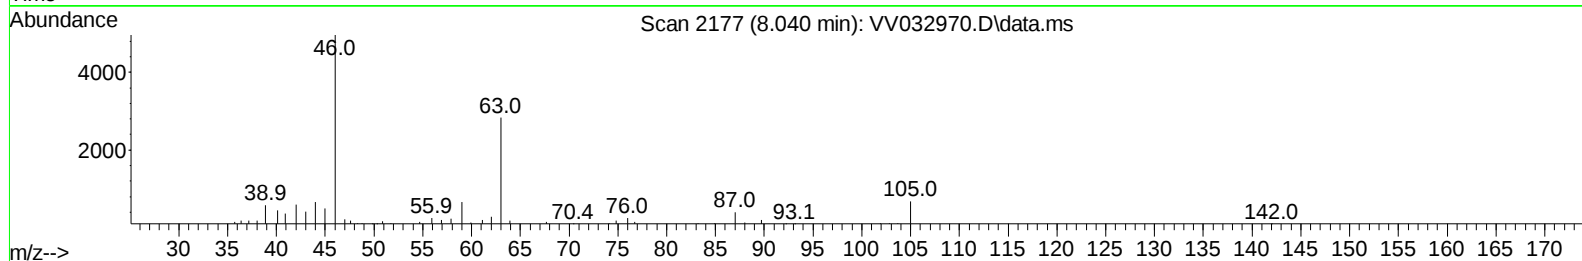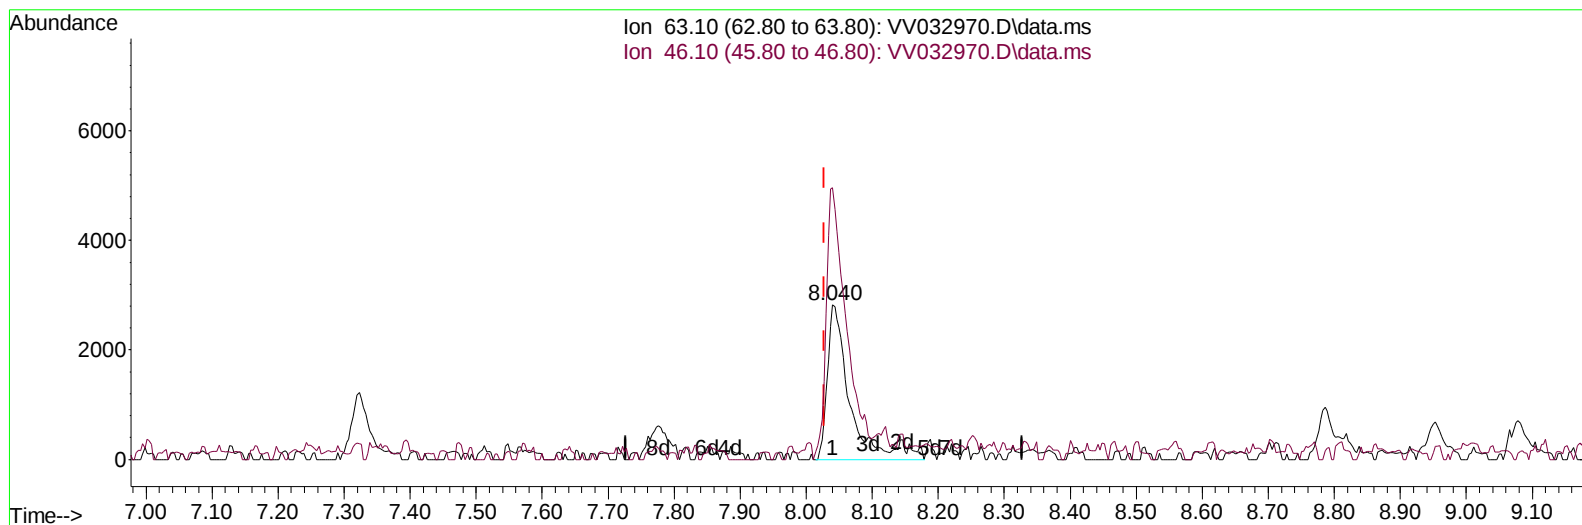

TIC: VV032970.D\data.ms

(46) 2-Hexanone-d5 (S)

8.040min (+ 0.013) 4.01 ug/L m

response 6726

Ion	Exp%	Act%
63.10	100.00	100.00
46.10	177.30	156.66
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111723\
 Data File : VV032970.D
 Acq On : 16 Nov 2023 17:36
 Operator : SY/MD
 Sample : VSTD0.510
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5210

Manual IntegrationsAPPROVED

Quant Time: Nov 17 00:30:12 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 17 00:29:50 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/20/2023
 Supervised By :Semsettin Yesilyurt 11/20/2023

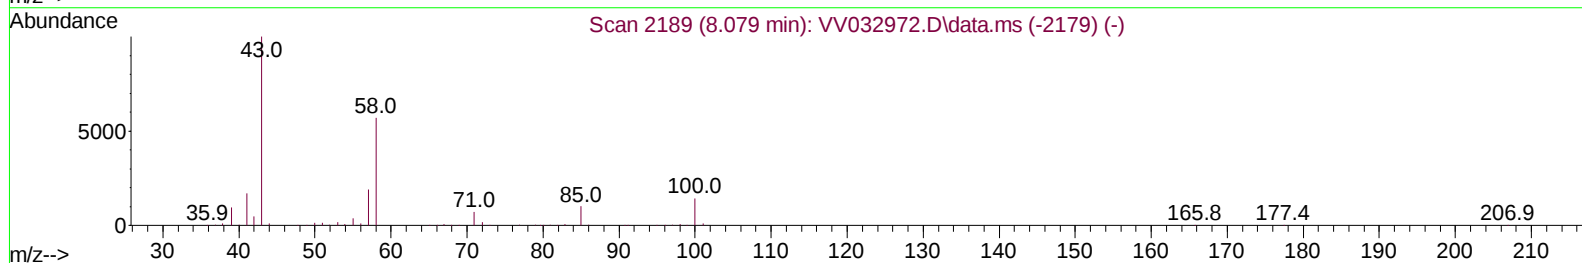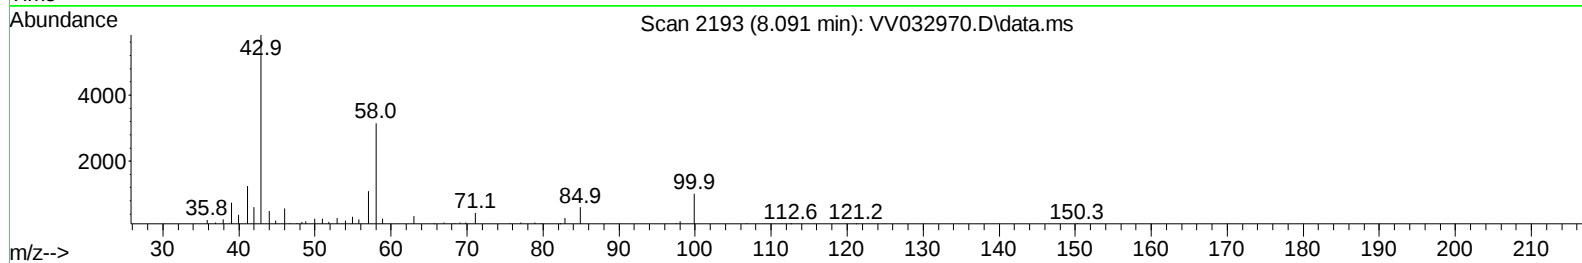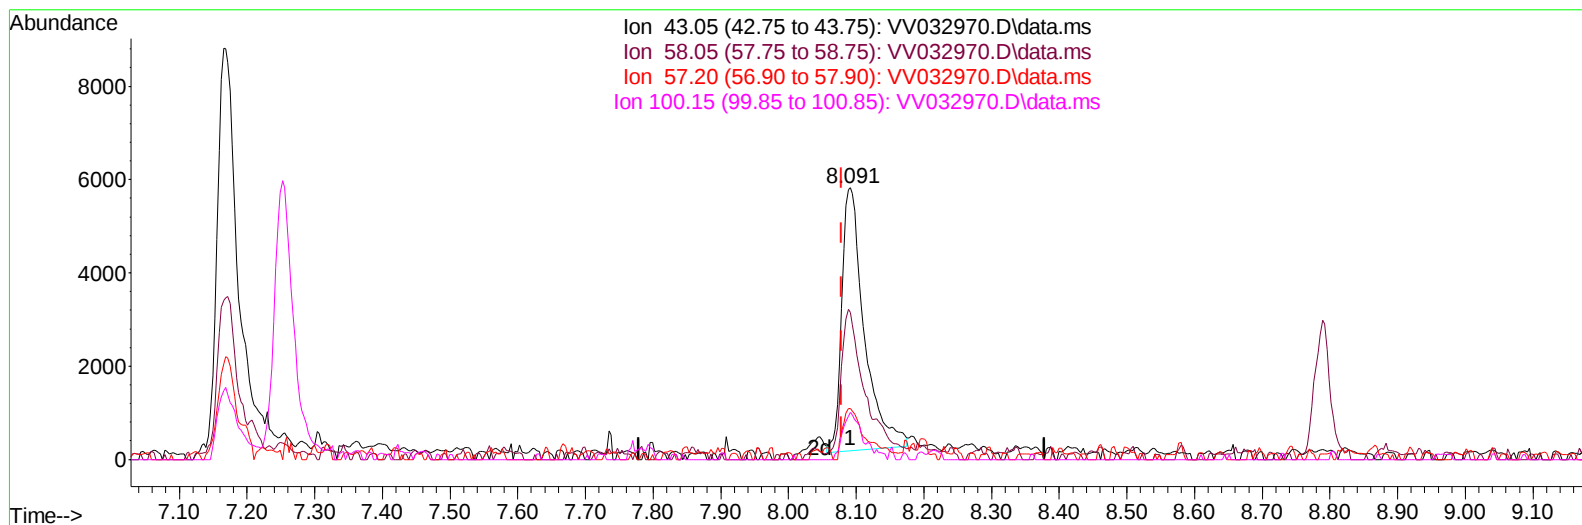

TIC: VV032970.D\data.ms

(48) 2-Hexanone (T)

8.091min (+ 0.013) 3.55 ug/L

response 13057

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	56.10	58.15
57.20	18.90	20.58
100.15	14.20	16.16




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111723\
 Data File : VV032970.D
 Acq On : 16 Nov 2023 17:36
 Operator : SY/MD
 Sample : VSTD0.510
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5210

Manual IntegrationsAPPROVED

Quant Time: Nov 17 00:30:12 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 17 00:29:50 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/20/2023
 Supervised By :Semsettin Yesilyurt 11/20/2023

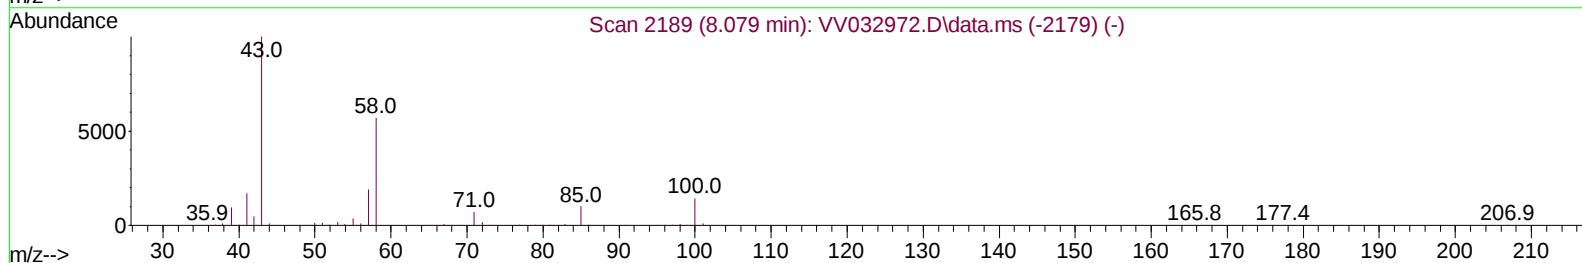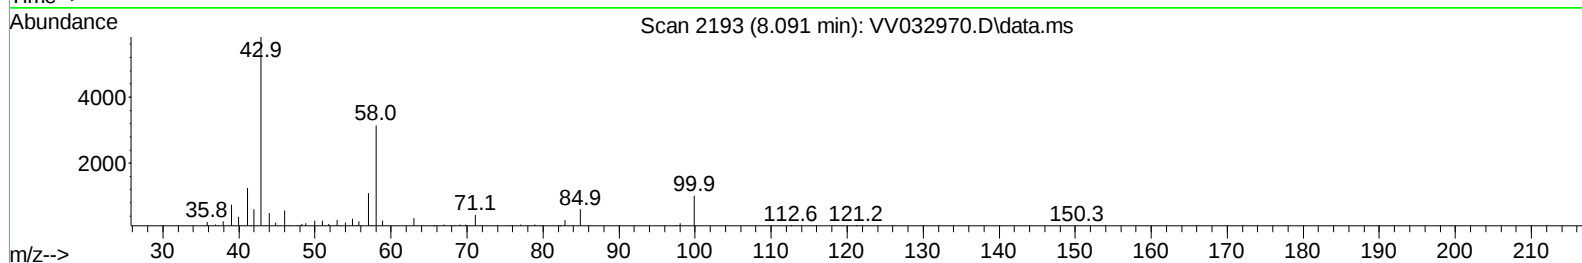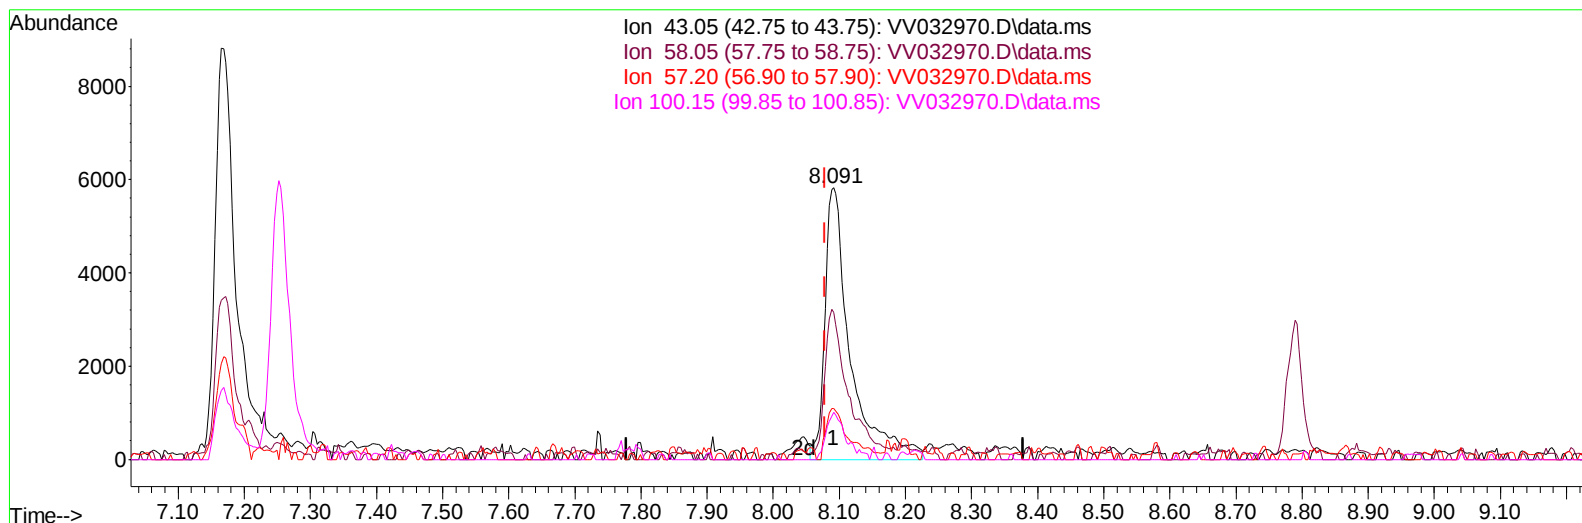

TIC: VV032970.D\data.ms

(48) 2-Hexanone (T)

8.091min (+ 0.013) 4.24 ug/L m

response 15590

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	56.10	48.70
57.20	18.90	17.24
100.15	14.20	13.53

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111723\
 Data File : VV032970.D
 Acq On : 16 Nov 2023 17:36
 Operator : SY/MD
 Sample : VSTD0.510
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5210

Manual IntegrationsAPPROVED

Quant Time: Nov 17 00:30:12 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 17 00:29:50 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/20/2023
 Supervised By :Semsettin Yesilyurt 11/20/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	167138	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	172885	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	82024	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	7188	0.505	ug/L	0.00
7) Chloroethane-d5	1.532	69	6121m	0.449	ug/L	0.00
11) 1,1-Dichloroethene-d2	2.059	65	3665	0.584	ug/L	0.00
20) 2-Butanone-d5	3.831	46	8412m	4.440	ug/L	0.03
24) Chloroform-d	4.262	84	11756	0.481	ug/L	0.01
26) 1,2-Dichloroethane-d4	4.963	65	5336	0.494	ug/L	0.02
32) Benzene-d6	4.969	84	20846	0.459	ug/L	0.00
36) 1,2-Dichloropropane-d6	5.998	67	6172	0.478	ug/L	0.00
41) Toluene-d8	7.249	98	18168	0.425	ug/L	0.00
43) trans-1,3-Dichloroprop...	7.574	79	2357	0.469	ug/L	0.02
46) 2-Hexanone-d5	8.040	63	6726m	4.011	ug/L	0.01
56) 1,1,2,2-Tetrachloroeth...	10.156	84	4719	0.496	ug/L	0.00
66) 1,2-Dichlorobenzene-d4	11.567	152	7860	0.551	ug/L	0.00
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.108	85	9568	0.524	ug/L	98
3) Chloromethane	1.217	50	9608	0.529	ug/L	89
5) Vinyl chloride	1.285	62	8545	0.495	ug/L	86
6) Bromomethane	1.487	94	6682	0.543	ug/L	95
8) Chloroethane	1.548	64	5577	0.431	ug/L	92
9) Trichlorofluoromethane	1.715	101	13809	0.516	ug/L	98
10) 1,1,2-Trichloro-1,2,2-...	2.069	101	8335	0.549	ug/L	95
12) 1,1-Dichloroethene	2.072	96	7420	0.526	ug/L	95
13) Acetone	2.121	43	10572	6.006	ug/L	94
14) Carbon disulfide	2.243	76	21241	0.521	ug/L	99
15) Methyl Acetate	2.394	43	1920	0.492	ug/L #	64
16) Methylene chloride	2.449	84	10746	0.643	ug/L	94
17) Methyl tert-butyl Ether	2.709	73	11084	0.471	ug/L	99
18) trans-1,2-Dichloroethene	2.699	96	6941	0.517	ug/L	96
19) 1,1-Dichloroethane	3.114	63	12444	0.524	ug/L	92
21) 2-Butanone	3.911	43	10299m	4.869	ug/L	
22) cis-1,2-Dichloroethene	3.825	96	6238	0.455	ug/L	92
23) Bromochloromethane	4.159	128	3082	0.490	ug/L	92
25) Chloroform	4.284	83	13858	0.529	ug/L	90
27) 1,2-Dichloroethane	5.053	62	7098	0.509	ug/L	100
29) 1,1,1-Trichloroethane	4.519	97	12441	0.521	ug/L #	85
30) Cyclohexane	4.587	56	8008	0.481	ug/L #	91
31) Carbon tetrachloride	4.735	117	9955	0.482	ug/L	91
33) Benzene	5.021	78	22299	0.437	ug/L	100
34) Trichloroethene	5.841	95	6717	0.478	ug/L	91
35) Methylcyclohexane	6.053	83	8525	0.458	ug/L	94
37) 1,2-Dichloropropane	6.101	63	6057	0.477	ug/L #	93
38) Bromodichloromethane	6.442	83	8639	0.494	ug/L	94
39) cis-1,3-Dichloropropene	6.969	75	7616	0.438	ug/L	95
40) 4-Methyl-2-pentanone	7.165	43	20050	4.005	ug/L	91
42) Toluene	7.323	91	23631	0.426	ug/L	91

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111723\
 Data File : VV032970.D
 Acq On : 16 Nov 2023 17:36
 Operator : SY/MD
 Sample : VSTD0.510
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5210

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 11/20/2023
 Supervised By :Semsettin Yesilyurt 11/20/2023

Quant Time: Nov 17 00:30:12 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 17 00:29:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) trans-1,3-Dichloropropene	7.596	75	5815	0.416	ug/L	88
45) 1,1,2-Trichloroethane	7.773	97	4239	0.464	ug/L	93
47) Tetrachloroethene	7.908	164	5913	0.500	ug/L	87
48) 2-Hexanone	8.091	43	15590m	4.241	ug/L	
49) Dibromochloromethane	8.181	129	5291	0.483	ug/L	99
50) 1,2-Dibromoethane	8.297	107	4282	0.490	ug/L #	99
51) Chlorobenzene	8.818	112	17915	0.481	ug/L	96
52) Ethylbenzene	8.953	91	23324	0.404	ug/L	100
53) m,p-Xylene	9.082	106	8954	0.402	ug/L	98
54) o-Xylene	9.484	106	8364	0.393	ug/L	100
55) Styrene	9.506	104	13341	0.364	ug/L	96
57) 1,1,2,2-Tetrachloroethane	10.185	83	5320	0.522	ug/L #	97
59) Bromoform	9.667	173	2473	0.478	ug/L #	89
60) Isopropylbenzene	9.869	105	21712	0.427	ug/L #	94
61) 1,2,3-Trichloropropane	10.217	75	3271	0.546	ug/L #	84
62) 1,3,5-Trimethylbenzene	10.480	105	17097	0.429	ug/L	98
63) 1,2,4-Trimethylbenzene	10.857	105	16098	0.401	ug/L	99
64) 1,3-Dichlorobenzene	11.123	146	13340	0.494	ug/L	96
65) 1,4-Dichlorobenzene	11.213	146	14323	0.520	ug/L	93
67) 1,2-Dichlorobenzene	11.583	146	11960	0.496	ug/L	100
68) 1,2-Dibromo-3-chloropr...	12.371	75	883	0.615	ug/L #	73
69) 1,3,5-Trichlorobenzene	12.586	180	10632	0.531	ug/L	95
70) 1,2,4-trichlorobenzene	13.204	180	9018	0.555	ug/L	91
71) Naphthalene	13.445	128	10602	0.469	ug/L #	93
72) 1,2,3-Trichlorobenzene	13.686	180	6995	0.494	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5210

Reviewed By :Mahesh Dadoda 11/20/2023
Supervised By :Semsettin Yesilyurt 11/20/2023

Reviewed By :Mahesh Dadoda 11/20/2023
Supervised By :Semsettin Yesilyurt 11/20/2023

