

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111723\
 Data File : VV032985.D
 Acq On : 17 Nov 2023 04:34
 Operator : SY/MD
 Sample : 05341-19
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QJ7

Quant Time: Nov 17 04:59:25 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 17 00:51:54 2023
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.535	114	200324	5.000	ug/L	0.00
28) Chlorobenzene-d5		8.786	117	202136	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.188	152	86013	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.278	65	100728	5.907	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	118.200%	
7) Chloroethane-d5		1.532	69	82463	5.045	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.800%	
11) 1,1-Dichloroethene-d2		2.059	65	42381	5.637	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	112.800%	
20) 2-Butanone-d5		3.793	46	114424	50.370	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.740%	
24) Chloroform-d		4.249	84	146094	4.983	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.600%	
26) 1,2-Dichloroethane-d4		4.947	65	64875	5.012	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.200%	
32) Benzene-d6		4.960	84	280502	5.278	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.600%	
36) 1,2-Dichloropropane-d6		5.989	67	83078	5.507	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	110.200%	
41) Toluene-d8		7.246	98	233960	4.680	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.600%	
43) trans-1,3-Dichloroprop...		7.561	79	26453	4.498	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.000%	
46) 2-Hexanone-d5		8.027	63	96144	47.819	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.640%	
56) 1,1,2,2-Tetrachloroeth...		10.156	84	52931	4.757	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.200%	
66) 1,2-Dichlorobenzene-d4		11.561	152	82391	5.505	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.000%	
Target Compounds							
13) Acetone		2.121	43	3924	1.860	ug/L	100
14) Carbon disulfide		2.240	76	7769	0.159	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111723\
Data File : VV032985.D
Acq On : 17 Nov 2023 04:34
Operator : SY/MD
Sample : 05341-19
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0QJ7

Quant Time: Nov 17 04:59:25 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 17 00:51:54 2023
Response via : Initial Calibration

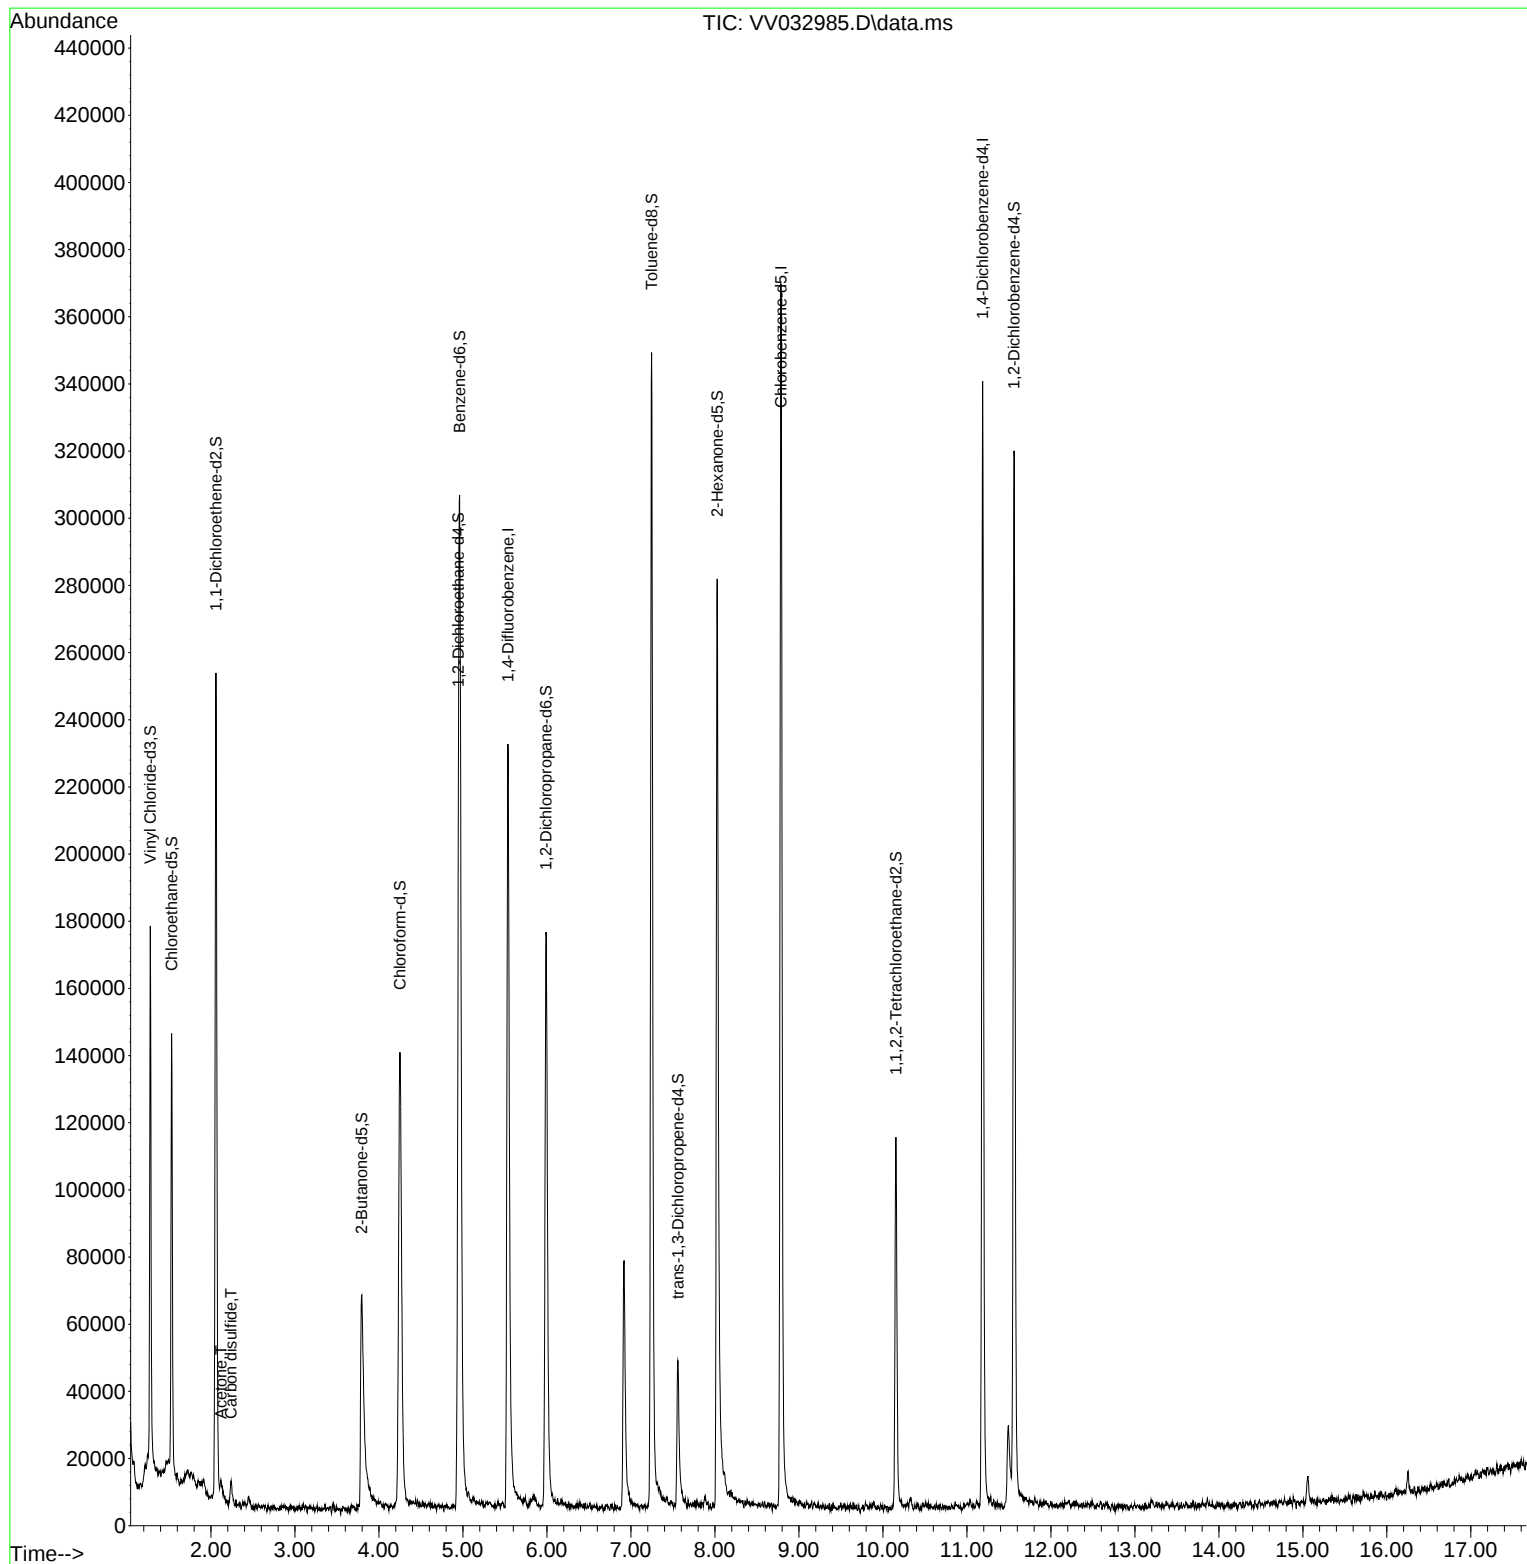

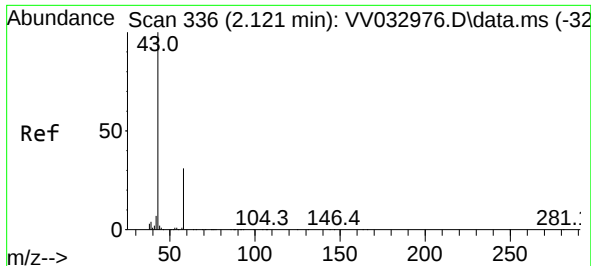

#13

Acetone

Concen: 1.860 ug/L

RT: 2.121 min Scan# 31

Delta R.T. -0.000 min

Lab File: VV032985.D

Acq: 17 Nov 2023 04:34

Instrument :

MSVOA_V

ClientSampleId :





C0QJ7

Tgt Ion: 43 Resp: 3924

Ion Ratio Lower Upper

43 100

58 32.0 0.0 63.6

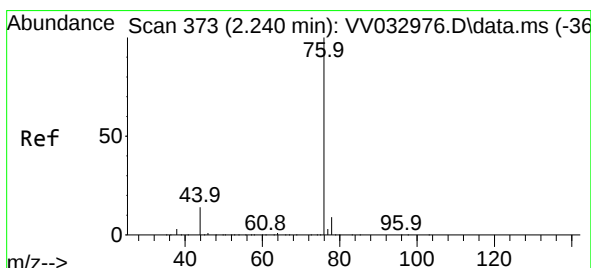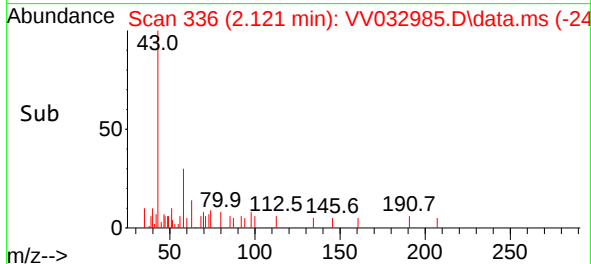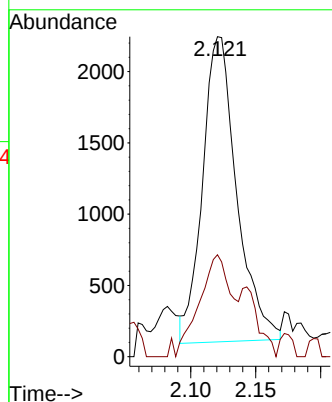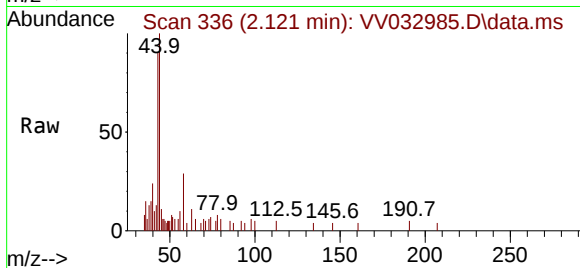

#14

Carbon disulfide

Concen: 0.159 ug/L

RT: 2.240 min Scan# 373

Delta R.T. -0.000 min

Lab File: VV032985.D

Acq: 17 Nov 2023 04:34

Tgt Ion: 76 Resp: 7769

Ion Ratio Lower Upper

76 100

78 11.2 7.7 11.5

