

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111723\
 Data File : VV032987.D
 Acq On : 17 Nov 2023 05:23
 Operator : SY/MD
 Sample : 05341-21
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QM2

Quant Time: Nov 17 06:31:28 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 17 00:51:54 2023
 Response via : Initial Calibration


Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards							
1) 1,4-Difluorobenzene		5.535	114	187201	5.000	ug/L	0.00
28) Chlorobenzene-d5		8.786	117	197302	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.188	152	83093	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.278	65	96662	6.066	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	121.400%	
7) Chloroethane-d5		1.532	69	84216	5.513	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	110.200%	
11) 1,1-Dichloroethene-d2		2.060	65	41708	5.937	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	118.800%	
20) 2-Butanone-d5		3.793	46	108116	50.929	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.860%	
24) Chloroform-d		4.249	84	142686	5.208	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.200%	
26) 1,2-Dichloroethane-d4		4.944	65	64250	5.312	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.200%	
32) Benzene-d6		4.963	84	276520	5.331	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.600%	
36) 1,2-Dichloropropane-d6		5.992	67	81920	5.563	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	111.200%	
41) Toluene-d8		7.246	98	232127	4.757	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.200%	
43) trans-1,3-Dichloroprop...		7.558	79	27632	4.814	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.200%	
46) 2-Hexanone-d5		8.024	63	89526	45.619	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.240%	
56) 1,1,2,2-Tetrachloroeth...		10.156	84	47662	4.388	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.800%	
66) 1,2-Dichlorobenzene-d4		11.561	152	83172	5.752	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	115.000%	
Target Compounds							Qvalue
13) Acetone		2.121	43	5936	3.011	ug/L	88
42) Toluene		7.326	91	10535	0.166	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111723\
Data File : VV032987.D
Acq On : 17 Nov 2023 05:23
Operator : SY/MD
Sample : 05341-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0QM2

Quant Time: Nov 17 06:31:28 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 17 00:51:54 2023
Response via : Initial Calibration

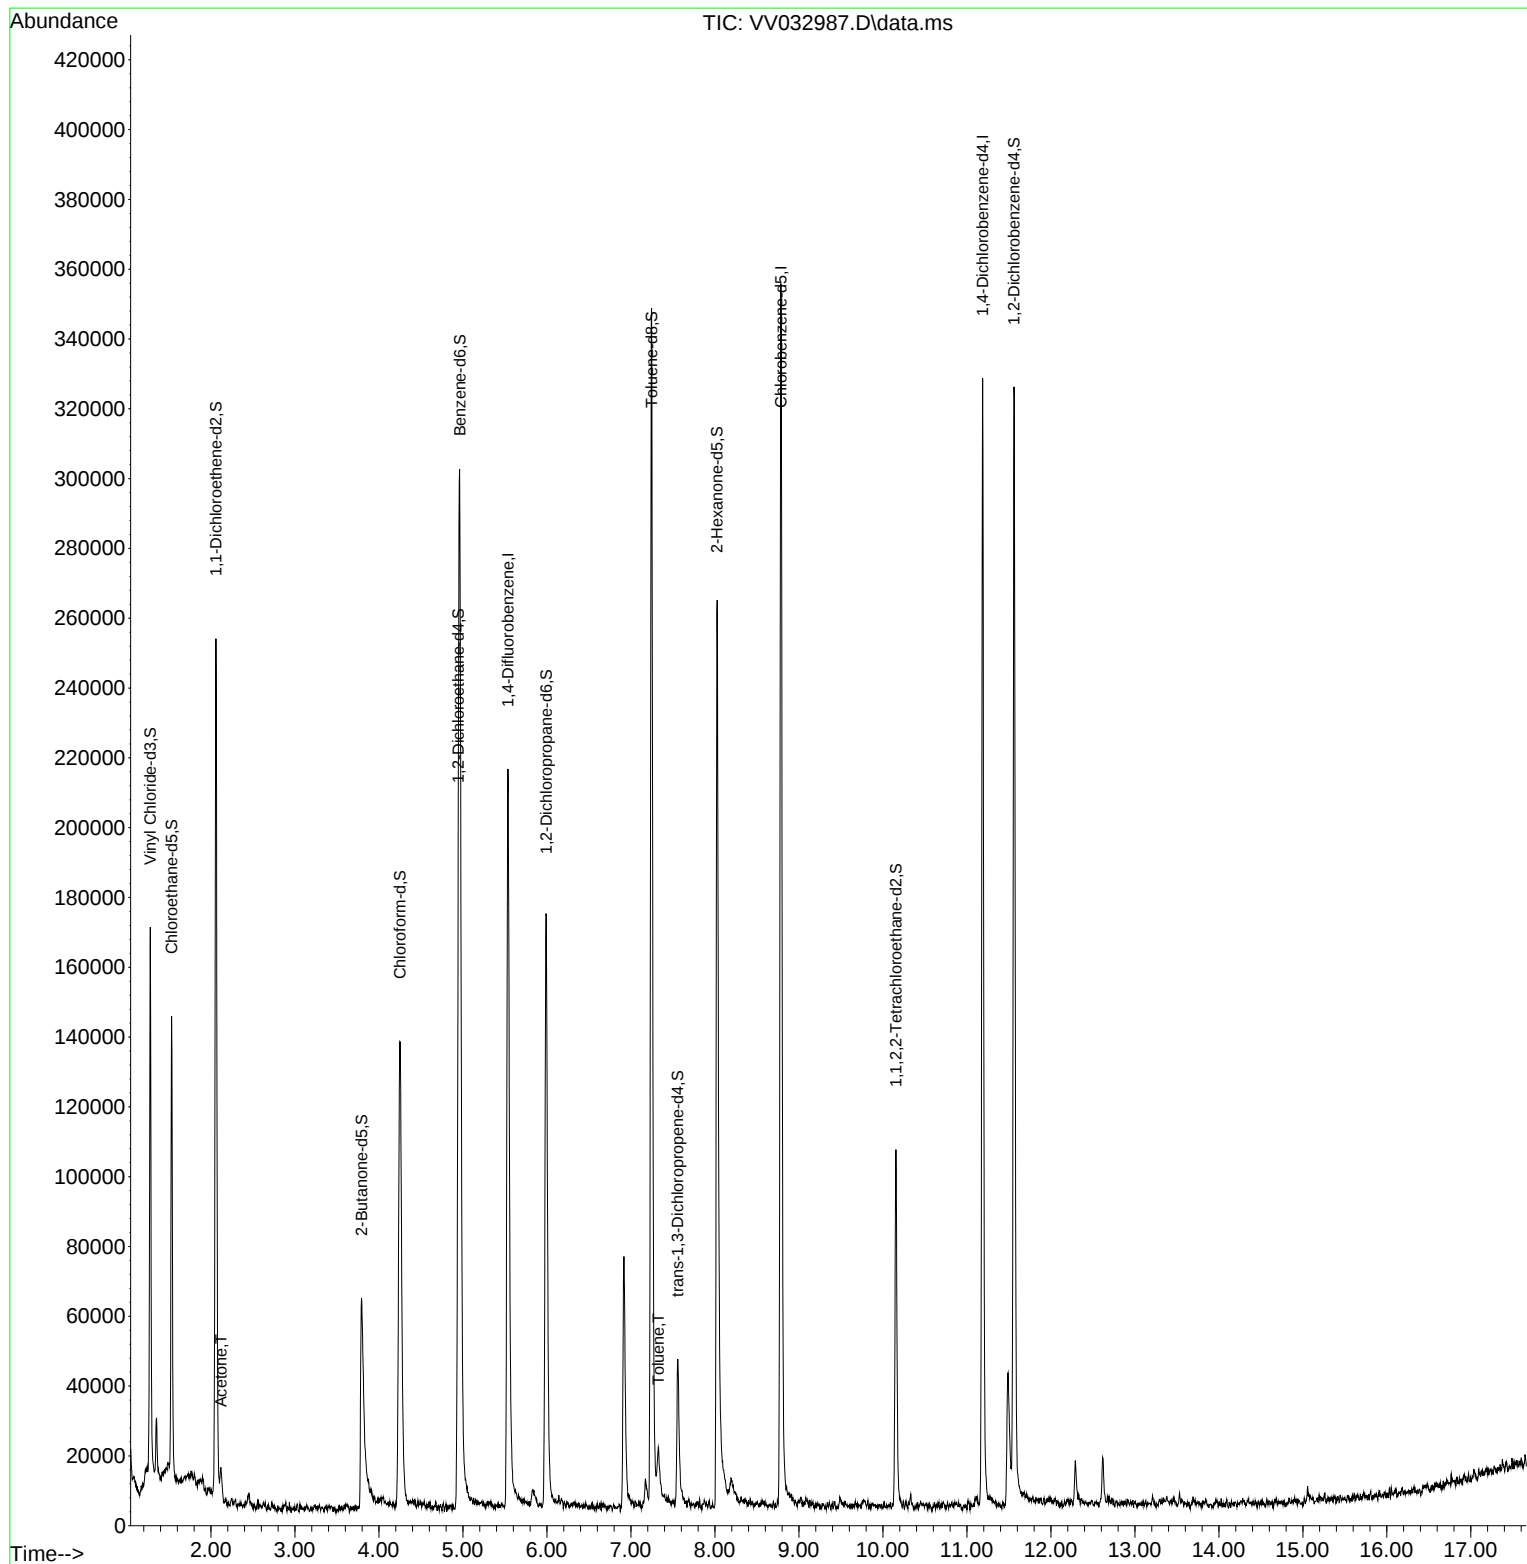

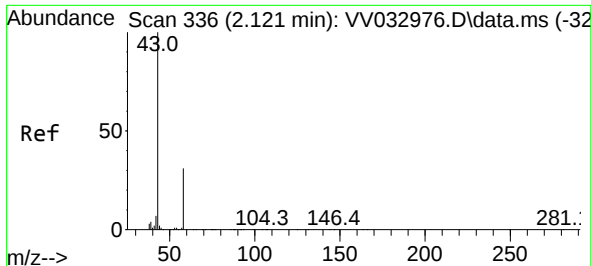

#13

Acetone

Concen: 3.011 ug/L

RT: 2.121 min Scan# 31

Delta R.T. 0.000 min

Lab File: VV032987.D

Acq: 17 Nov 2023 05:23

Instrument :

MSVOA_V

ClientSampleId :





C0QM2

Tgt Ion: 43 Resp: 5936

Ion Ratio Lower Upper

43 100

58 38.4 0.0 63.6

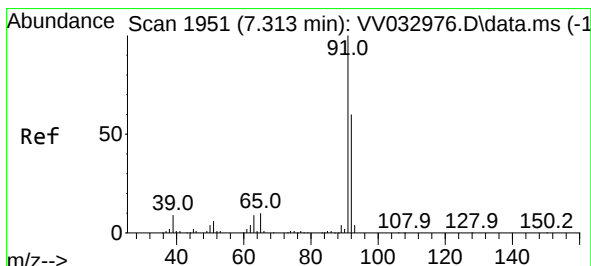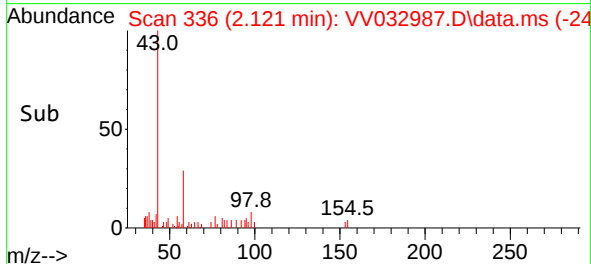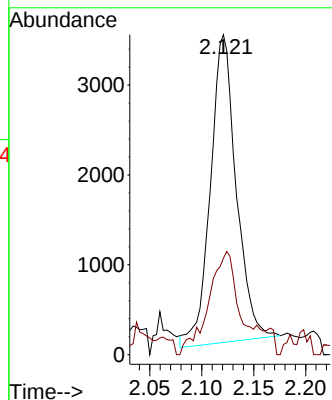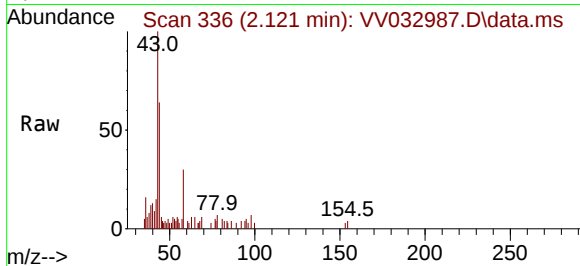

#42

Toluene

Concen: 0.166 ug/L

RT: 7.326 min Scan# 1955

Delta R.T. 0.013 min

Lab File: VV032987.D

Acq: 17 Nov 2023 05:23

Tgt Ion: 91 Resp: 10535

Ion Ratio Lower Upper

91 100

92 64.4 41.3 76.7

