

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111723\
 Data File : VW032988.D
 Acq On : 17 Nov 2023 05:47
 Operator : SY/MD
 Sample : 05389-16
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCGD7

Quant Time: Nov 17 06:31:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 17 00:51:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	177698	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	182197	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	77174	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	94140	6.224	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	124.400%
7) Chloroethane-d5	1.532	69	84563	5.832	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	116.600%
11) 1,1-Dichloroethene-d2	2.060	65	41263	6.188	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	123.800%
20) 2-Butanone-d5	3.796	46	104716	51.966	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.940%
24) Chloroform-d	4.252	84	142311	5.472	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.400%
26) 1,2-Dichloroethane-d4	4.944	65	65874	5.738	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	114.800%
32) Benzene-d6	4.963	84	270696	5.651	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	113.000%
36) 1,2-Dichloropropane-d6	5.989	67	79151	5.821	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	116.400%
41) Toluene-d8	7.246	98	223954	4.970	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.400%
43) trans-1,3-Dichloroprop...	7.558	79	25537	4.818	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.400%
46) 2-Hexanone-d5	8.027	63	86406	47.679	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.360%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	47683	4.754	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.000%
66) 1,2-Dichlorobenzene-d4	11.561	152	77477	5.769	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	115.400%
Target Compounds						
					Qvalue	
13) Acetone	2.127	43	3040	1.624	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111723\
Data File : VV032988.D
Acq On : 17 Nov 2023 05:47
Operator : SY/MD
Sample : 05389-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCGD7

Quant Time: Nov 17 06:31:44 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 17 00:51:54 2023
Response via : Initial Calibration

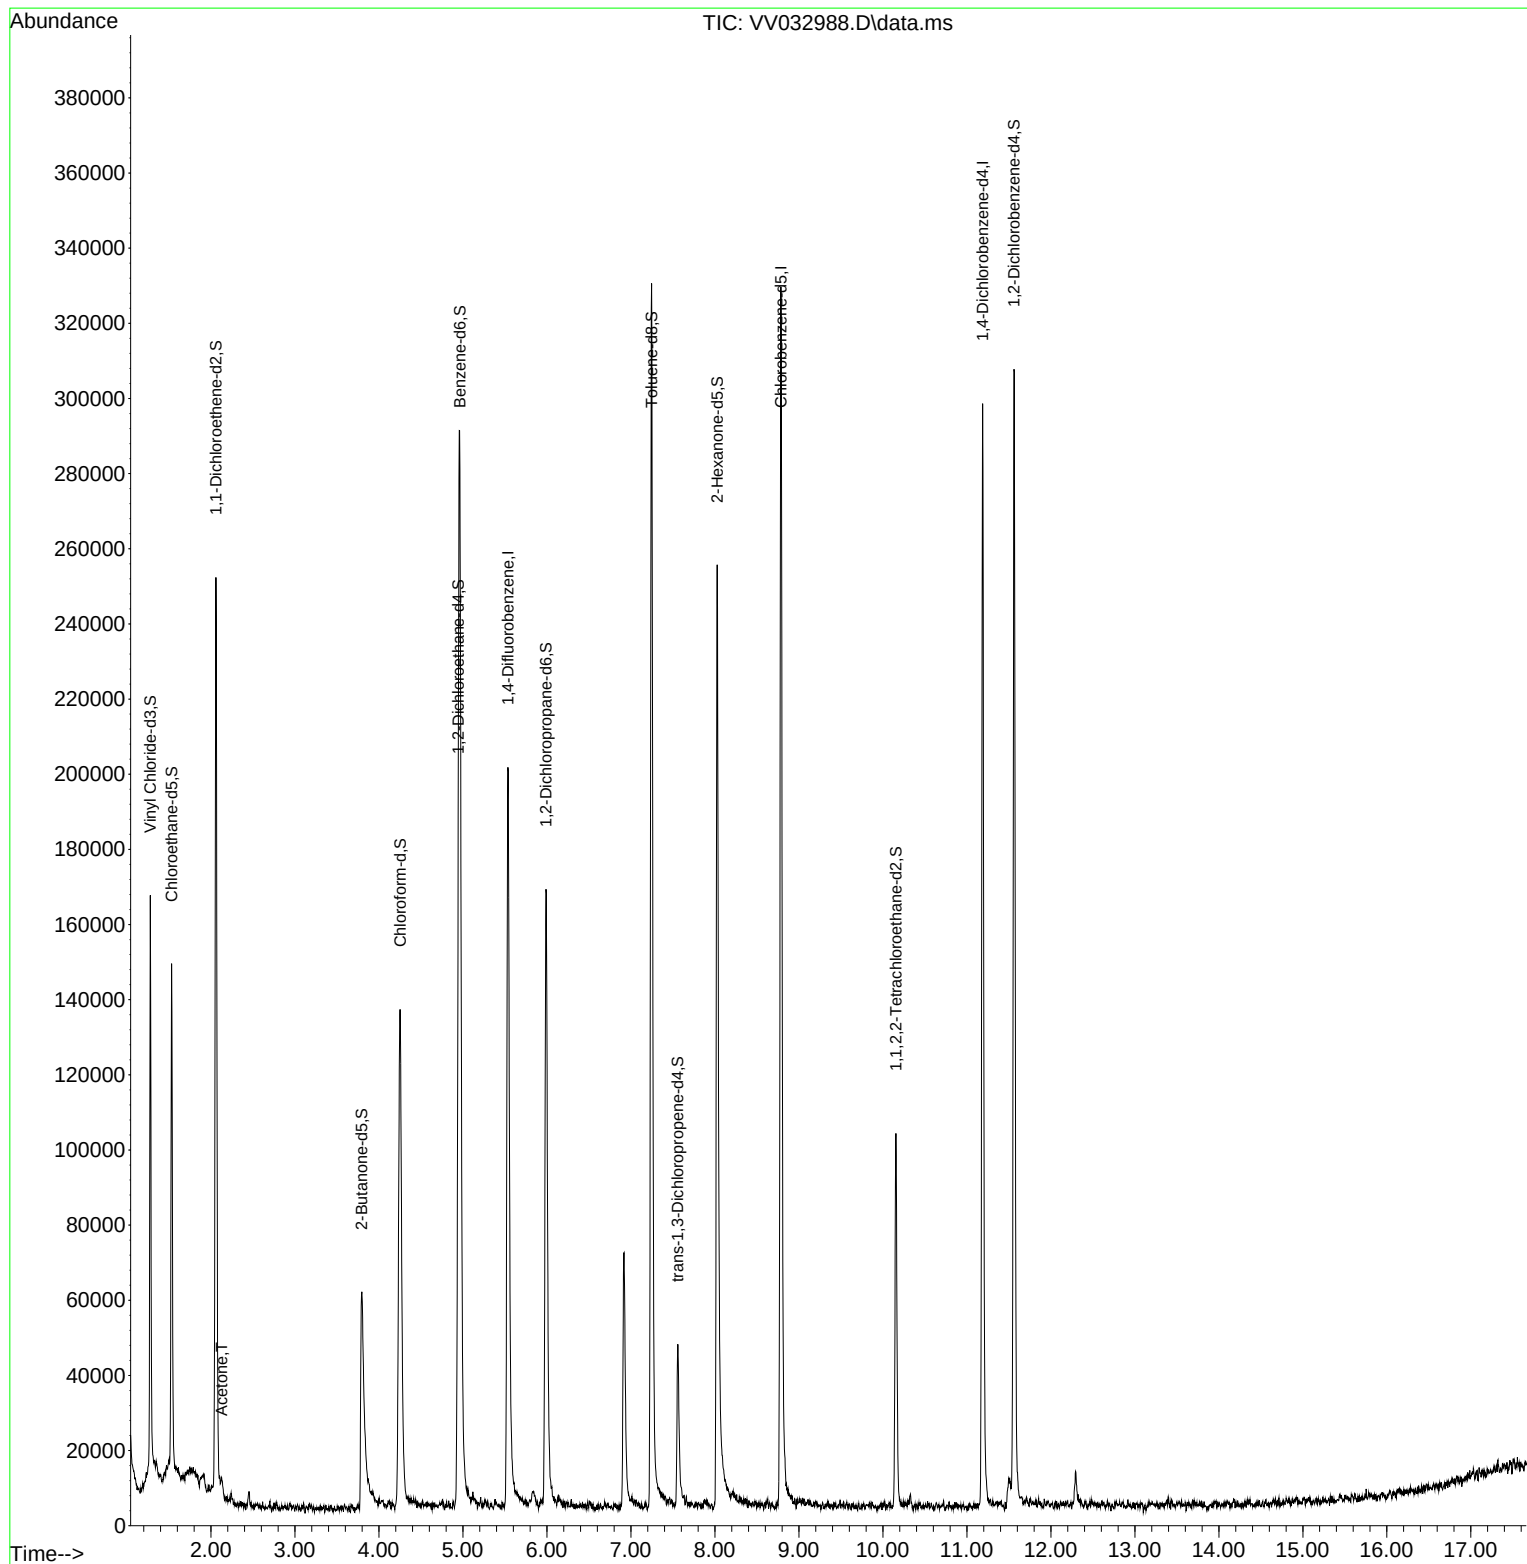

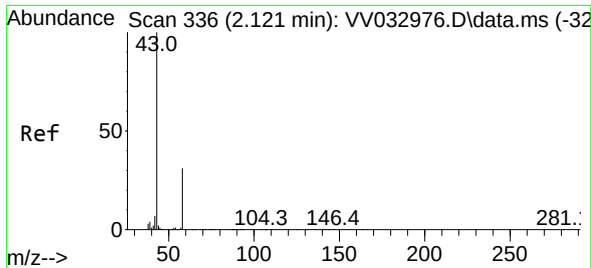

#13
 Acetone
 Concen: 1.624 ug/L
 RT: 2.127 min Scan# 31
 Delta R.T. 0.007 min
 Lab File: VV032988.D
 Acq: 17 Nov 2023 05:47

Instrument :
 MSVOA_V
 ClientSampleId :
 YCGD7

Tgt Ion: 43 Resp: 3040
 Ion Ratio Lower Upper
 43 100
 58 32.1 0.0 63.6

