

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111723\
 Data File : VW032990.D
 Acq On : 17 Nov 2023 06:35
 Operator : SY/MD
 Sample : 05389-09
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCG56

Quant Time: Nov 17 07:21:41 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 17 00:51:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	220072	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	224371	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	92623	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	106042	5.661	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	113.200%	
7) Chloroethane-d5	1.532	69	85126	4.740	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	94.800%	
11) 1,1-Dichloroethene-d2	2.060	65	39030	4.726	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	94.600%	
20) 2-Butanone-d5	3.796	46	132096	52.931	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	105.860%	
24) Chloroform-d	4.252	84	166495	5.170	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	103.400%	
26) 1,2-Dichloroethane-d4	4.944	65	71104	5.001	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	100.000%	
32) Benzene-d6	4.963	84	326064	5.528	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	110.600%	
36) 1,2-Dichloropropane-d6	5.989	67	98484	5.881	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	117.600%	
41) Toluene-d8	7.246	98	267203	4.815	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	96.200%	
43) trans-1,3-Dichloroprop...	7.558	79	30771	4.714	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	94.200%	
46) 2-Hexanone-d5	8.027	63	108543	48.636	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	97.280%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84	59265	4.798	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	96.000%	
66) 1,2-Dichlorobenzene-d4	11.561	152	90068	5.588	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	111.800%	
Target Compounds					Qvalue	
13) Acetone	2.121	43	3895	1.680	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111723\
Data File : VV032990.D
Acq On : 17 Nov 2023 06:35
Operator : SY/MD
Sample : 05389-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCG56

Quant Time: Nov 17 07:21:41 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 17 00:51:54 2023
Response via : Initial Calibration

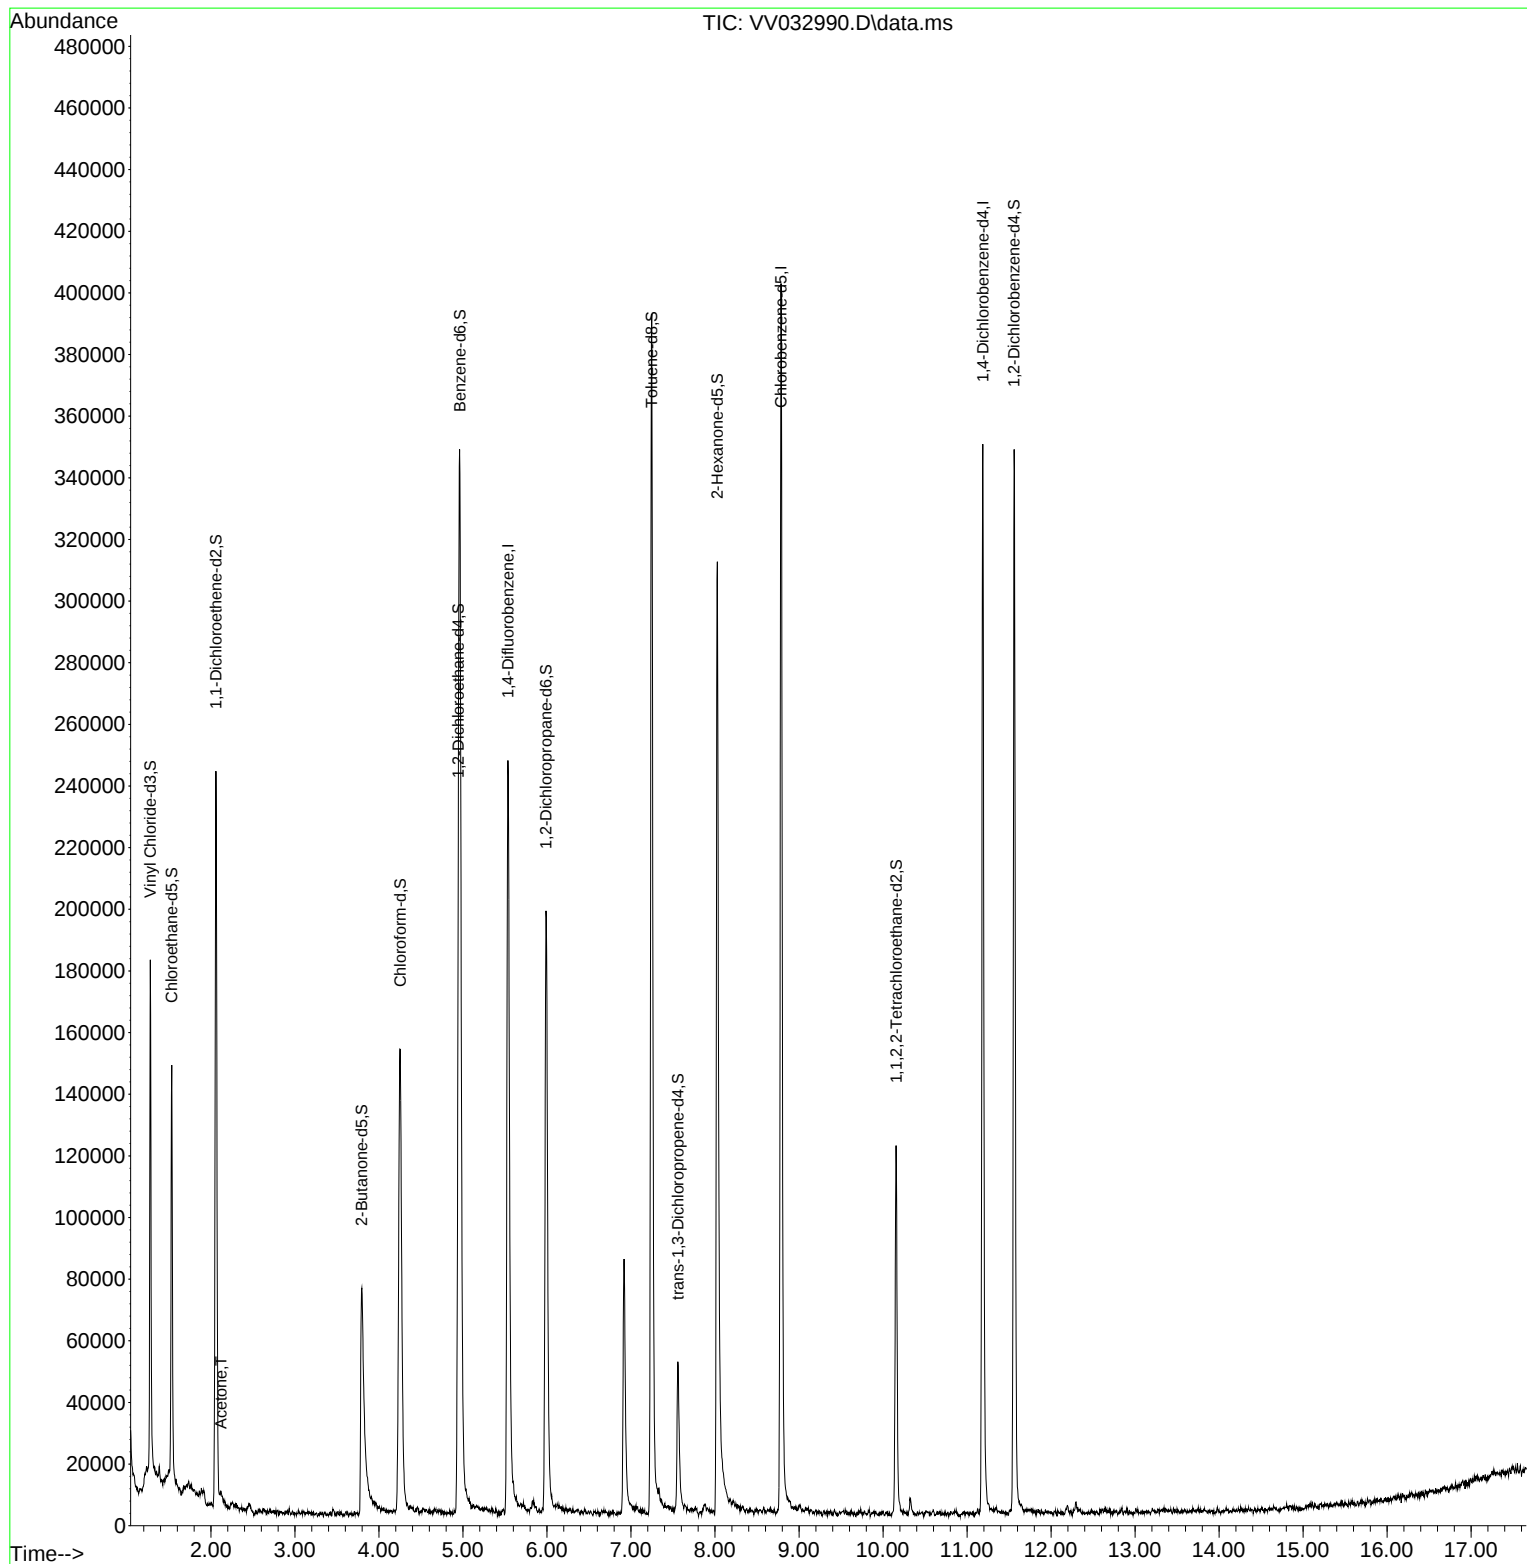

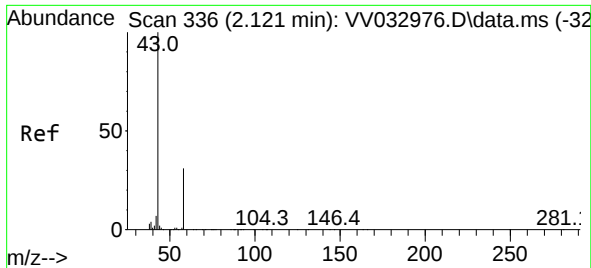

#13

Acetone

Concen: 1.680 ug/L

RT: 2.121 min Scan# 31

Delta R.T. 0.000 min

Lab File: VV032990.D


Acq: 17 Nov 2023 06:35

Instrument :

MSVOA_V

ClientSampleId :

YCG56

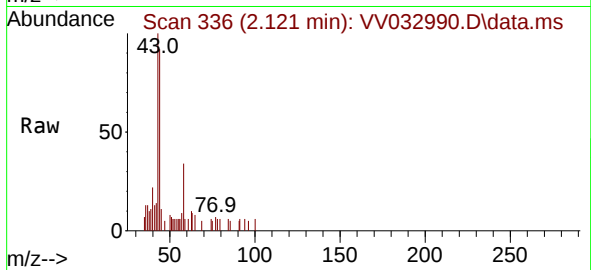

Tgt Ion: 43 Resp: 3895

Ion Ratio Lower Upper

43 100

58 35.2 0.0 63.6

