

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111723\
 Data File : VW032996.D
 Acq On : 17 Nov 2023 08:59
 Operator : SY/MD
 Sample : 05333-21
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCG64

Quant Time: Nov 17 22:38:36 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 17 00:51:54 2023
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.535	114	214432	5.000	ug/L	0.00
28) Chlorobenzene-d5		8.786	117	216203	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.188	152	92872	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.278	65	92372	5.061	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.200%	
7) Chloroethane-d5		1.532	69	67519	3.859	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	77.200%	
11) 1,1-Dichloroethene-d2		2.060	65	33254	4.132	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.600%	
20) 2-Butanone-d5		3.793	46	115262	47.401	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.800%	
24) Chloroform-d		4.249	84	147107	4.688	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.800%	
26) 1,2-Dichloroethane-d4		4.944	65	65956	4.761	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.200%	
32) Benzene-d6		4.963	84	291238	5.124	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.400%	
36) 1,2-Dichloropropane-d6		5.992	67	87006	5.392	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.800%	
41) Toluene-d8		7.246	98	235928	4.412	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.200%	
43) trans-1,3-Dichloroprop...		7.561	79	25924	4.122	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.400%	
46) 2-Hexanone-d5		8.024	63	98961	46.018	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.040%	
56) 1,1,2,2-Tetrachloroeth...		10.156	84	55113	4.630	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.600%	
66) 1,2-Dichlorobenzene-d4		11.561	152	79513	4.920	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.400%	
Target Compounds							
13) Acetone		2.118	43	5484	2.428	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111723\
Data File : VV032996.D
Acq On : 17 Nov 2023 08:59
Operator : SY/MD
Sample : 05333-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCG64

Quant Time: Nov 17 22:38:36 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 17 00:51:54 2023
Response via : Initial Calibration

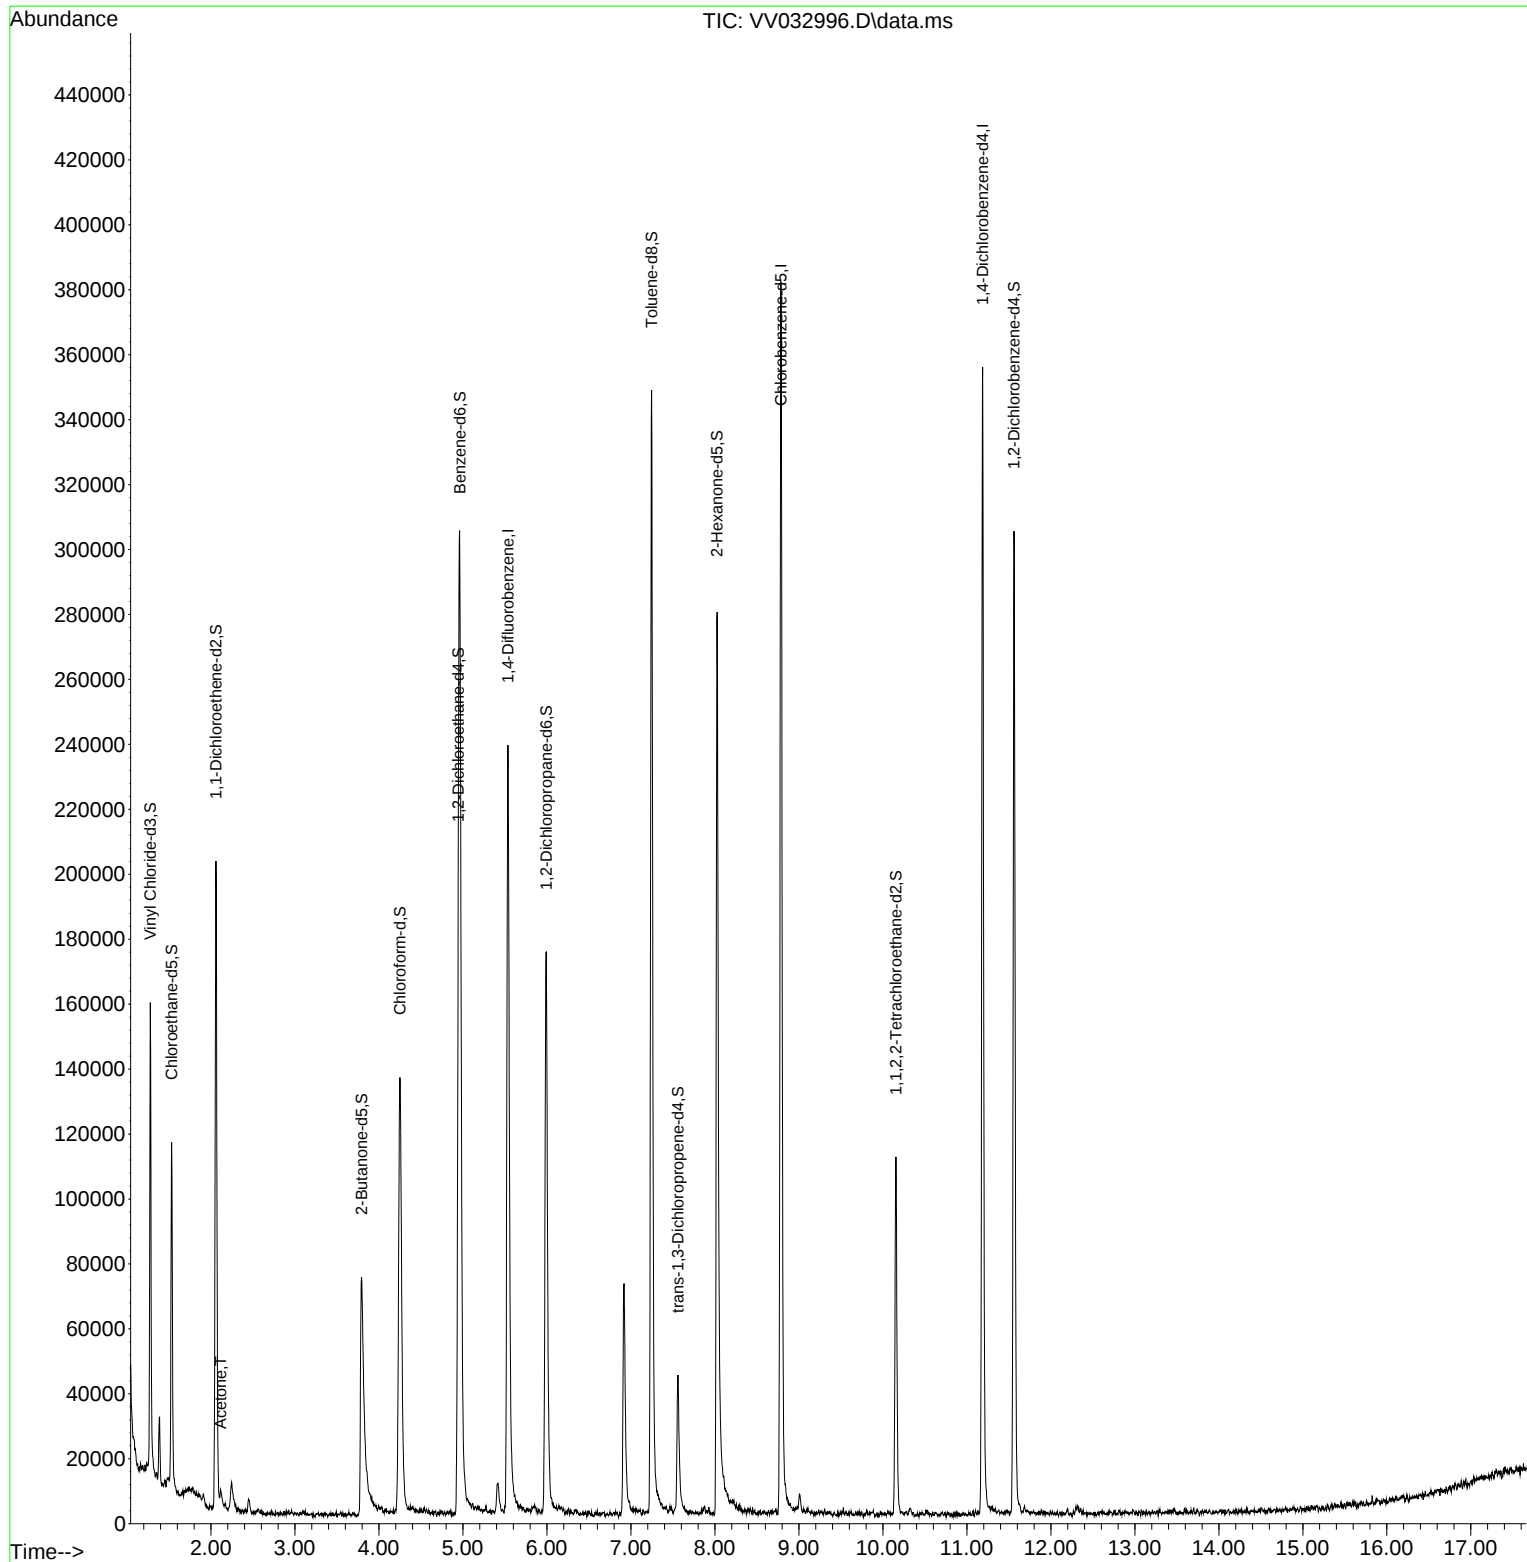

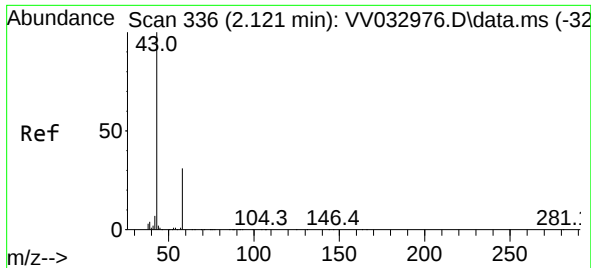

#13

Acetone

Concen: 2.428 ug/L

RT: 2.118 min Scan# 31

Delta R.T. -0.003 min

Lab File: VV032996.D

Acq: 17 Nov 2023 08:59

Instrument :

MSVOA_V

ClientSampleId :

YCG64

Tgt Ion: 43 Resp: 5484

Ion Ratio Lower Upper

43 100

58 34.3 0.0 63.6

