

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111723\
 Data File : VW032997.D
 Acq On : 17 Nov 2023 09:23
 Operator : SY/MD
 Sample : 05333-22
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCG66

Quant Time: Nov 17 22:38:51 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 17 00:51:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	208026	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	216116	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	89756	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	101348	5.724	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	114.400%	
7) Chloroethane-d5	1.532	69	73212	4.313	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	86.200%	
11) 1,1-Dichloroethene-d2	2.060	65	37136	4.757	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	95.200%	
20) 2-Butanone-d5	3.789	46	136947	58.053	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	116.100%	
24) Chloroform-d	4.253	84	161204	5.295	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	106.000%	
26) 1,2-Dichloroethane-d4	4.944	65	68391	5.089	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	101.800%	
32) Benzene-d6	4.963	84	313497	5.518	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	110.400%	
36) 1,2-Dichloropropane-d6	5.989	67	93937	5.824	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	116.400%	
41) Toluene-d8	7.246	98	251590	4.707	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	94.200%	
43) trans-1,3-Dichloroprop...	7.558	79	28366	4.512	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	90.200%	
46) 2-Hexanone-d5	8.024	63	108724	50.578	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	101.160%	
56) 1,1,2,2-Tetrachloroeth...	10.153	84	59151	4.972	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	99.400%	
66) 1,2-Dichlorobenzene-d4	11.561	152	85443	5.471	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	109.400%	
Target Compounds					Qvalue	
13) Acetone	2.118	43	6883	3.141	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111723\
Data File : VV032997.D
Acq On : 17 Nov 2023 09:23
Operator : SY/MD
Sample : 05333-22
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCG66

Quant Time: Nov 17 22:38:51 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 17 00:51:54 2023
Response via : Initial Calibration

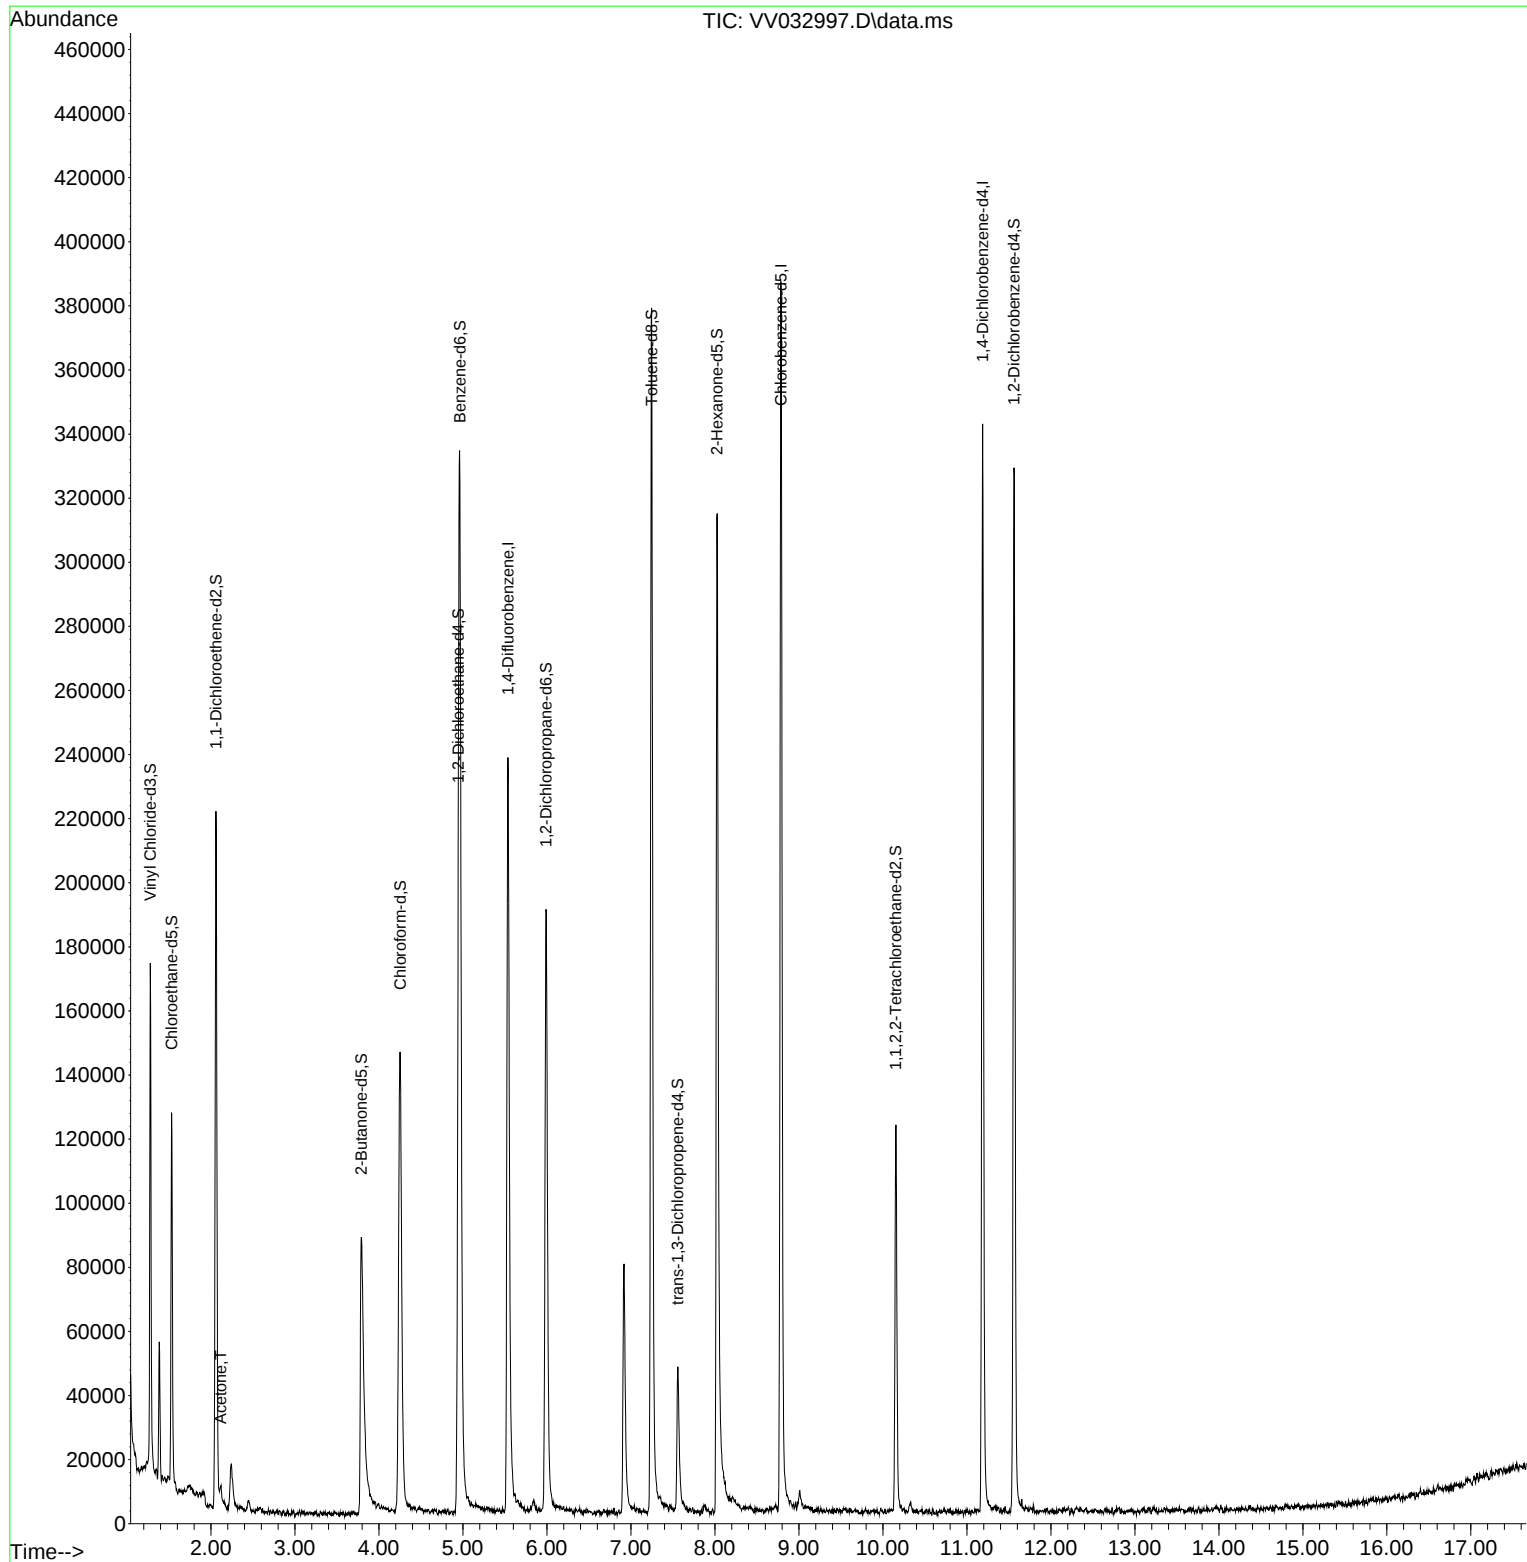

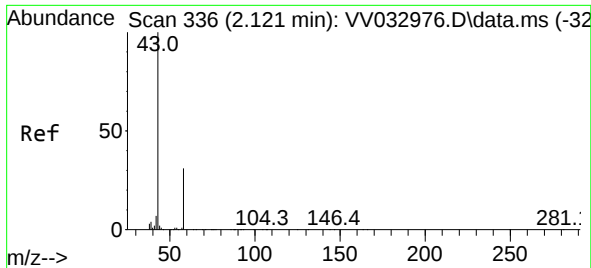

#13

Acetone

Concen: 3.141 ug/L

RT: 2.118 min Scan# 31

Delta R.T. -0.003 min

Lab File: VV032997.D

Acq: 17 Nov 2023 09:23

Instrument :

MSVOA_V

ClientSampleId :

YCG66

Tgt Ion: 43 Resp: 6883

Ion Ratio Lower Upper

43 100

58 31.3 0.0 63.6

