


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111723\
 Data File : VV032969.D
 Acq On : 16 Nov 2023 16:32
 Operator : SY/MD
 Sample : BFB232
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB232

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111723WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Nov 17 00:51:54 2023

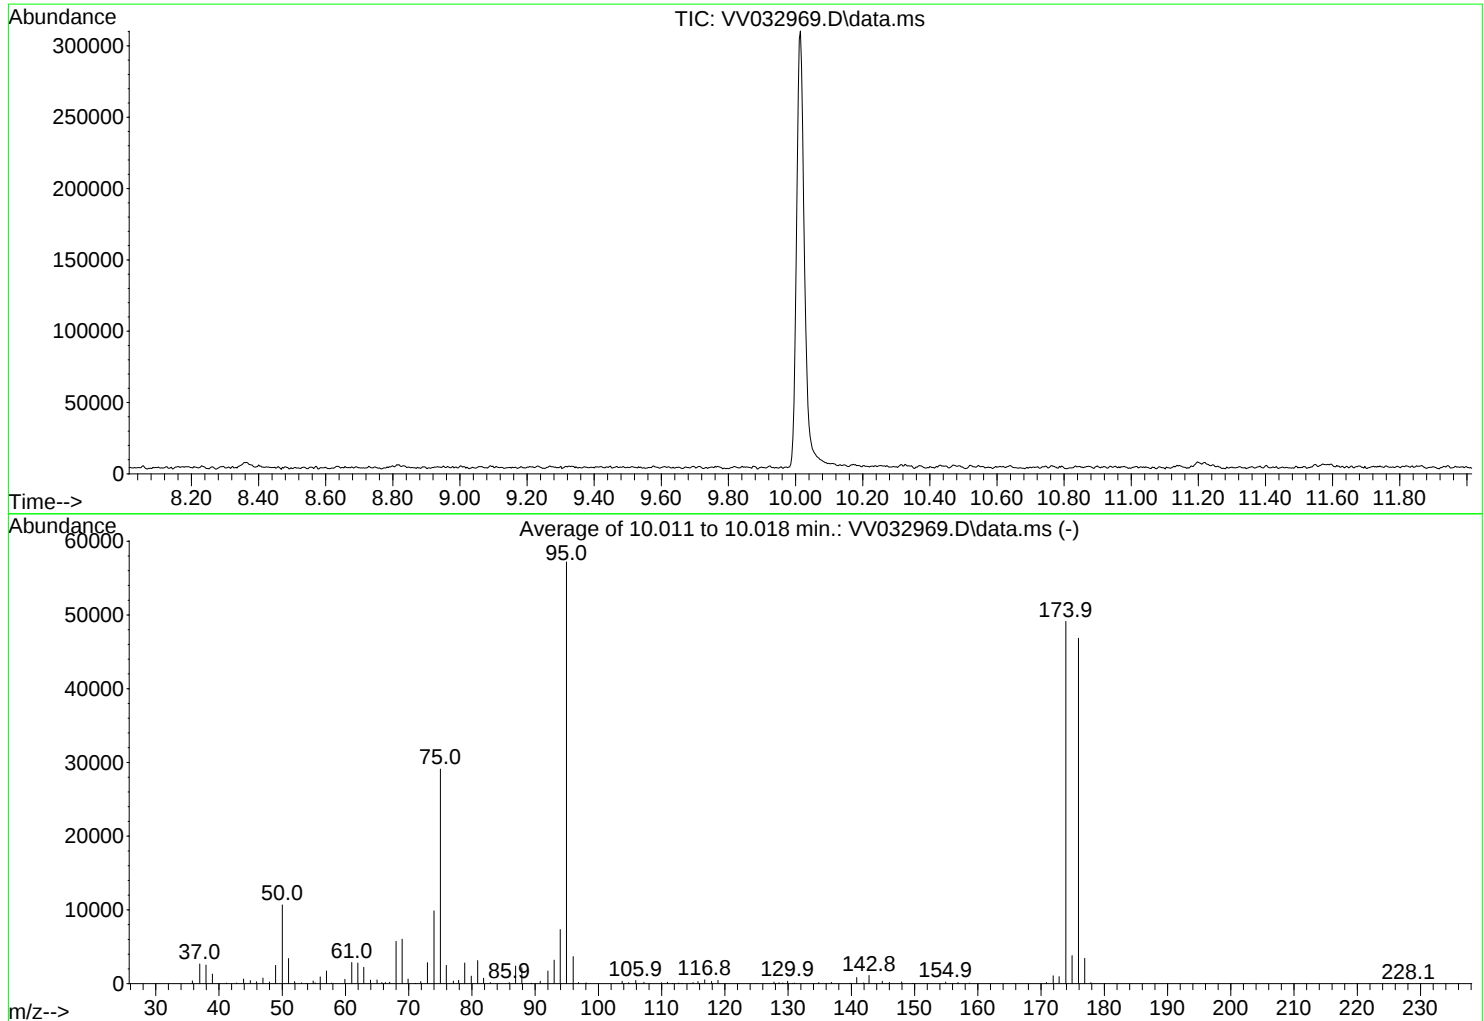

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	10680	PASS
75	95	30	80	50.9	29096	PASS
95	95	100	100	100.0	57205	PASS
96	95	5	9	6.4	3669	PASS
173	174	0.00	2	2.0	967	PASS
174	95	50	120	85.9	49125	PASS
175	174	5	9	7.7	3795	PASS
176	174	95	105	95.4	46861	PASS
177	176	5	10	7.3	3430	PASS

m/z	Abundance
35.10	156.0
35.90	211.0
36.90	138.0
38.00	154.0
38.80	139.0
40.00	271.0
40.90	171.0
41.70	207.0
42.80	110.0
43.90	450.0
44.90	202.0
46.80	151.0
47.80	120.0
48.70	103.0
49.50	113.0
51.00	107.0
51.70	112.0
52.30	106.0
53.90	117.0
58.30	124.0
59.20	110.0
61.70	157.0
62.50	101.0
62.90	101.0
64.40	109.0
65.00	104.0
68.10	115.0
69.00	112.0
72.70	108.0
74.60	122.0
75.90	103.0
94.90	126.0
97.30	135.0
124.90	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB232

m/z	Abundance
35.80	600.0
37.00	3043.0
38.00	2773.0
39.00	1631.0
40.10	311.0
40.80	136.0
41.20	146.0
41.70	109.0
42.80	212.0
43.90	1041.0
45.00	619.0
46.00	276.0
47.00	826.0
48.00	334.0
49.00	2439.0
50.00	10897.0
51.00	3760.0
52.00	291.0
53.70	162.0
55.00	270.0
55.90	1057.0
57.00	1998.0
59.90	524.0
61.00	2960.0
61.90	2953.0
63.00	2331.0
63.90	438.0
65.00	560.0
65.80	113.0
66.30	149.0
67.00	220.0
68.00	6103.0
68.90	6092.0
69.90	567.0
72.00	346.0
73.00	3007.0
74.00	10125.0
75.00	30480.0
76.00	2620.0
77.10	353.0
77.90	396.0
78.90	3030.0
79.90	1130.0
80.90	3229.0
81.90	736.0
82.90	170.0
85.90	121.0
86.90	2656.0
87.90	2124.0
89.40	114.0
90.80	319.0
92.00	1718.0
93.00	3082.0
94.00	7409.0
95.00	58224.0
96.00	3873.0
96.80	192.0
98.00	101.0
103.80	319.0
104.80	148.0
105.90	420.0
107.20	204.0
109.90	125.0
110.90	191.0
112.70	132.0
113.20	117.0
114.60	108.0
115.00	128.0
115.80	314.0
116.80	511.0
117.90	285.0
119.00	487.0
124.80	114.0
127.70	214.0
128.50	158.0
129.90	285.0
130.70	134.0
134.80	134.0
136.80	182.0
140.90	912.0
141.90	125.0
142.80	1076.0
143.70	100.0
144.80	381.0
146.00	138.0
148.10	269.0
154.90	209.0
156.90	134.0
158.60	138.0
170.90	138.0
171.90	907.0
172.80	937.0

Instrument :
MSVOA_V
ClientSampleId :
BFB232

173.90	49072.0
174.90	3811.0
175.90	46392.0
176.90	3534.0
177.90	154.0

Instrument :
MSVOA_V
ClientSampleId :
BFB232

m/z	Abundance
35.80	609.0
37.00	2920.0
37.90	2731.0
39.00	1494.0
40.10	301.0
40.80	147.0
41.20	129.0
41.80	114.0
42.80	224.0
43.90	1096.0
45.00	642.0
46.00	287.0
47.00	986.0
48.00	328.0
48.90	2503.0
50.00	11103.0
51.00	3668.0
51.90	286.0
53.00	167.0
53.70	137.0
54.80	273.0
55.10	287.0
56.00	906.0
57.00	1750.0
57.80	109.0
58.40	118.0
59.90	604.0
61.00	2918.0
62.00	2817.0
62.90	2374.0
64.00	481.0
65.00	659.0
65.70	151.0
66.30	173.0
67.00	188.0
68.00	6045.0
69.00	6230.0
69.90	638.0
71.90	264.0
72.90	2975.0
74.00	10196.0
75.00	30176.0
76.00	2646.0
77.10	357.0
77.90	499.0
78.80	2872.0
79.90	1052.0
80.90	3249.0
81.90	707.0
82.90	140.0
85.90	166.0
86.90	2429.0
87.90	2277.0
89.40	104.0
90.80	323.0
92.00	1750.0
93.00	3352.0
93.90	7613.0
95.00	59280.0
96.00	3771.0
96.90	176.0
98.00	119.0
103.70	334.0
104.80	119.0
105.90	447.0
107.20	223.0
108.10	108.0
110.00	139.0
110.90	192.0
112.70	101.0
115.00	146.0
115.80	287.0
116.80	548.0
117.90	319.0
118.90	456.0
124.90	139.0
127.70	208.0
128.50	122.0
129.10	122.0
129.90	344.0
131.00	132.0
134.80	149.0
136.90	183.0
139.80	103.0
140.80	870.0
142.00	103.0
142.80	1164.0
144.90	318.0
146.00	160.0
147.90	247.0
154.90	227.0
156.80	161.0

Instrument :
MSVOA_V
ClientSampleId :
BFB232

158.70	118.0
170.80	154.0
171.90	1108.0
172.80	1016.0
173.90	50728.0
174.90	3910.0
175.90	48464.0
176.90	3532.0
177.90	149.0

Instrument :
MSVOA_V
ClientSampleId :
BFB232

m/z	Abundance
35.80	542.0
37.00	2451.0
37.90	2500.0
39.00	1197.0
40.00	249.0
40.80	155.0
41.80	106.0
42.90	188.0
44.00	1084.0
45.00	576.0
45.90	243.0
47.00	946.0
47.70	326.0
48.90	2455.0
50.00	10040.0
51.00	3088.0
51.90	259.0
53.10	185.0
53.80	126.0
54.80	298.0
55.20	327.0
56.10	762.0
57.00	1369.0
57.80	124.0
58.40	119.0
59.90	632.0
61.00	2728.0
62.00	2629.0
63.00	2214.0
64.00	493.0
65.00	597.0
65.70	191.0
66.30	165.0
67.00	183.0
68.00	5391.0
69.00	6090.0
69.90	704.0
71.10	107.0
71.80	267.0
72.90	2574.0
74.00	9318.0
75.00	26632.0
76.00	2488.0
76.90	341.0
77.90	451.0
78.80	2513.0
79.90	861.0
80.90	2910.0
81.80	745.0
82.90	118.0
85.90	192.0
86.90	2071.0
87.90	2101.0
90.80	315.0
92.00	1664.0
93.00	3159.0
94.00	6975.0
95.00	54488.0
96.00	3364.0
96.90	110.0
98.10	125.0
103.70	355.0
104.80	124.0
105.90	406.0
107.20	170.0
109.90	131.0
110.90	174.0
111.70	119.0
114.90	152.0
115.70	260.0
116.80	512.0
117.90	295.0
118.80	457.0
124.90	126.0
127.80	202.0
128.60	111.0
129.20	160.0
129.90	335.0
131.00	147.0
134.90	176.0
136.00	127.0
136.90	179.0
139.80	126.0
140.80	723.0
142.00	116.0
142.80	1096.0
145.00	251.0
146.00	129.0
147.90	197.0
149.70	132.0
154.90	201.0
156.80	179.0

Instrument :
MSVOA_V
ClientSampleId :
BFB232

170.80	186.0
171.90	1173.0
172.90	949.0
173.90	47576.0
174.90	3665.0
175.90	45728.0
176.90	3225.0
177.80	107.0
228.10	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB232