


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV111821\  
Data File : VV023605.D  
Acq On : 18 Nov 2021 15:36  
Operator : SY/MD  
Sample : M4627-19DL 5X  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
Client Sample ID :  
H4674DL

Quant Time: Nov 19 02:14:02 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR110421WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Fri Nov 19 02:11:08 2021  
Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/19/2021  
Supervised By : Mahesh Dadoda 11/19/2021

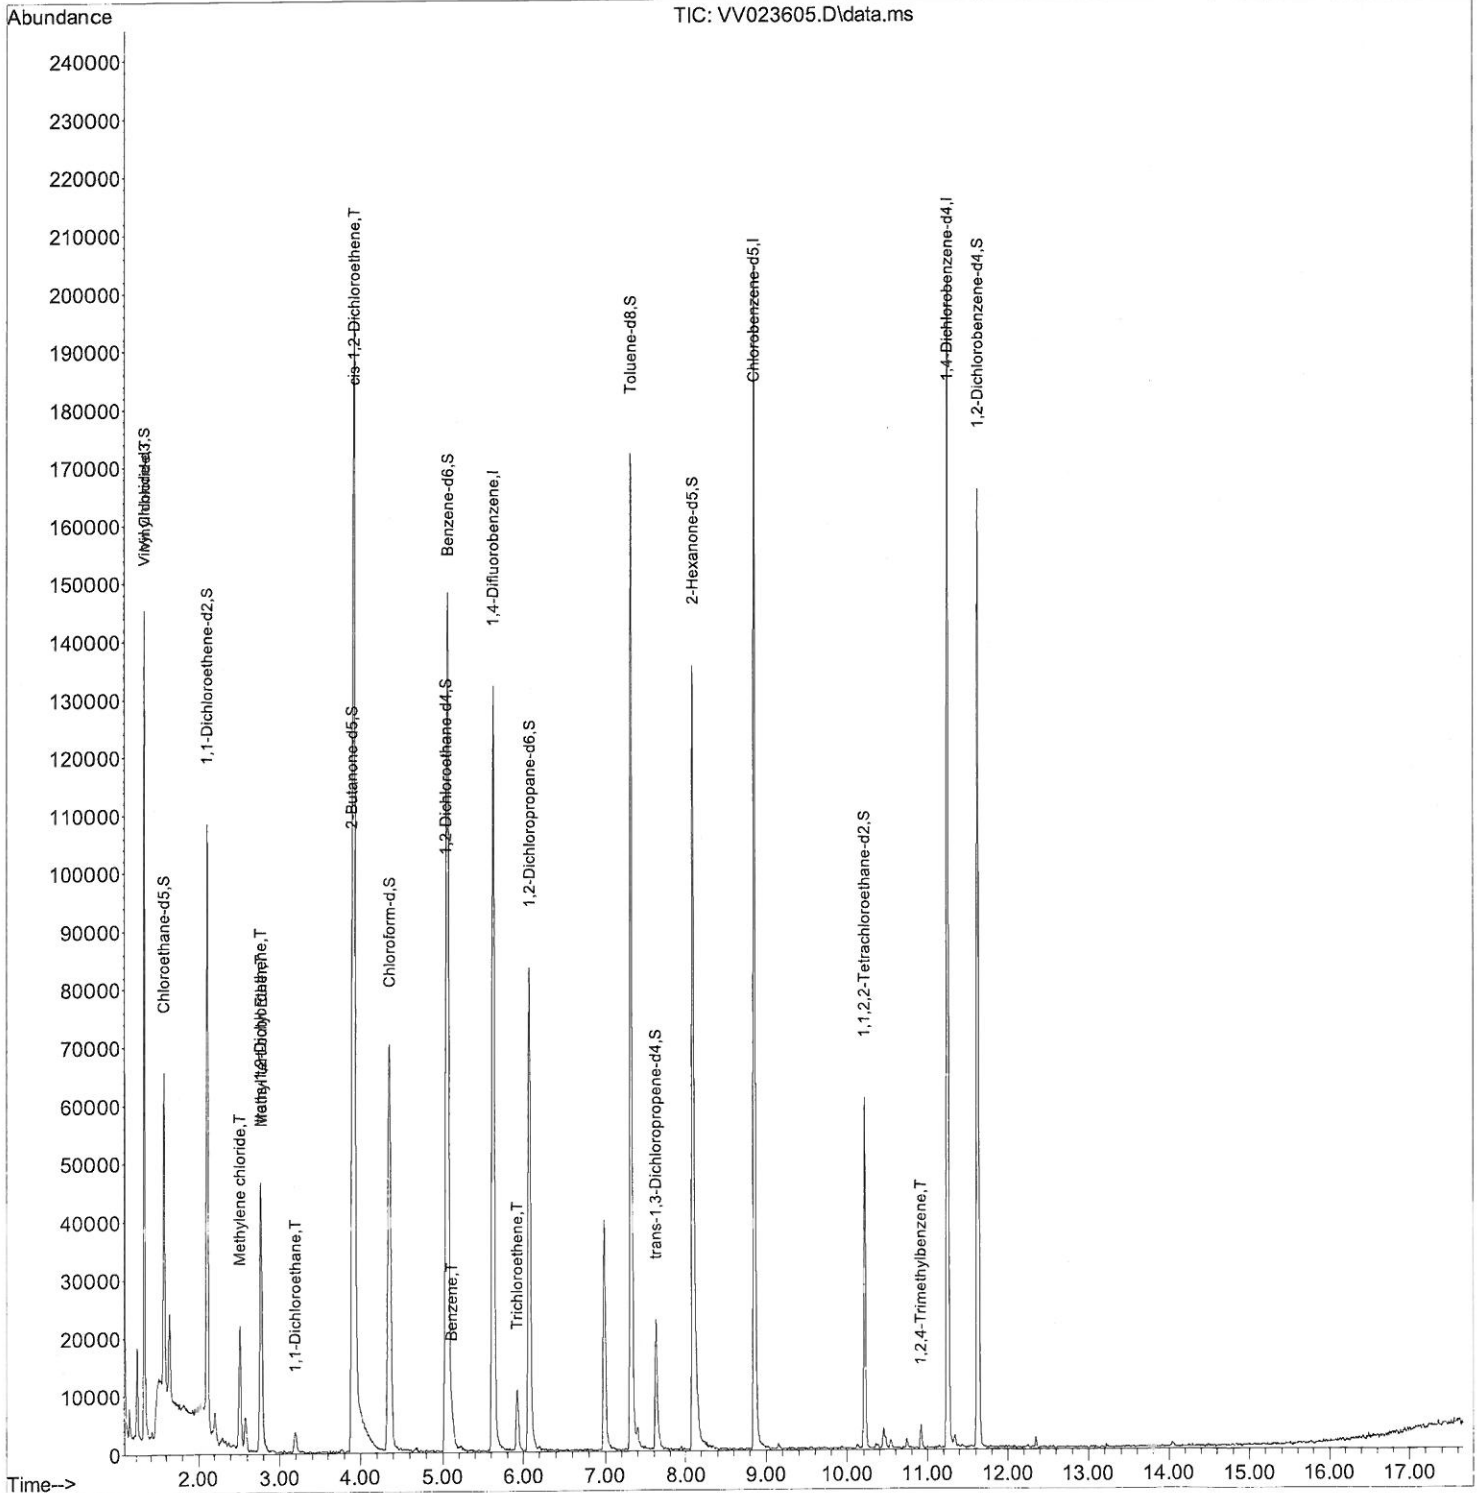

# Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV111821\  
 Data File : VV023605.D  
 Acq On : 18 Nov 2021 15:36  
 Operator : SY/MD  
 Sample : M4627-19DL 5X  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 H4674DL

Quant Time: Nov 19 02:14:02 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR110421WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Fri Nov 19 02:11:08 2021  
 Response via : Initial Calibration

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 11/19/2021  
 Supervised By :Mahesh Dadoda 11/19/2021

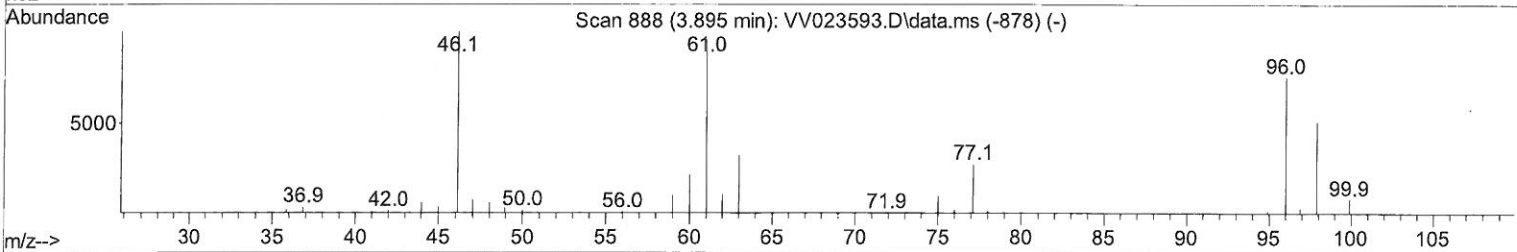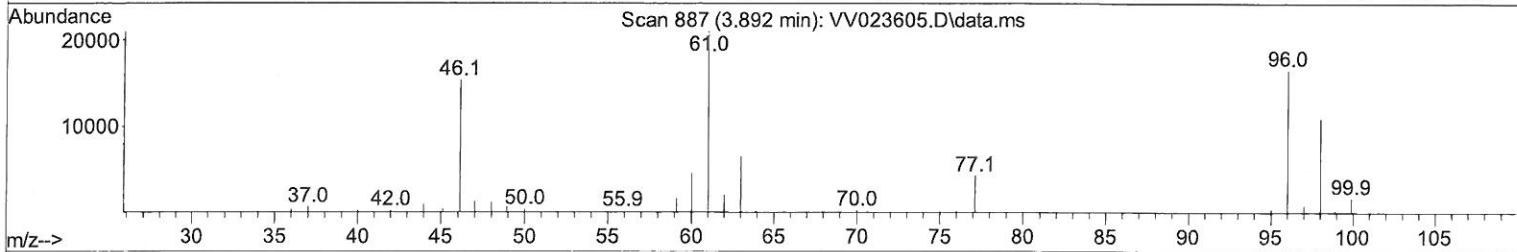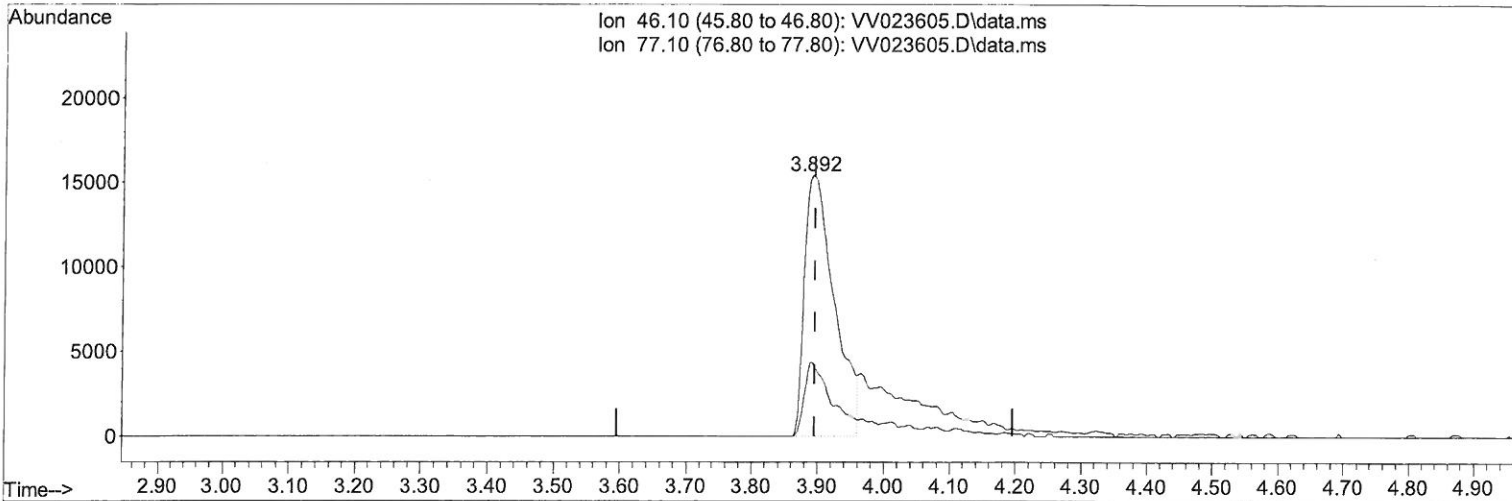

TIC: VV023605.D\data.ms

(20) 2-Butanone-d5 (S)

3.892min (-0.003) 38.16 ug/L

response 48469

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.30	29.46#
0.00	0.00	0.00
0.00	0.00	0.00

# Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV111821\  
 Data File : VV023605.D  
 Acq On : 18 Nov 2021 15:36  
 Operator : SY/MD  
 Sample : M4627-19DL 5X  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 Client Sampled :  
 H4674DL

Quant Time: Nov 19 02:14:02 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR110421WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Fri Nov 19 02:11:08 2021  
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/19/2021  
 Supervised By : Mahesh Dadoda 11/19/2021

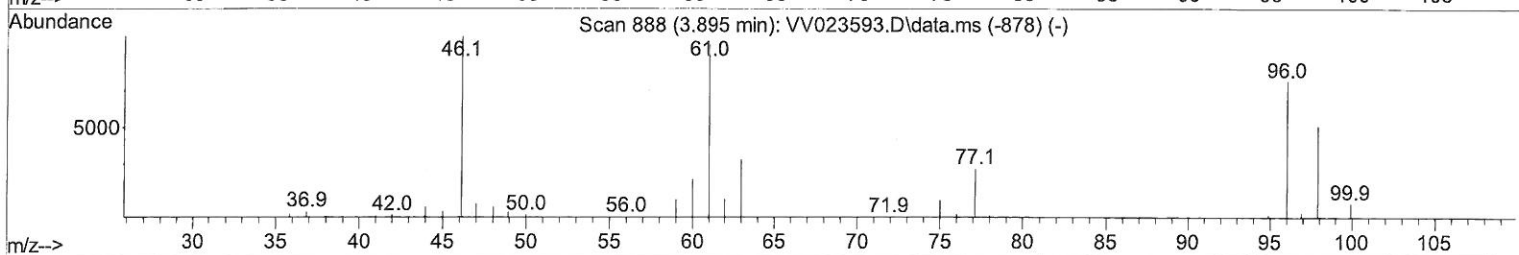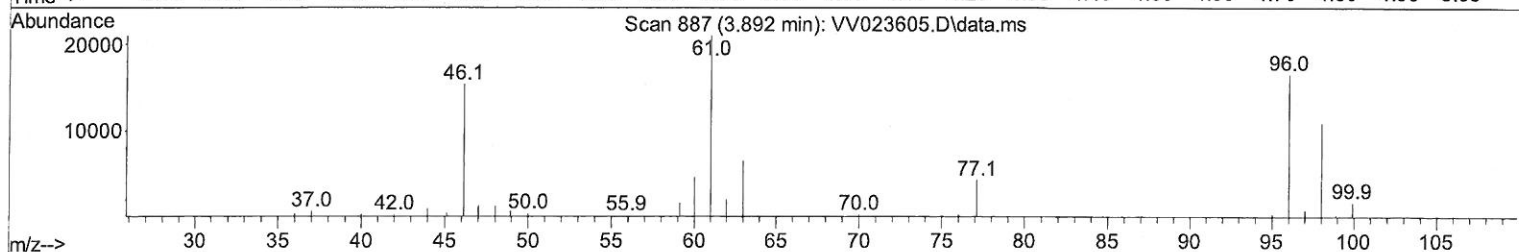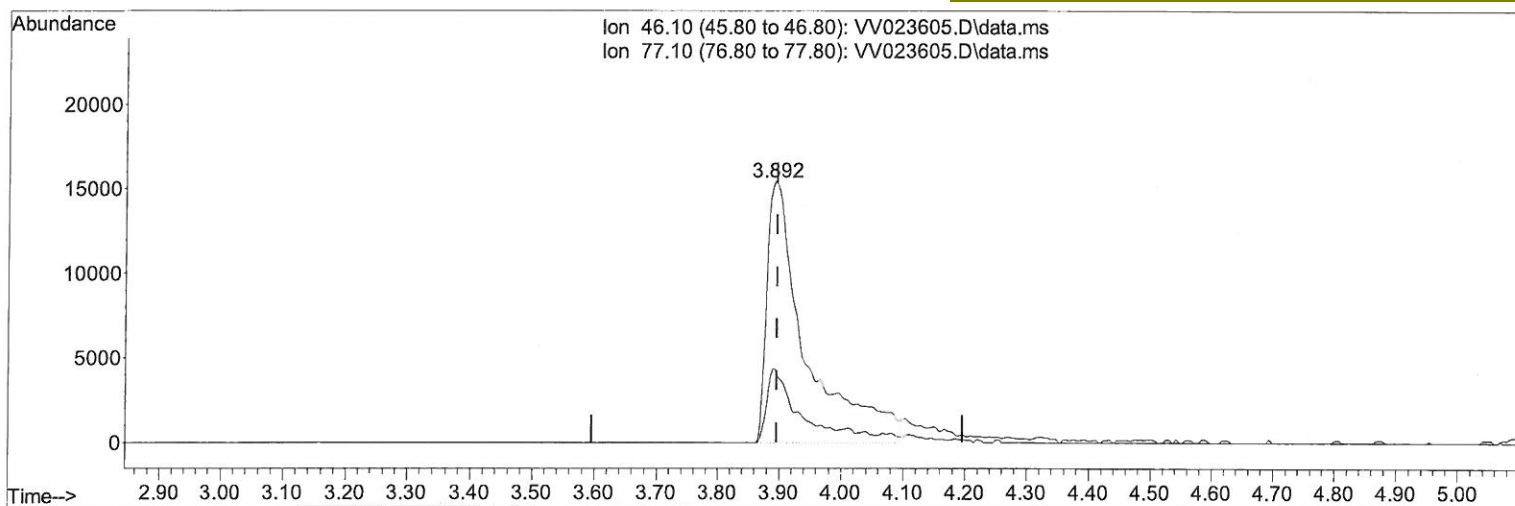

TIC: VV023605.D\data.ms

(20) 2-Butanone-d5 (S)

3.892min (-0.003) 52.97 ug/L m

response 67280

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.30	21.22
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV111821\  
 Data File : VV023605.D  
 Acq On : 18 Nov 2021 15:36  
 Operator : SY/MD  
 Sample : M4627-19DL 5X  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 Client Sampled :  
 H4674DL

Quant Time: Nov 19 02:14:02 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR110421WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Fri Nov 19 02:11:08 2021  
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/19/2021  
 Supervised By : Mahesh Dadoda 11/19/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	117686	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	115070	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	53670	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	39510	5.359	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 107.200%		
7) Chloroethane-d5	1.568	69	31316	5.212	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 104.200%		
11) 1,1-Dichloroethene-d2	2.108	63	52301	3.789	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 75.800%		
20) 2-Butanone-d5	3.892	46	67280m	52.970	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	= 105.940%		
24) Chloroform-d	4.352	84	70944	4.515	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 90.400%		
26) 1,2-Dichloroethane-d4	5.034	65	33195	4.698	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 94.000%		
32) Benzene-d6	5.053	84	133868	4.534	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 90.600%		
36) 1,2-Dichloropropane-d6	6.069	67	39255	4.517	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 90.400%		
41) Toluene-d8	7.317	98	114885	4.152	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 83.000%		
43) trans-1,3-Dichloroprop...	7.625	79	13650	4.142	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 82.800%		
46) 2-Hexanone-d5	8.091	63	51347	42.347	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 84.700%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	27407	4.385	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 87.600%		
66) 1,2-Dichlorobenzene-d4	11.625	152	45070	5.043	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 100.800%		
Target Compounds						Qvalue
5) Vinyl chloride	1.310	62	34246	3.514	ug/L	93
16) Methylene chloride	2.510	84	8766	0.856	ug/L	99
17) Methyl tert-butyl Ether	2.770	73	35570	2.302	ug/L	97
18) trans-1,2-Dichloroethene	2.767	96	4485	0.520	ug/L	95
19) 1,1-Dichloroethane	3.195	63	3800	0.261	ug/L	94
22) cis-1,2-Dichloroethene	3.912	96	105110	12.660	ug/L #	92
33) Benzene	5.108	78	5330	0.166	ug/L	100
34) Trichloroethene	5.921	95	3359	0.393	ug/L	93
63) 1,2,4-Trimethylbenzene	10.918	105	2356	0.093	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed