

Quantitation Report (QT/LSC Reviewed)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
 Data File : VV023607.D
 Acq On : 18 Nov 2021 16:23
 Operator : SY/MD
 Sample : M4694-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 H4653

Quant Time: Nov 19 02:14:27 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 19 02:11:08 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/19/2021
 Supervised By : Mahesh Dadoda 11/19/2021

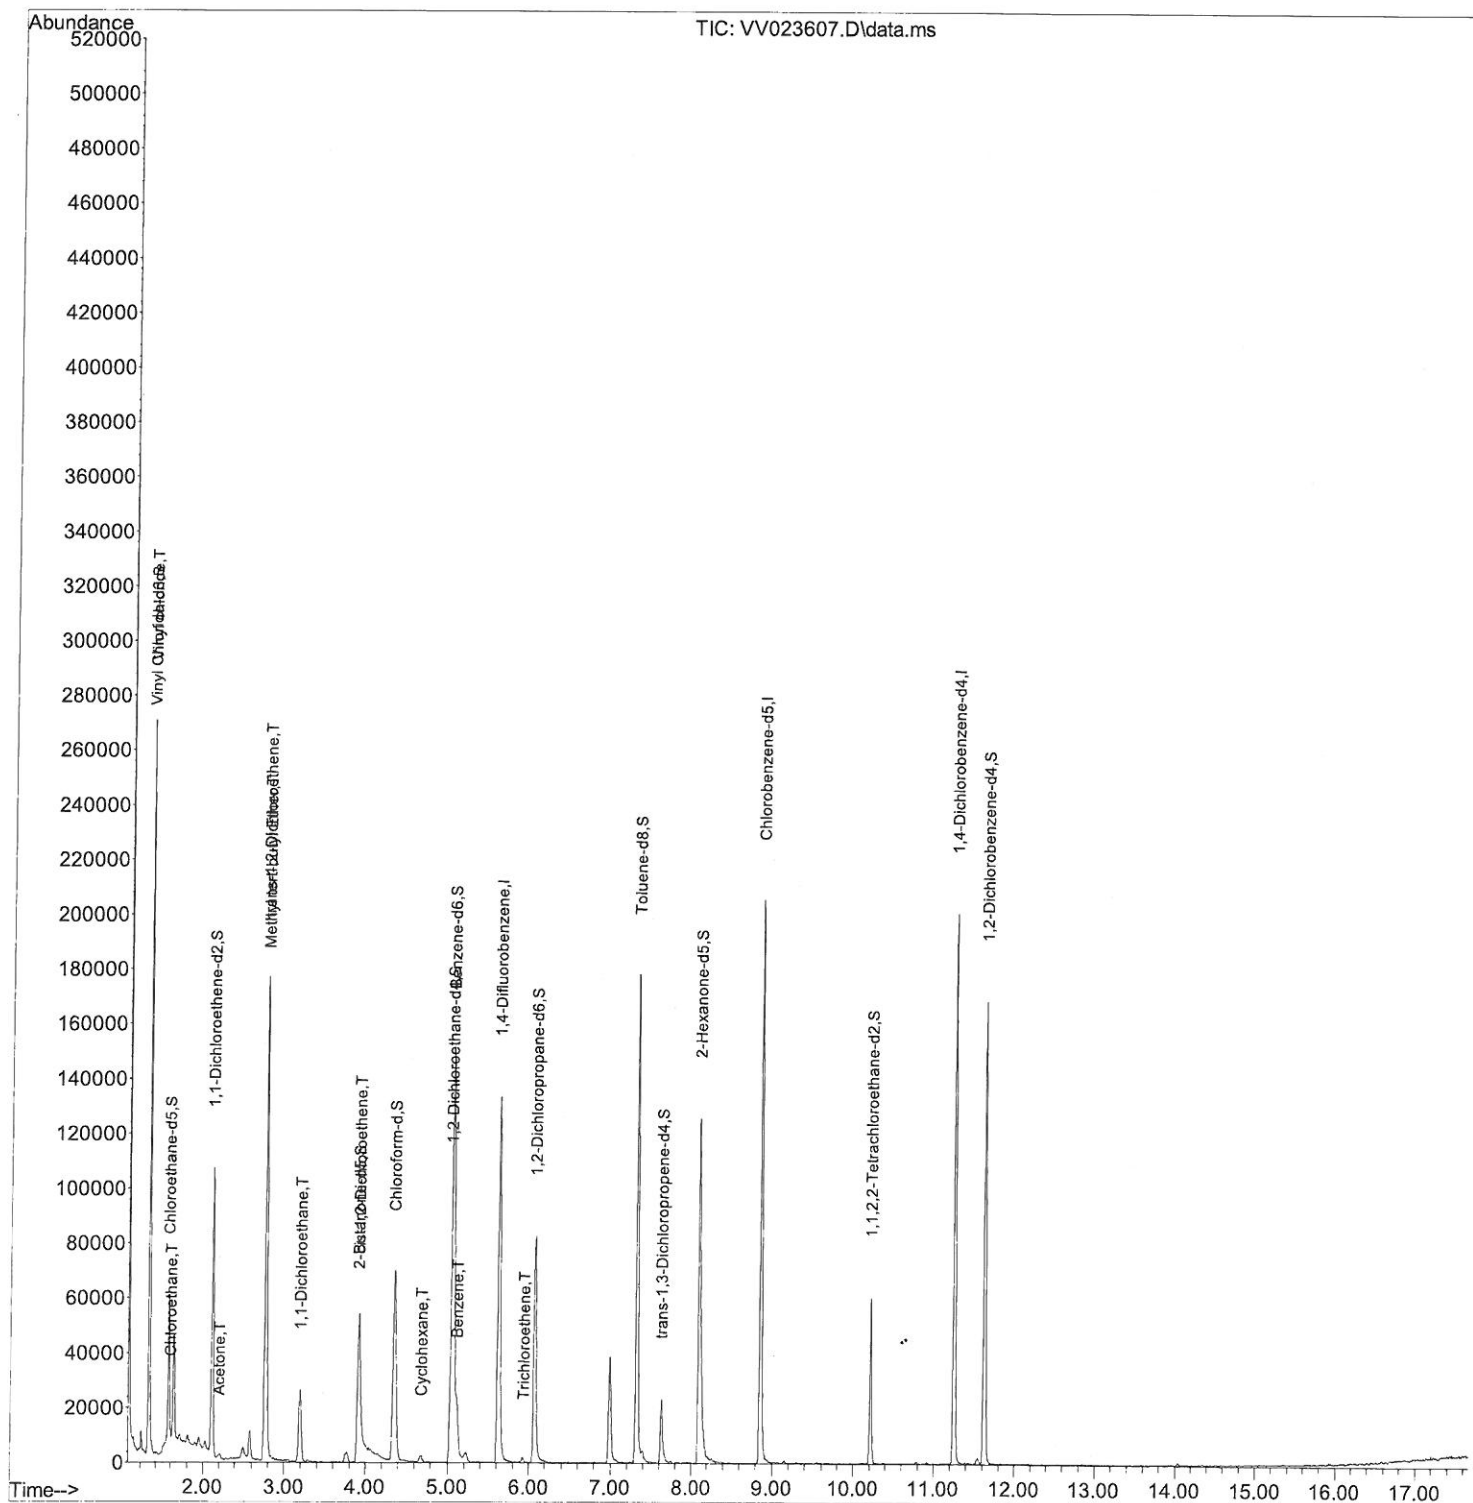

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
 Data File : VV023607.D
 Acq On : 18 Nov 2021 16:23
 Operator : SY/MD
 Sample : M4694-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 H4653

Quant Time: Nov 19 02:14:27 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 19 02:11:08 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/19/2021
 Supervised By : Mahesh Dadoda 11/19/2021

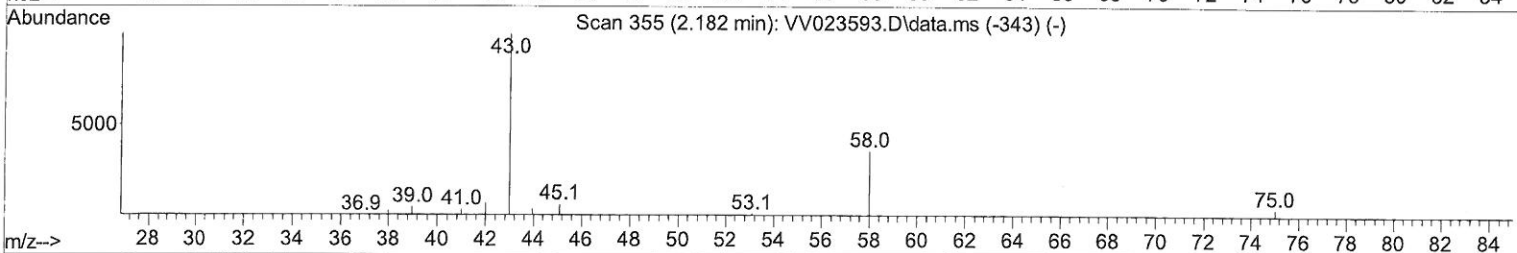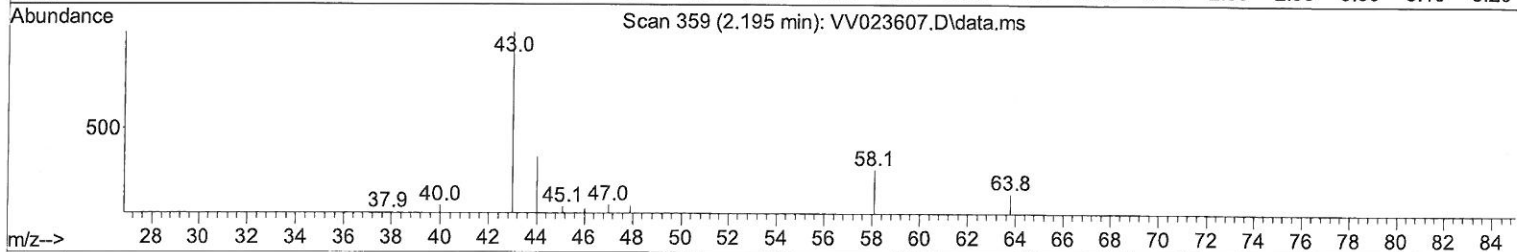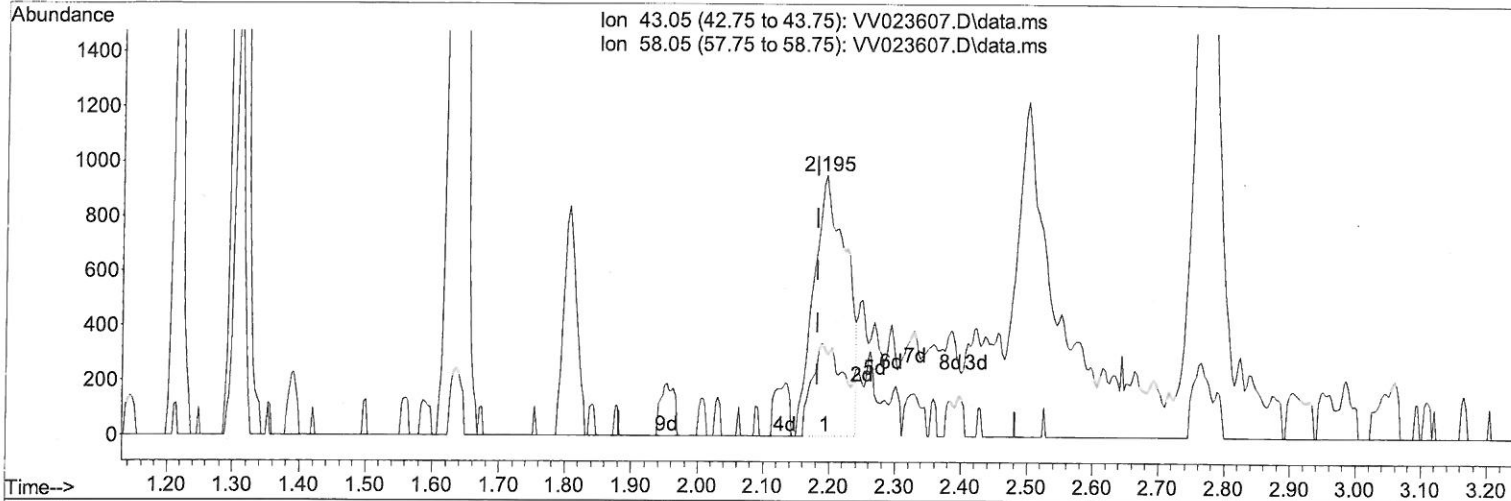

TIC: VV023607.D\data.ms

(13) Acetone (T)

2.195min (+ 0.013) 4.04 ug/L

response 3231

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.70	17.39
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
 Data File : VV023607.D
 Acq On : 18 Nov 2021 16:23
 Operator : SY/MD
 Sample : M4694-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 H4653

Quant Time: Nov 19 02:14:27 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 19 02:11:08 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/19/2021
 Supervised By : Mahesh Dadoda 11/19/2021

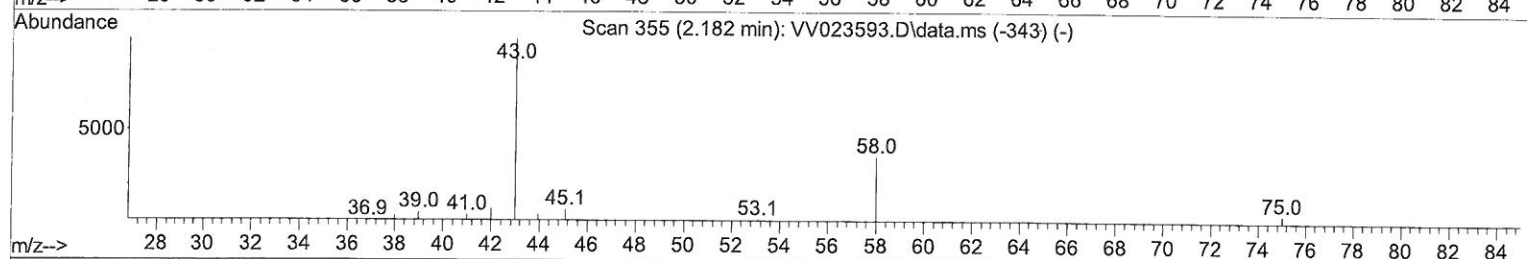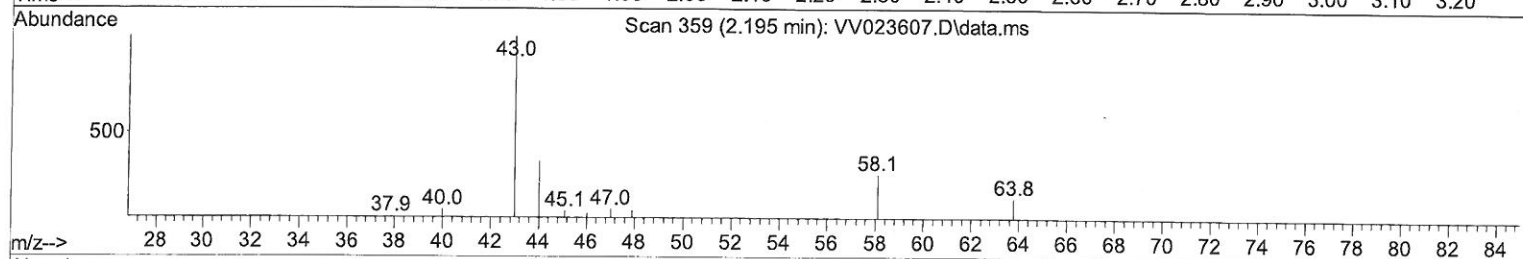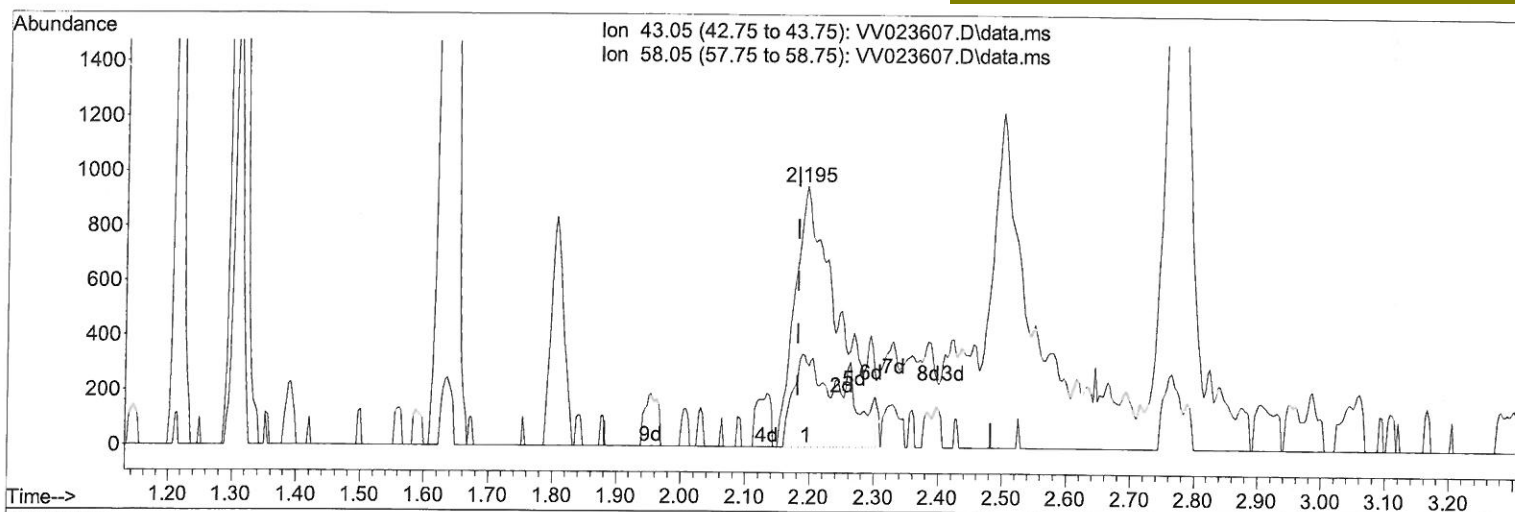

TIC: VV023607.D\data.ms

(13) Acetone (T)

2.195min (+ 0.013) 5.79 ug/L m

response 4627

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.70	12.15
0.00	0.00	0.00
0.00	0.00	0.00

7 MD
 11/26/21

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
 Data File : VV023607.D
 Acq On : 18 Nov 2021 16:23
 Operator : SY/MD
 Sample : M4694-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 H4653

Quant Time: Nov 19 02:14:27 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 19 02:11:08 2021
 Response via : Initial Calibration

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 11/19/2021
 Supervised By :Mahesh Dadoda 11/19/2021

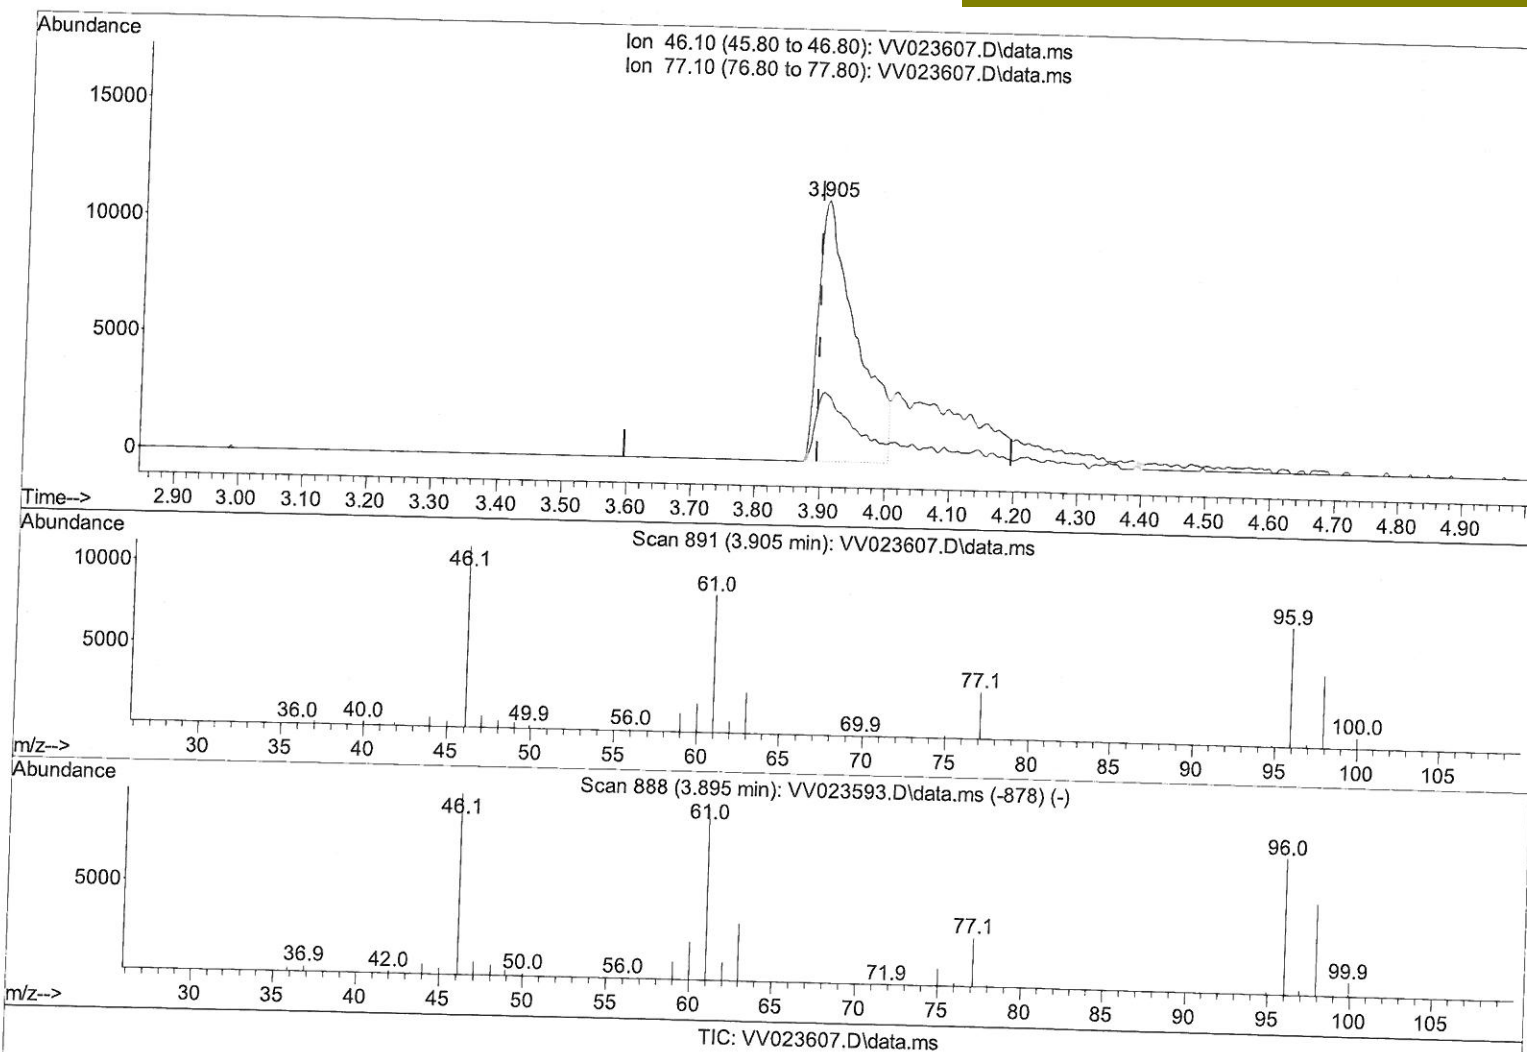

(20) 2-Butanone-d5 (S)

3.905min (+ 0.010) 34.26 ug/L

response 44826

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.30	23.89
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
 Data File : VV023607.D
 Acq On : 18 Nov 2021 16:23
 Operator : SY/MD
 Sample : M4694-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4653

Quant Time: Nov 19 02:14:27 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 19 02:11:08 2021
 Response via : Initial Calibration

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 11/19/2021
 Supervised By :Mahesh Dadoda 11/19/2021

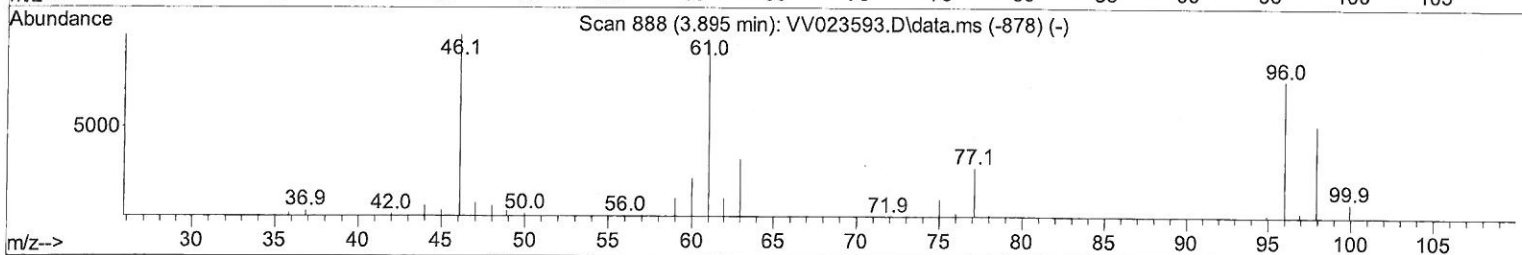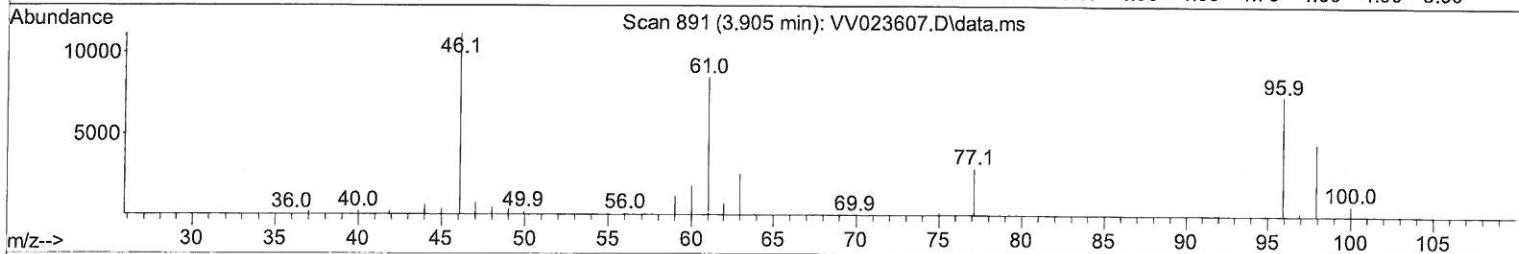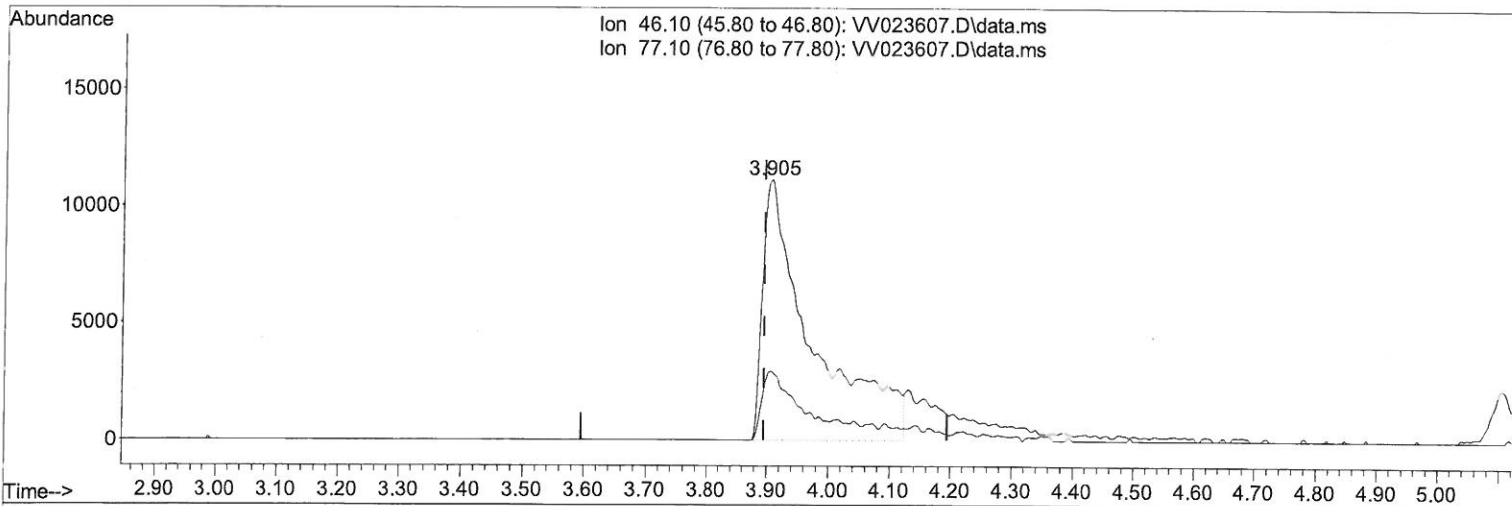

TIC: VV023607.D\data.ms

(20) 2-Butanone-d5 (S)

3.905min (+ 0.010) 47.64 ug/L m

response 62346

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.30	17.18
0.00	0.00	0.00
0.00	0.00	0.00

7 mg
11/26/24

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
 Data File : VV023607.D
 Acq On : 18 Nov 2021 16:23
 Operator : SY/MD
 Sample : M4694-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 H4653

Quant Time: Nov 19 02:14:27 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 19 02:11:08 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/19/2021
 Supervised By : Mahesh Dadoda 11/19/2021

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards							
1) 1,4-Difluorobenzene		5.619	114	121247	5.000	ug/L	0.00
28) Chlorobenzene-d5		8.853	117	119146	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.249	152	54572	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.307	65	39025	5.138	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130		Recovery	= 102.800%		
7) Chloroethane-d5		1.568	69	31245	5.047	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130		Recovery	= 101.000%		
11) 1,1-Dichloroethene-d2		2.108	63	53491	3.762	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125		Recovery	= 75.200%		
20) 2-Butanone-d5		3.905	46	62346m	47.643	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130		Recovery	= 95.280%		
24) Chloroform-d		4.349	84	70425	4.351	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125		Recovery	= 87.000%		
26) 1,2-Dichloroethane-d4		5.034	65	35027	4.812	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130		Recovery	= 96.200%		
32) Benzene-d6		5.050	84	138230	4.522	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125		Recovery	= 90.400%		
36) 1,2-Dichloropropane-d6		6.072	67	40771	4.531	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140		Recovery	= 90.600%		
41) Toluene-d8		7.317	98	120702	4.213	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130		Recovery	= 84.200%		
43) trans-1,3-Dichloroprop...		7.625	79	14121	4.138	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130		Recovery	= 82.800%		
46) 2-Hexanone-d5		8.095	63	53750	42.812	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130		Recovery	= 85.620%		
56) 1,1,2,2-Tetrachloroeth...		10.217	84	28051	4.334	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120		Recovery	= 86.600%		
66) 1,2-Dichlorobenzene-d4		11.625	152	45497	5.007	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120		Recovery	= 100.200%		
Target Compounds							Qvalue
5) Vinyl chloride		1.310	62	121839	12.136	ug/L	100
8) Chloroethane		1.587	64	2799	0.483	ug/L #	70
13) Acetone		2.195	43	4627m	5.787	ug/L	
17) Methyl tert-butyl Ether		2.767	73	29825	1.874	ug/L #	89
18) trans-1,2-Dichloroethene		2.760	96	58471	6.578	ug/L	98
19) 1,1-Dichloroethane		3.191	63	26706	1.780	ug/L	96
22) cis-1,2-Dichloroethene		3.915	96	21776	2.546	ug/L #	91
30) Cyclohexane		4.683	56	1296	0.100	ug/L	95
33) Benzene		5.108	78	24282	0.729	ug/L	100
34) Trichloroethene		5.934	95	476	0.054	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed