

Quantitation Report (QT/LSC Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
Data File : VV023610.D
Acq On : 18 Nov 2021 17:40
Operator : SY/MD
Sample : M4627-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
Client Sampled :
VHBLK001

Quant Time: Nov 19 04:08:19 2021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M


Quant Title : TRACE VOA SFAM1.0

QLast Update : Fri Nov 19 03:51:44 2021

Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/19/2021
Supervised By : Mahesh Dadoda 11/19/2021

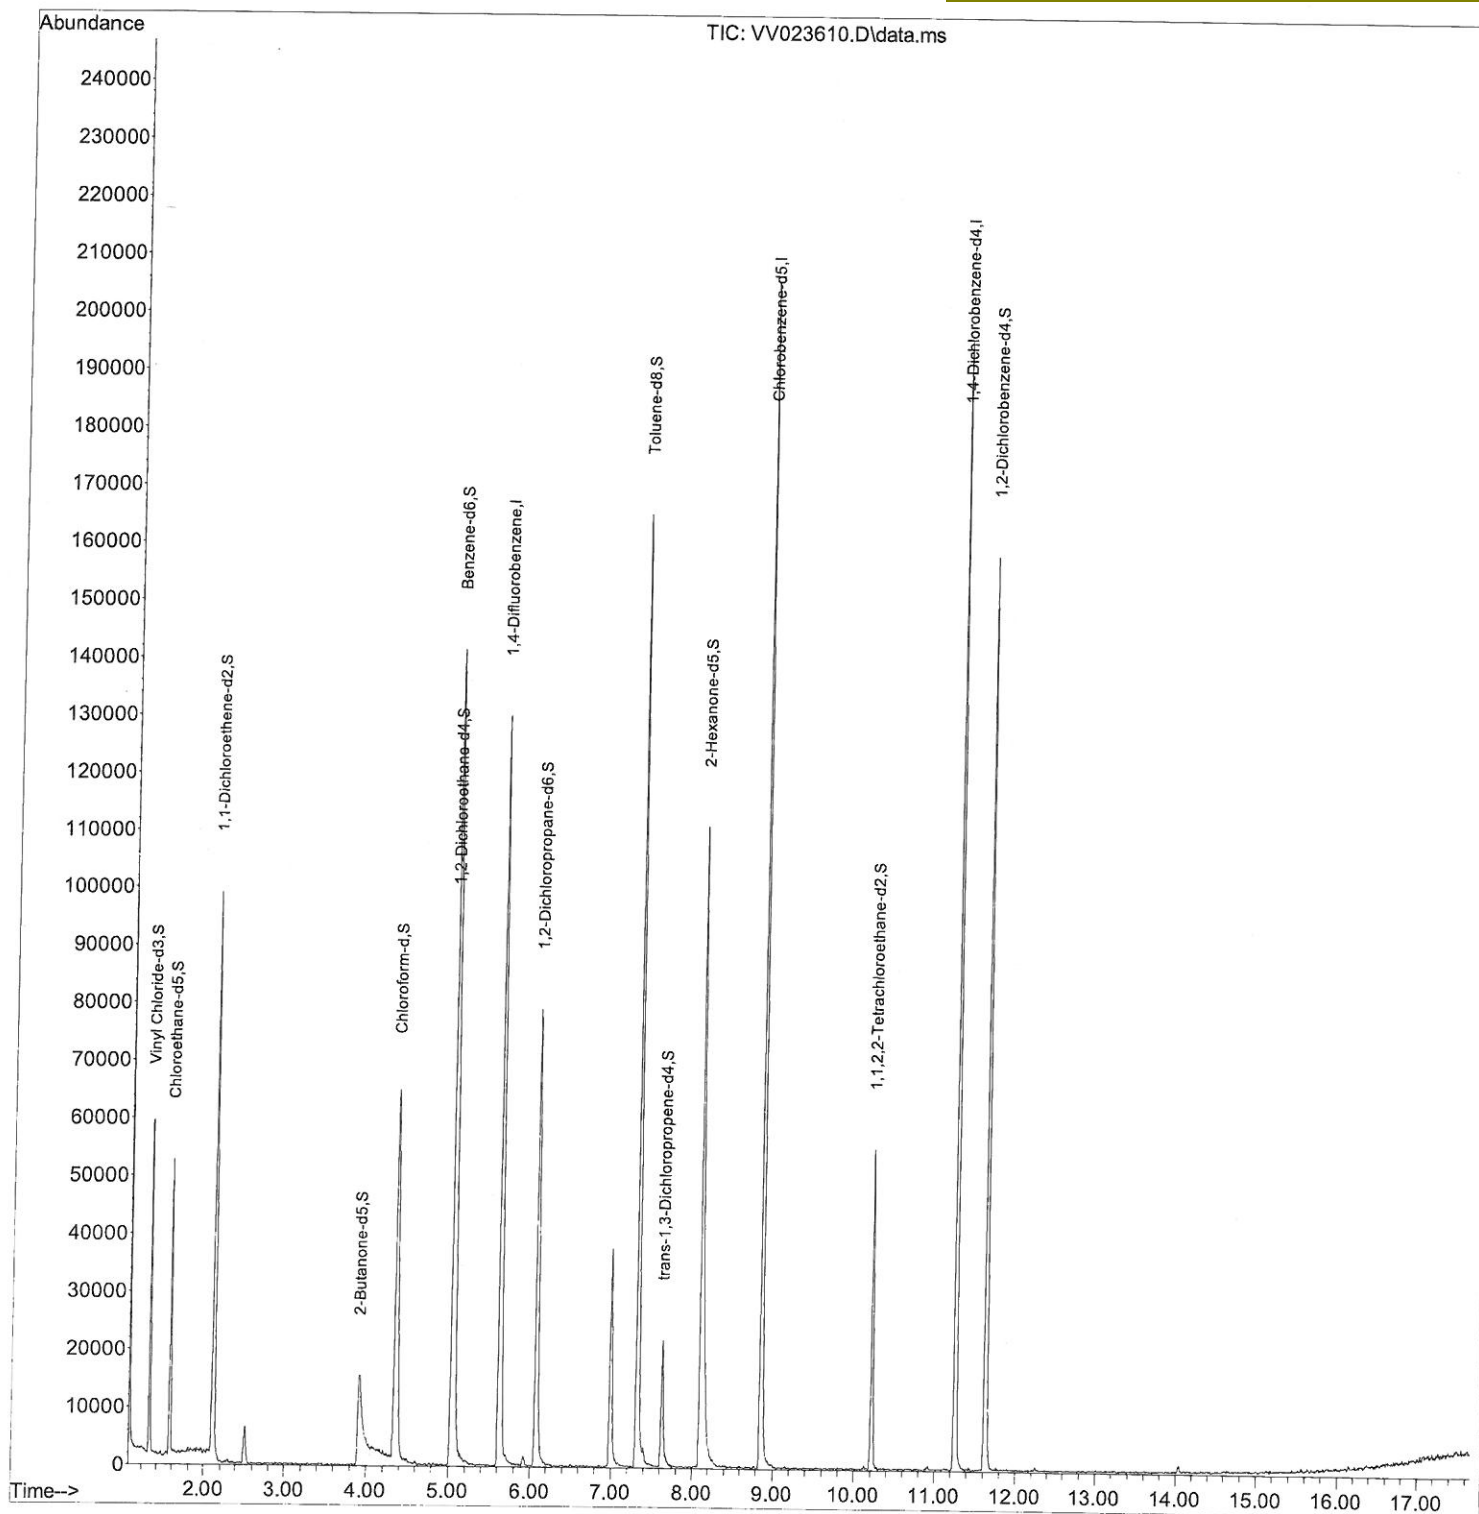

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
 Data File : VV023610.D
 Acq On : 18 Nov 2021 17:40
 Operator : SY/MD
 Sample : M4627-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Nov 19 04:08:19 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 19 03:51:44 2021
 Response via : Initial Calibration

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 11/19/2021
 Supervised By :Mahesh Dadoda 11/19/2021

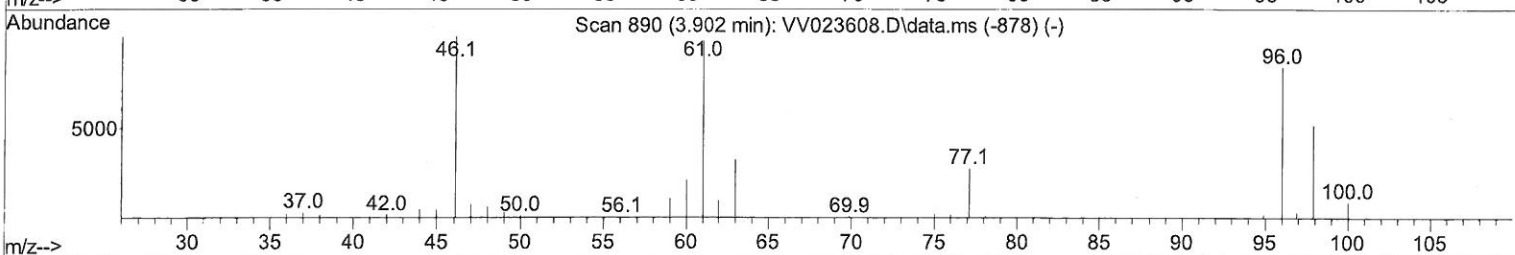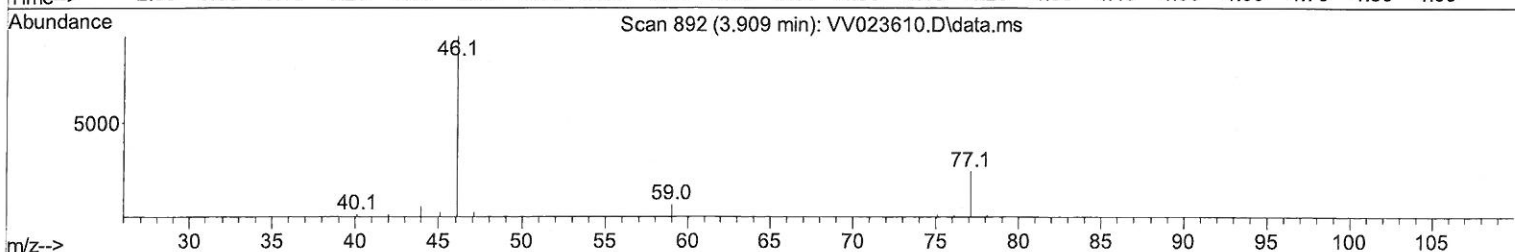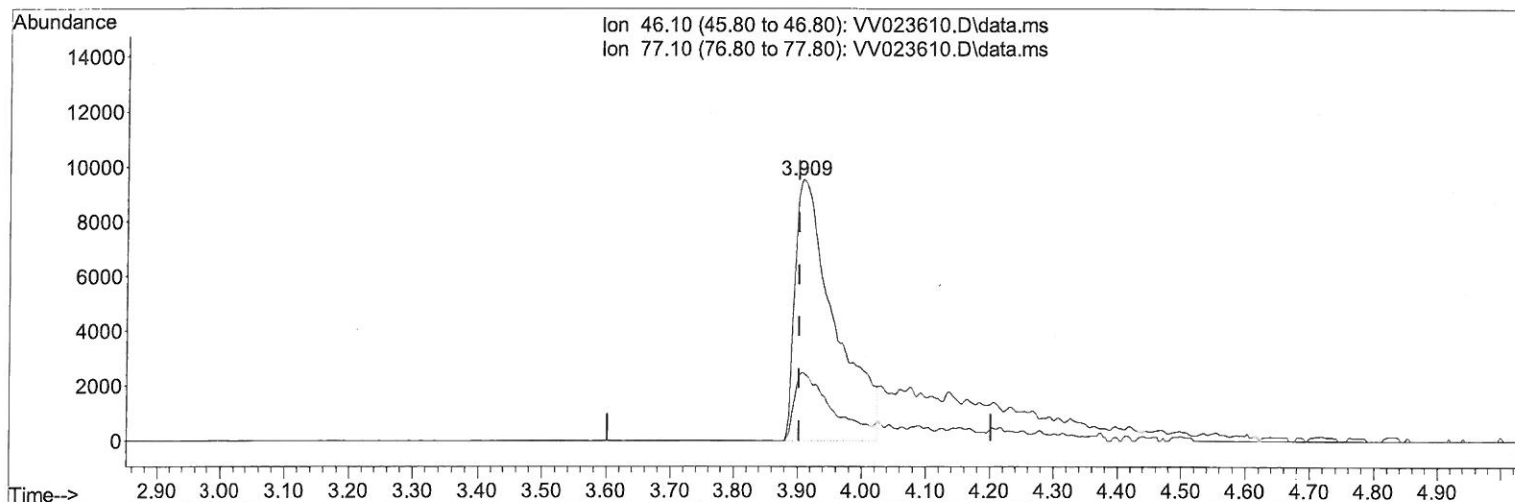

TIC: VV023610.D\data.ms

(20) 2-Butanone-d5 (S)

3.909min (+ 0.007) 32.79 ug/L

response 40743

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.30	20.07
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
 Data File : VV023610.D
 Acq On : 18 Nov 2021 17:40
 Operator : SY/MD
 Sample : M4627-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 VHBLK001

Quant Time: Nov 19 04:08:19 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 19 03:51:44 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/19/2021
 Supervised By : Mahesh Dadoda 11/19/2021

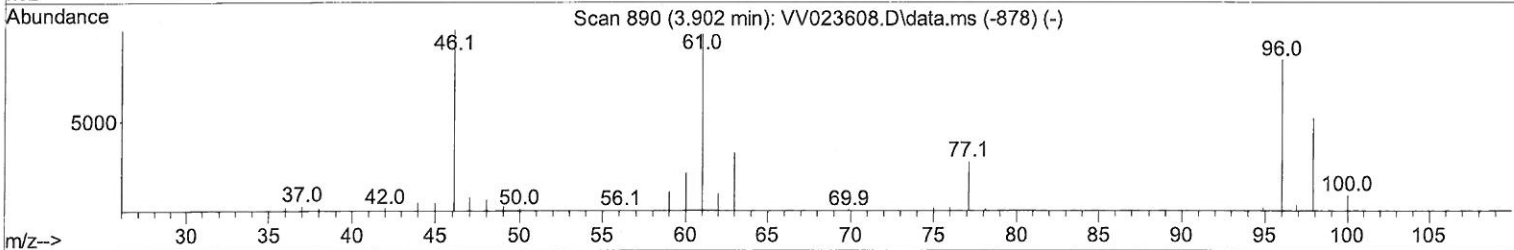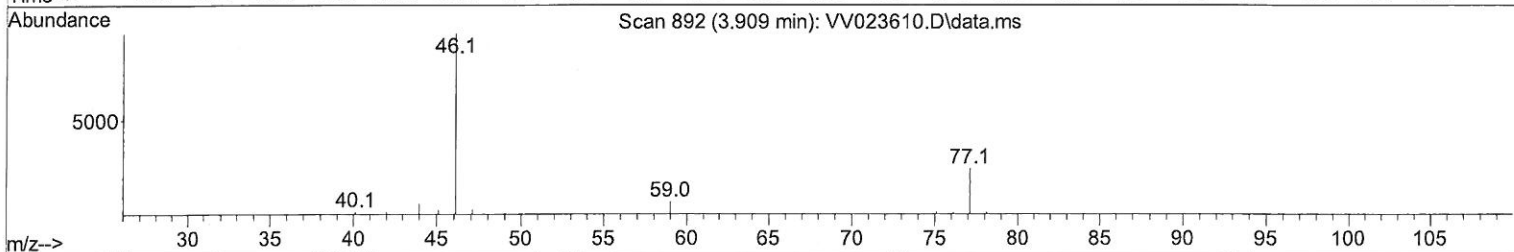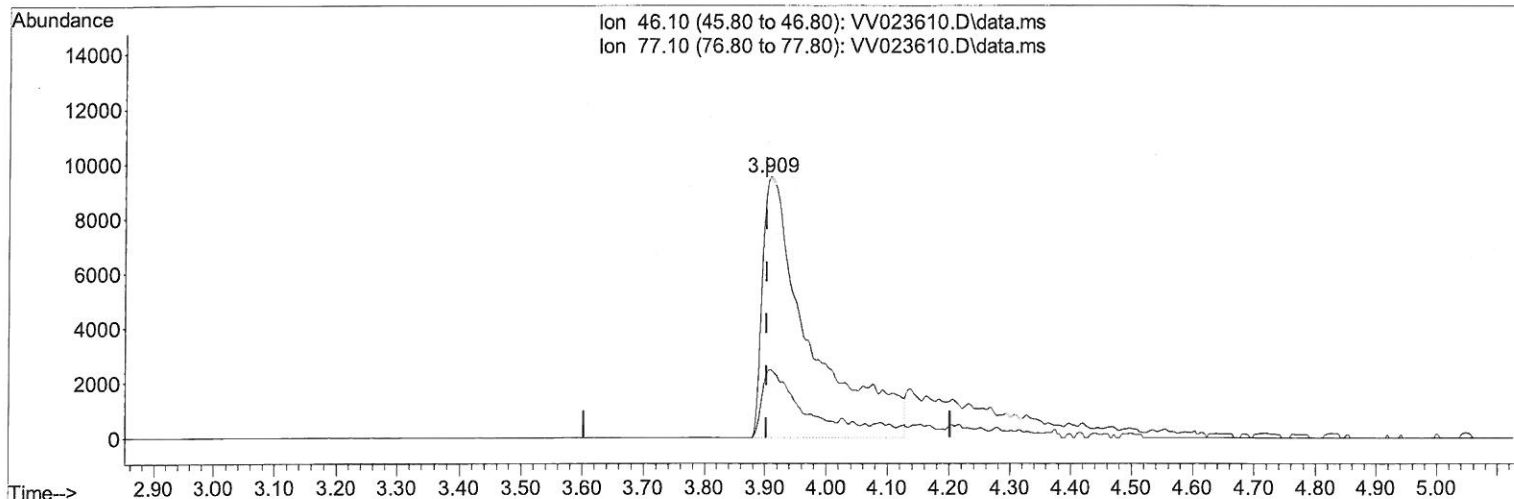

TIC: VV023610.D\data.ms

(20) 2-Butanone-d5 (S)

3.909min (+ 0.007) 41.36 ug/L m

response 51385

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.30	15.92
0.00	0.00	0.00
0.00	0.00	0.00

7 MD
 11/26/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111821\
 Data File : VW023610.D
 Acq On : 18 Nov 2021 17:40
 Operator : SY/MD
 Sample : M4627-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 VHBLK001

Quant Time: Nov 19 04:08:19 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 Qlast Update : Fri Nov 19 03:51:44 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/19/2021
 Supervised By : Mahesh Dadoda 11/19/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	115114	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	116931	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	52446	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	36250	5.027	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 100.600%		
7) Chloroethane-d5	1.568	69	29361	4.996	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 100.000%		
11) 1,1-Dichloroethene-d2	2.108	63	49805	3.689	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 73.800%		
20) 2-Butanone-d5	3.909	46	51385m	41.359	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	= 82.720%		
24) Chloroform-d	4.349	84	67412	4.386	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 87.800%		
26) 1,2-Dichloroethane-d4	5.034	65	32740	4.737	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 94.800%		
32) Benzene-d6	5.050	84	129081	4.302	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 86.000%		
36) 1,2-Dichloropropane-d6	6.069	67	36518	4.135	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 82.600%		
41) Toluene-d8	7.317	98	110965	3.947	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 79.000%		
43) trans-1,3-Dichloroprop...	7.625	79	13617	4.066	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 81.400%		
46) 2-Hexanone-d5	8.092	63	48766	39.578	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 79.160%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	26394	4.156	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 83.200%		
66) 1,2-Dichlorobenzene-d4	11.625	152	43151	4.941	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 98.800%		

7 mg
11/26/21

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed