

Quantitation Report (QT/LSC Reviewed)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
 Data File : VV023617.D
 Acq On : 18 Nov 2021 20:27
 Operator : SY/MD
 Sample : M4694-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Nov 19 04:09:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 19 03:51:44 2021
 Response via : Initial Calibration

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 11/19/2021
 Supervised By :Mahesh Dadoda 11/19/2021

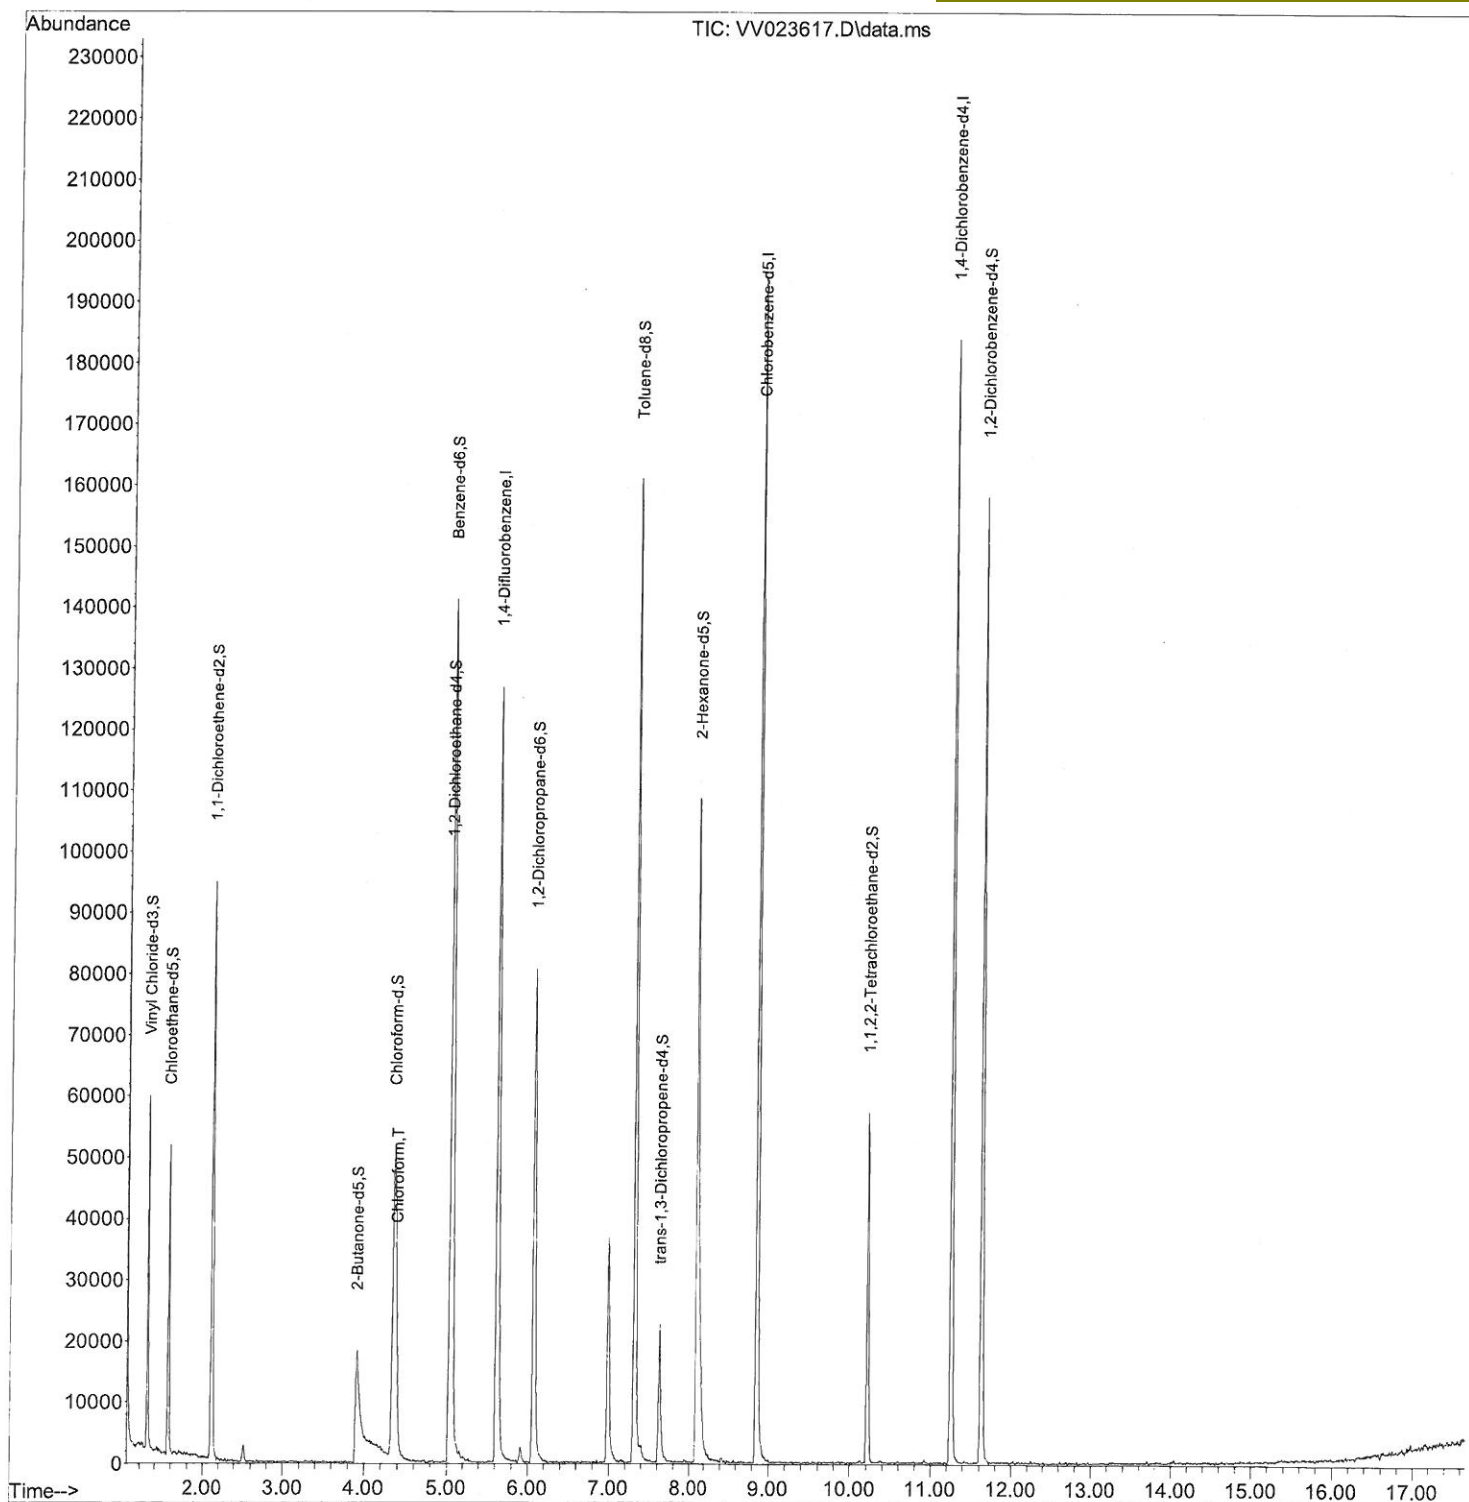

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
 Data File : VV023617.D
 Acq On : 18 Nov 2021 20:27
 Operator : SY/MD
 Sample : M4694-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Nov 19 04:09:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 19 03:51:44 2021
 Response via : Initial Calibration

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 11/19/2021
 Supervised By :Mahesh Dadoda 11/19/2021

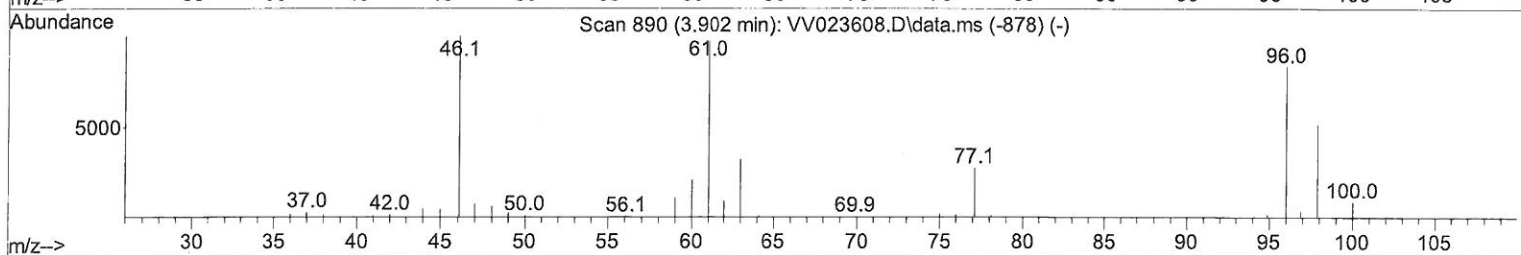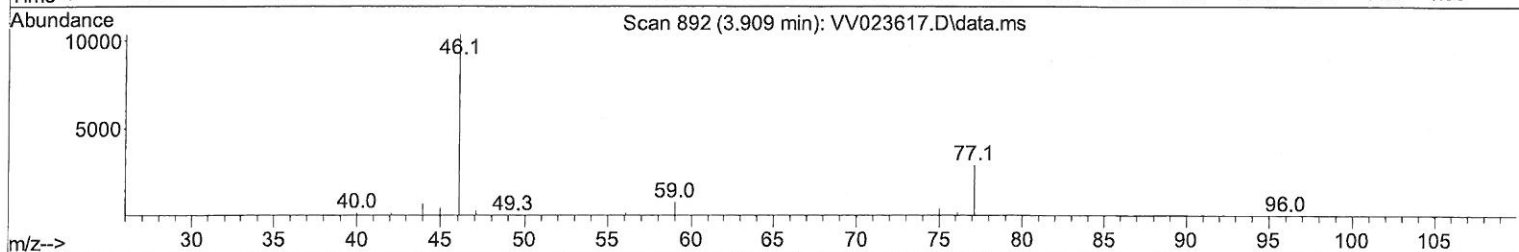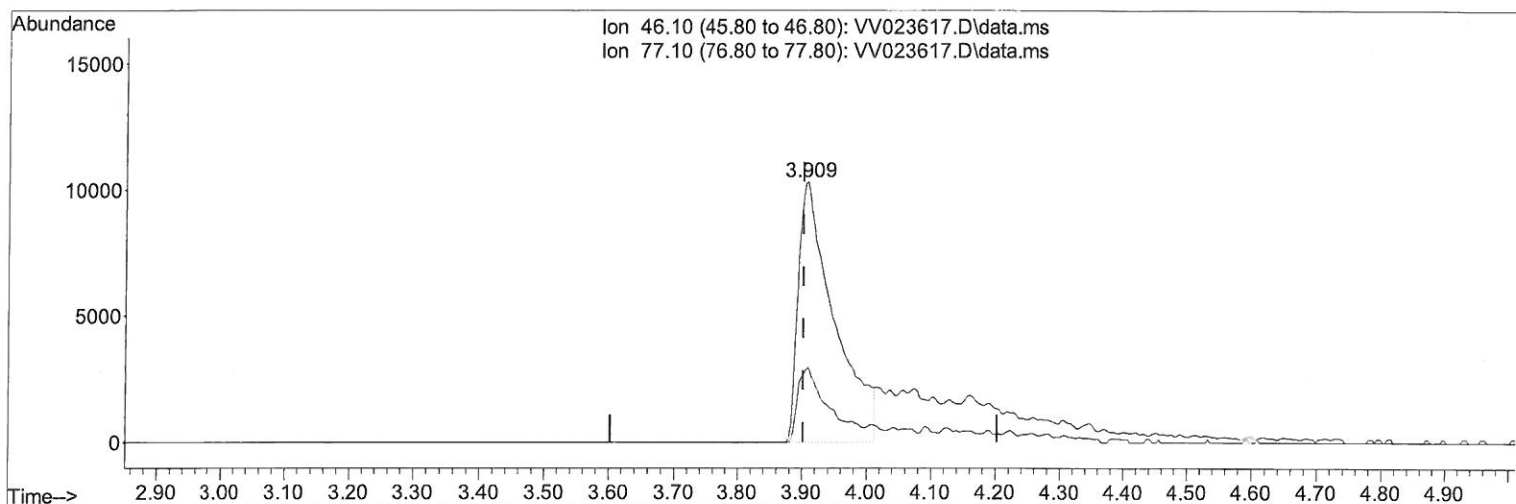

TIC: VV023617.D\data.ms

(20) 2-Butanone-d5 (S)

3.909min (+ 0.007) 32.83 ug/L

response 39697

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.30	24.93
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
 Data File : VV023617.D
 Acq On : 18 Nov 2021 20:27
 Operator : SY/MD
 Sample : M4694-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Nov 19 04:09:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 19 03:51:44 2021
 Response via : Initial Calibration

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 11/19/2021
 Supervised By :Mahesh Dadoda 11/19/2021

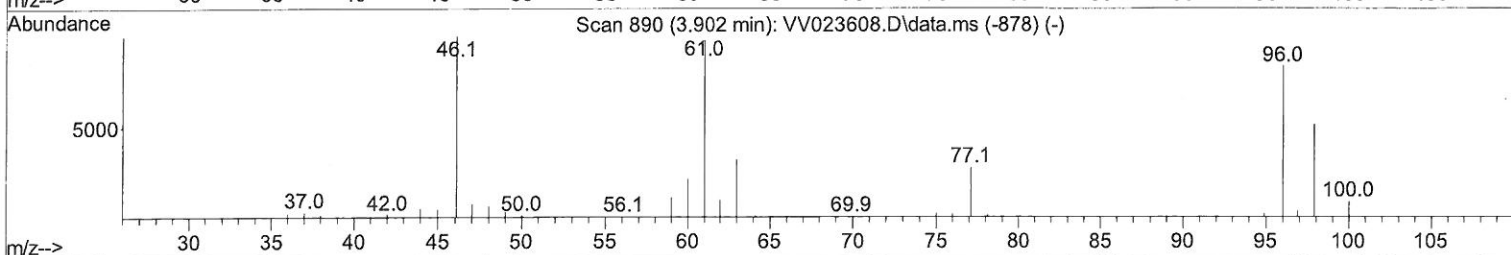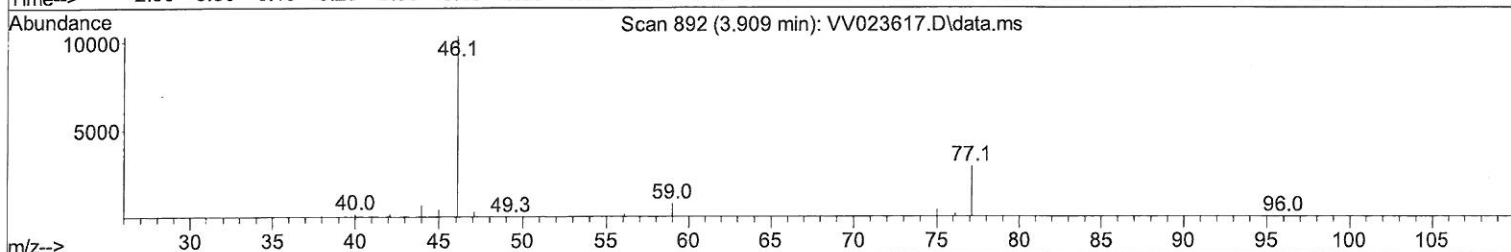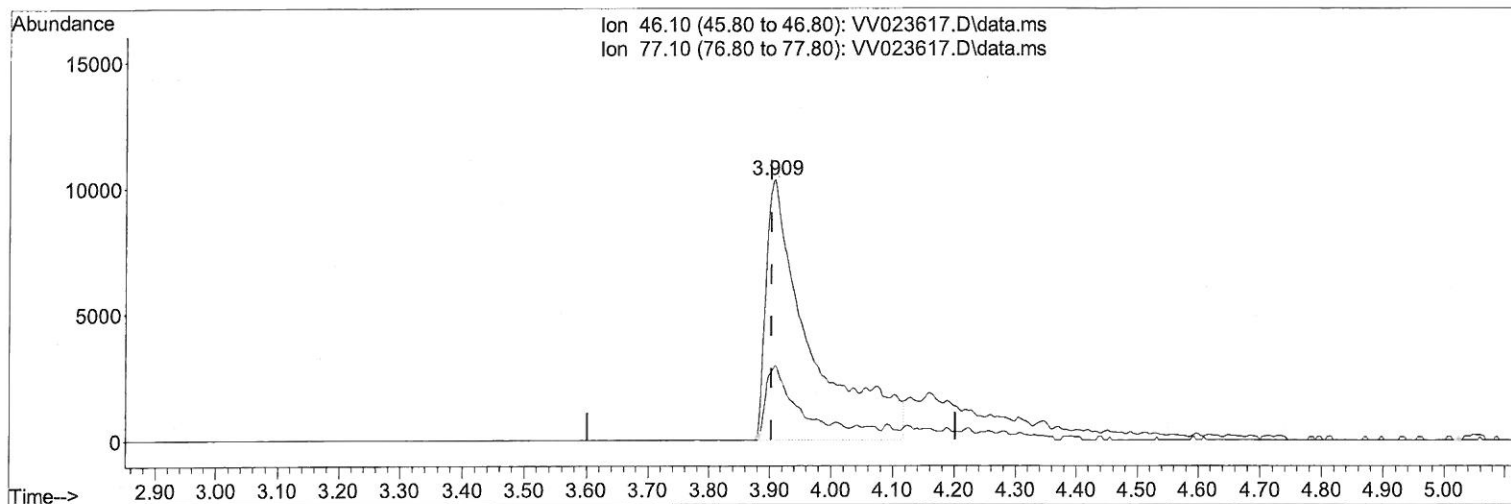

TIC: VV023617.D\data.ms

(20) 2-Butanone-d5 (S)

3.909min (+ 0.007) 42.79 ug/L m

response 51735

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.30	19.13
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
 Data File : VV023617.D
 Acq On : 18 Nov 2021 20:27
 Operator : SY/MD
 Sample : M4694-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 VHBLK001

Quant Time: Nov 19 04:09:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 19 03:51:44 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/19/2021
 Supervised By : Mahesh Dadoda 11/19/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	112032	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	112973	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	50022	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	34149	4.866	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery = 97.400%			
7) Chloroethane-d5	1.568	69	29214	5.107	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery = 102.200%			
11) 1,1-Dichloroethene-d2	2.108	63	49122	3.739	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery = 74.800%			
20) 2-Butanone-d5	3.909	46	51735m	42.787	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery = 85.580%			
24) Chloroform-d	4.352	84	47046	3.145	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 63.000%#			
26) 1,2-Dichloroethane-d4	5.034	65	33692	5.009	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 100.200%			
32) Benzene-d6	5.050	84	128265	4.425	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 88.400%			
36) 1,2-Dichloropropane-d6	6.069	67	38935	4.563	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery = 91.200%			
41) Toluene-d8	7.317	98	107767	3.967	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 79.400%			
43) trans-1,3-Dichloroprop...	7.625	79	13118	4.054	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery = 81.000%			
46) 2-Hexanone-d5	8.092	63	46796	39.310	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery = 78.620%			
56) 1,1,2,2-Tetrachloroeth...	10.217	84	26921	4.387	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery = 87.800%			
66) 1,2-Dichlorobenzene-d4	11.625	152	42019	5.045	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery = 100.800%			
Target Compounds						
25) Chloroform	4.381	83	21679	1.467	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed