

Quantitation Report (QT/LSC Reviewed)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
 Data File : VV023626.D
 Acq On : 19 Nov 2021 00:03
 Operator : SY/MD
 Sample : M4706-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 B0AB5

Quant Time: Nov 19 04:11:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 19 03:51:44 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/19/2021
 Supervised By : Mahesh Dadoda 11/19/2021

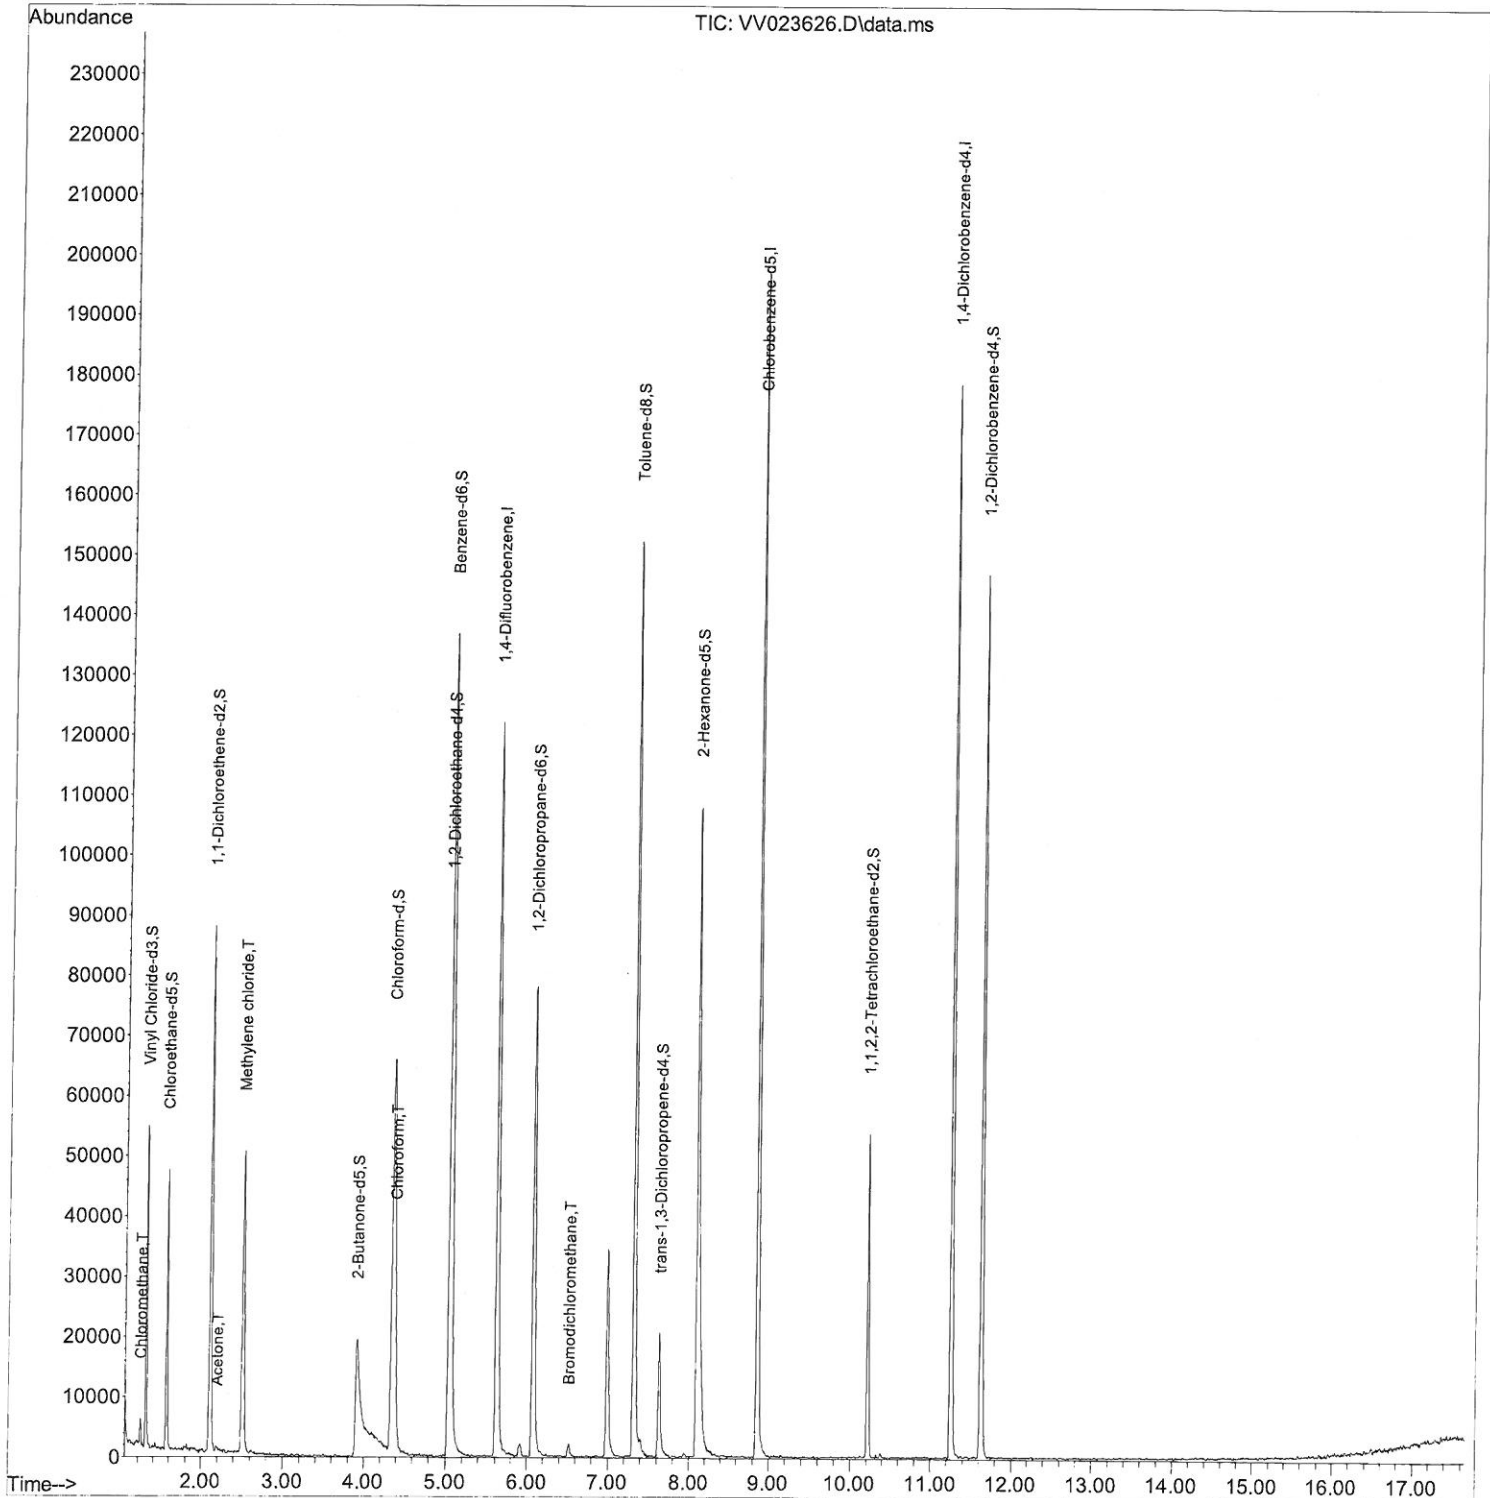

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
 Data File : VV023626.D
 Acq On : 19 Nov 2021 00:03
 Operator : SY/MD
 Sample : M4706-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 B0AB5

Quant Time: Nov 19 04:11:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 19 03:51:44 2021
 Response via : Initial Calibration

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 11/19/2021
 Supervised By :Mahesh Dadoda 11/19/2021

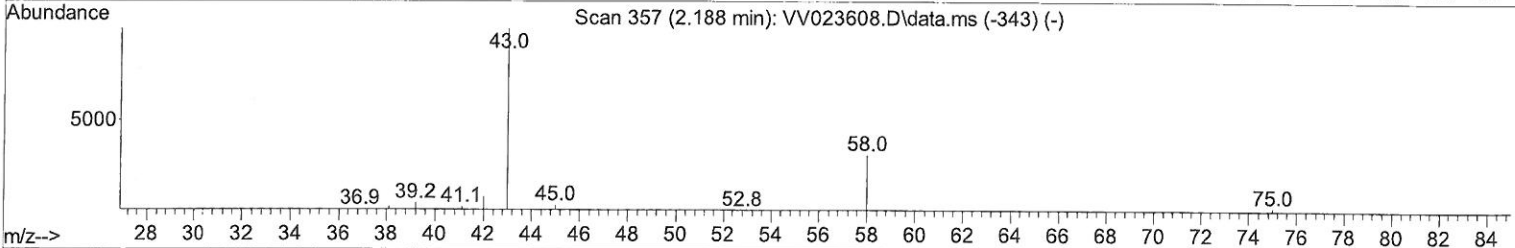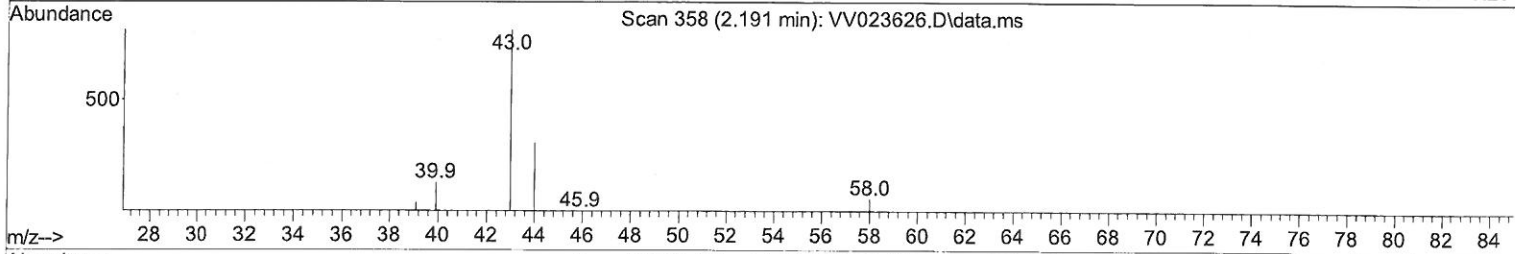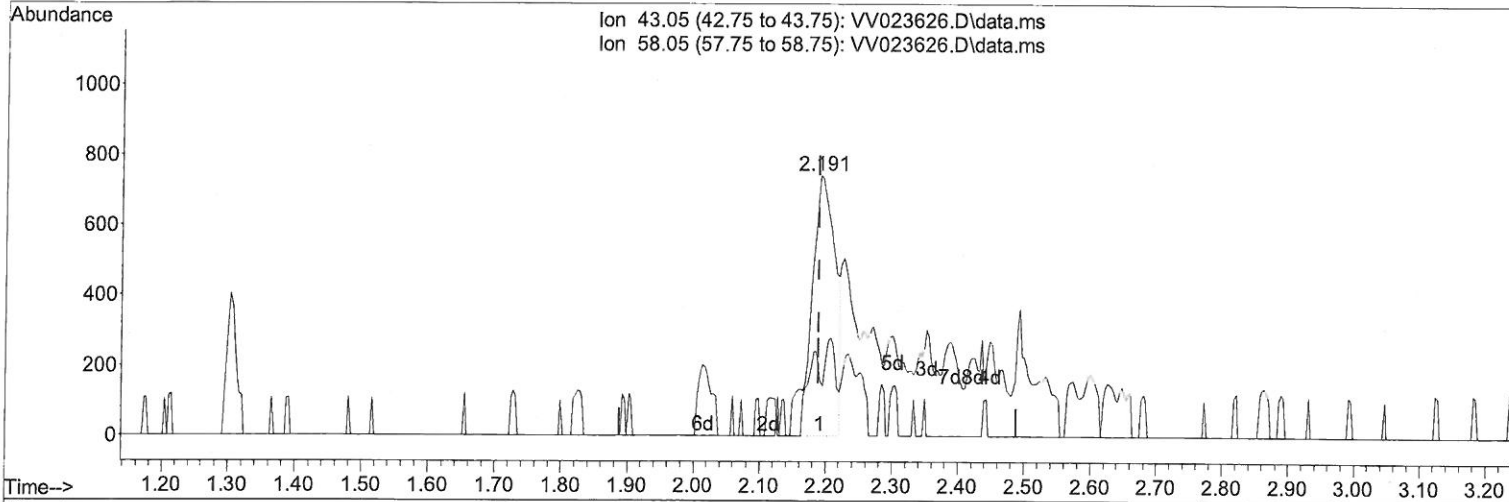

TIC: VV023626.D\data.ms

(13) Acetone (T)

2.191min (+ 0.003) 2.61 ug/L

response 1863

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.70	18.20
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
 Data File : VV023626.D
 Acq On : 19 Nov 2021 00:03
 Operator : SY/MD
 Sample : M4706-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 B0AB5

Quant Time: Nov 19 04:11:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 19 03:51:44 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/19/2021
 Supervised By : Mahesh Dadoda 11/19/2021

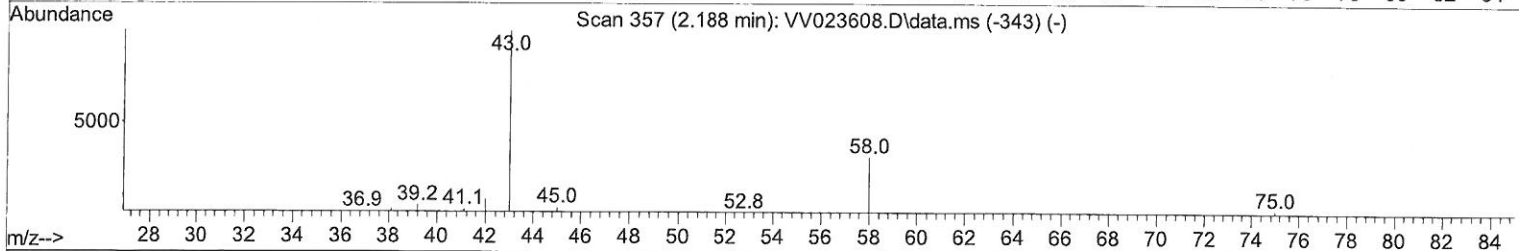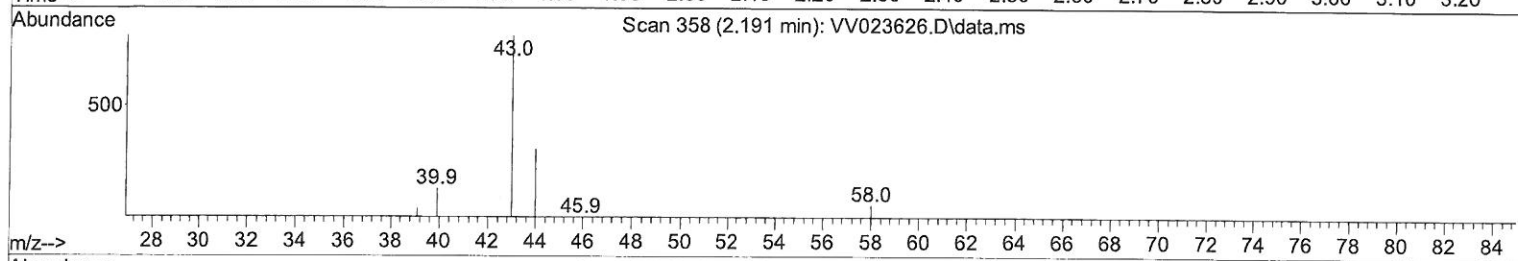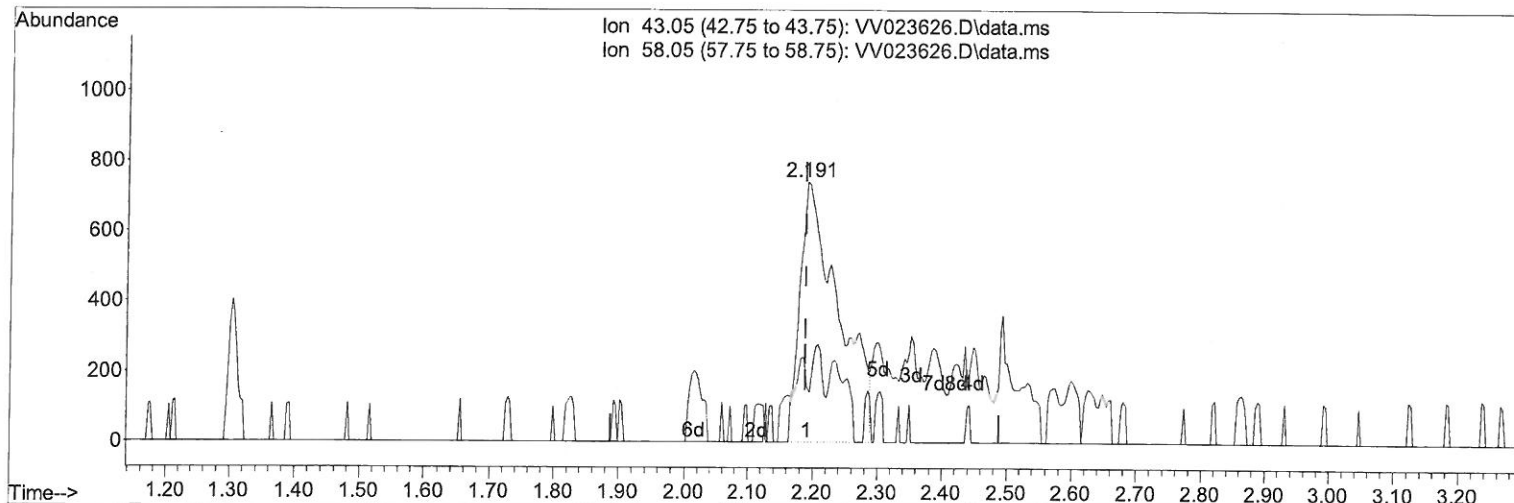

TIC: VV023626.D\data.ms

(13) Acetone (T)

2.191min (+ 0.003) 4.44 ug/L m

response 3175

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.70	10.68
0.00	0.00	0.00
0.00	0.00	0.00

MD
 11/26/21

Quantitation Report (QT/LSC Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
 Data File : VV023626.D
 Acq On : 19 Nov 2021 00:03
 Operator : SY/MD
 Sample : M4706-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 B0AB5

Quant Time: Nov 19 04:11:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 Qlast Update : Fri Nov 19 03:51:44 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/19/2021
 Supervised By : Mahesh Dadoda 11/19/2021

Compound	R.T.	QIon	Response	Conc Units	Dev(Min)
Internal Standards					
1) 1,4-Difluorobenzene	5.619	114	108419	5.000 ug/L	0.00
28) Chlorobenzene-d5	8.853	117	110958	5.000 ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	48394	5.000 ug/L	0.00
System Monitoring Compounds					
4) Vinyl Chloride-d3	1.304	65	32501	4.785 ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	95.800%	
7) Chloroethane-d5	1.568	69	27302	4.932 ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	98.600%	
11) 1,1-Dichloroethene-d2	2.108	63	45291	3.562 ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	71.200%	
20) 2-Butanone-d5	3.912	46	40087	34.258 ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	68.520%	
24) Chloroform-d	4.352	84	64044	4.425 ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	88.400%	
26) 1,2-Dichloroethane-d4	5.034	65	31428	4.828 ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	96.600%	
32) Benzene-d6	5.050	84	120860	4.245 ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	85.000%	
36) 1,2-Dichloropropane-d6	6.069	67	36313	4.333 ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	86.600%	
41) Toluene-d8	7.317	98	102089	3.827 ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	76.600%	
43) trans-1,3-Dichloroprop...	7.628	79	12857	4.046 ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	81.000%	
46) 2-Hexanone-d5	8.091	63	44397	37.972 ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	75.940%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	25196	4.181 ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	83.600%	
66) 1,2-Dichlorobenzene-d4	11.625	152	39341	4.882 ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	97.600%	
Target Compounds					
3) Chloromethane	1.240	50	2724	0.303 ug/L	98
13) Acetone	2.191	43	3175m	4.441 ug/L	
16) Methylene chloride	2.506	84	21577	2.287 ug/L	93
25) Chloroform	4.381	83	21258	1.486 ug/L	95
38) Bromodichloromethane	6.519	83	1807	0.186 ug/L #	98

7 m0
 11/26/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed