

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
 Data File : VV023596.D
 Acq On : 18 Nov 2021 12:01
 Operator : SY/MD
 Sample : M4616-21
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Nov 19 02:12:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 19 02:11:08 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	113808	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	111712	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	52027	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	43117	6.048	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	121.000%
7) Chloroethane-d5	1.568	69	31960	5.500	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	110.000%
11) 1,1-Dichloroethene-d2	2.108	63	57582	4.314	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	86.200%
20) 2-Butanone-d5	3.886	46	63965	52.076	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.160%
24) Chloroform-d	4.346	84	73519	4.839	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.800%
26) 1,2-Dichloroethane-d4	5.031	65	34296	5.019	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.400%
32) Benzene-d6	5.050	84	142261	4.963	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.200%
36) 1,2-Dichloropropane-d6	6.069	67	40179	4.762	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.200%
41) Toluene-d8	7.317	98	121804	4.535	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.600%
43) trans-1,3-Dichloroprop...	7.625	79	14480	4.526	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.600%
46) 2-Hexanone-d5	8.088	63	47751	40.565	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.140%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	26808	4.418	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.400%
66) 1,2-Dichlorobenzene-d4	11.625	152	45305	5.230	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.600%
Target Compounds						Qvalue
16) Methylene chloride	2.510	84	4576	0.462	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
Data File : VV023596.D
Acq On : 18 Nov 2021 12:01
Operator : SY/MD
Sample : M4616-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Nov 19 02:12:09 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 19 02:11:08 2021
Response via : Initial Calibration

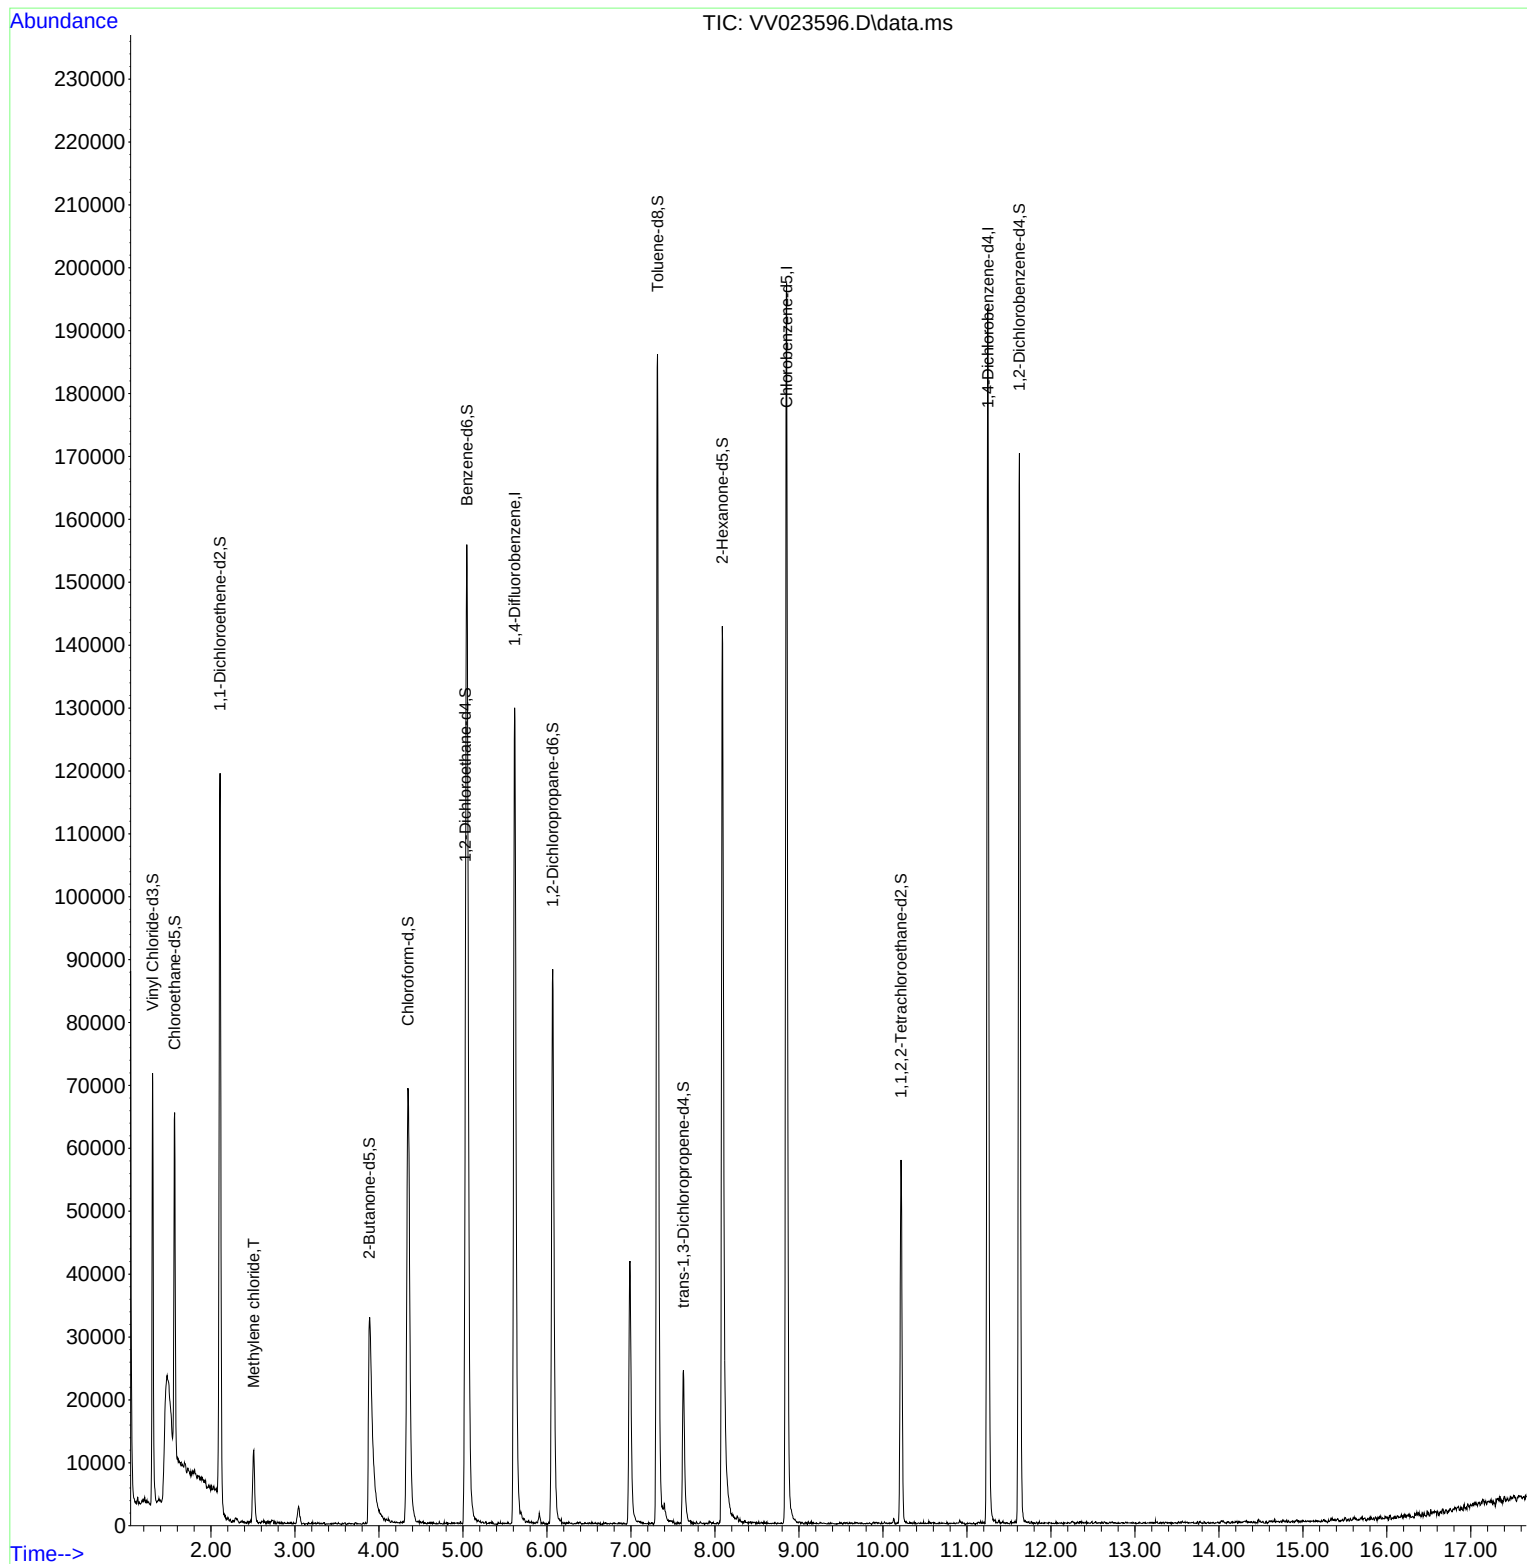

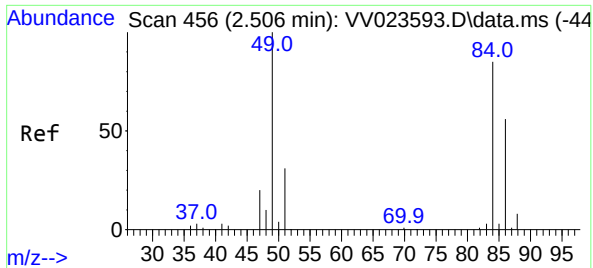

#16
 Methylene chloride
 Concen: 0.462 ug/L
 RT: 2.510 min Scan# 4
 Delta R.T. 0.003 min
 Lab File: VV023596.D
 Acq: 18 Nov 2021 12:01

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Tgt Ion: 84 Resp: 4576

Ion	Ratio	Lower	Upper
84	100		
86	70.1	42.3	78.5
49	115.5	79.7	148.1

