

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
 Data File : VV023603.D
 Acq On : 18 Nov 2021 14:48
 Operator : SY/MD
 Sample : M4694-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4634

Quant Time: Nov 19 02:13:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 19 02:11:08 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	119460	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	114836	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	54114	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	37690	5.036	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	100.800%	
7) Chloroethane-d5	1.568	69	29570	4.848	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	97.000%	
11) 1,1-Dichloroethene-d2	2.108	63	51132	3.650	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	73.000%	
20) 2-Butanone-d5	3.899	46	52749	40.913	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	81.820%	
24) Chloroform-d	4.349	84	68534	4.297	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	86.000%	
26) 1,2-Dichloroethane-d4	5.037	65	32569	4.541	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	90.800%	
32) Benzene-d6	5.053	84	133162	4.519	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.400%	
36) 1,2-Dichloropropane-d6	6.072	67	37948	4.375	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	87.600%	
41) Toluene-d8	7.317	98	112172	4.063	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	81.200%	
43) trans-1,3-Dichloroprop...	7.625	79	13746	4.180	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	83.600%	
46) 2-Hexanone-d5	8.092	63	48575	40.142	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	80.280%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	25561	4.098	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	82.000%	
66) 1,2-Dichlorobenzene-d4	11.625	152	42979	4.770	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	95.400%	
Target Compounds					Qvalue	
13) Acetone	2.179	43	6375	8.092	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
Data File : VV023603.D
Acq On : 18 Nov 2021 14:48
Operator : SY/MD
Sample : M4694-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4634

Quant Time: Nov 19 02:13:38 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 19 02:11:08 2021
Response via : Initial Calibration

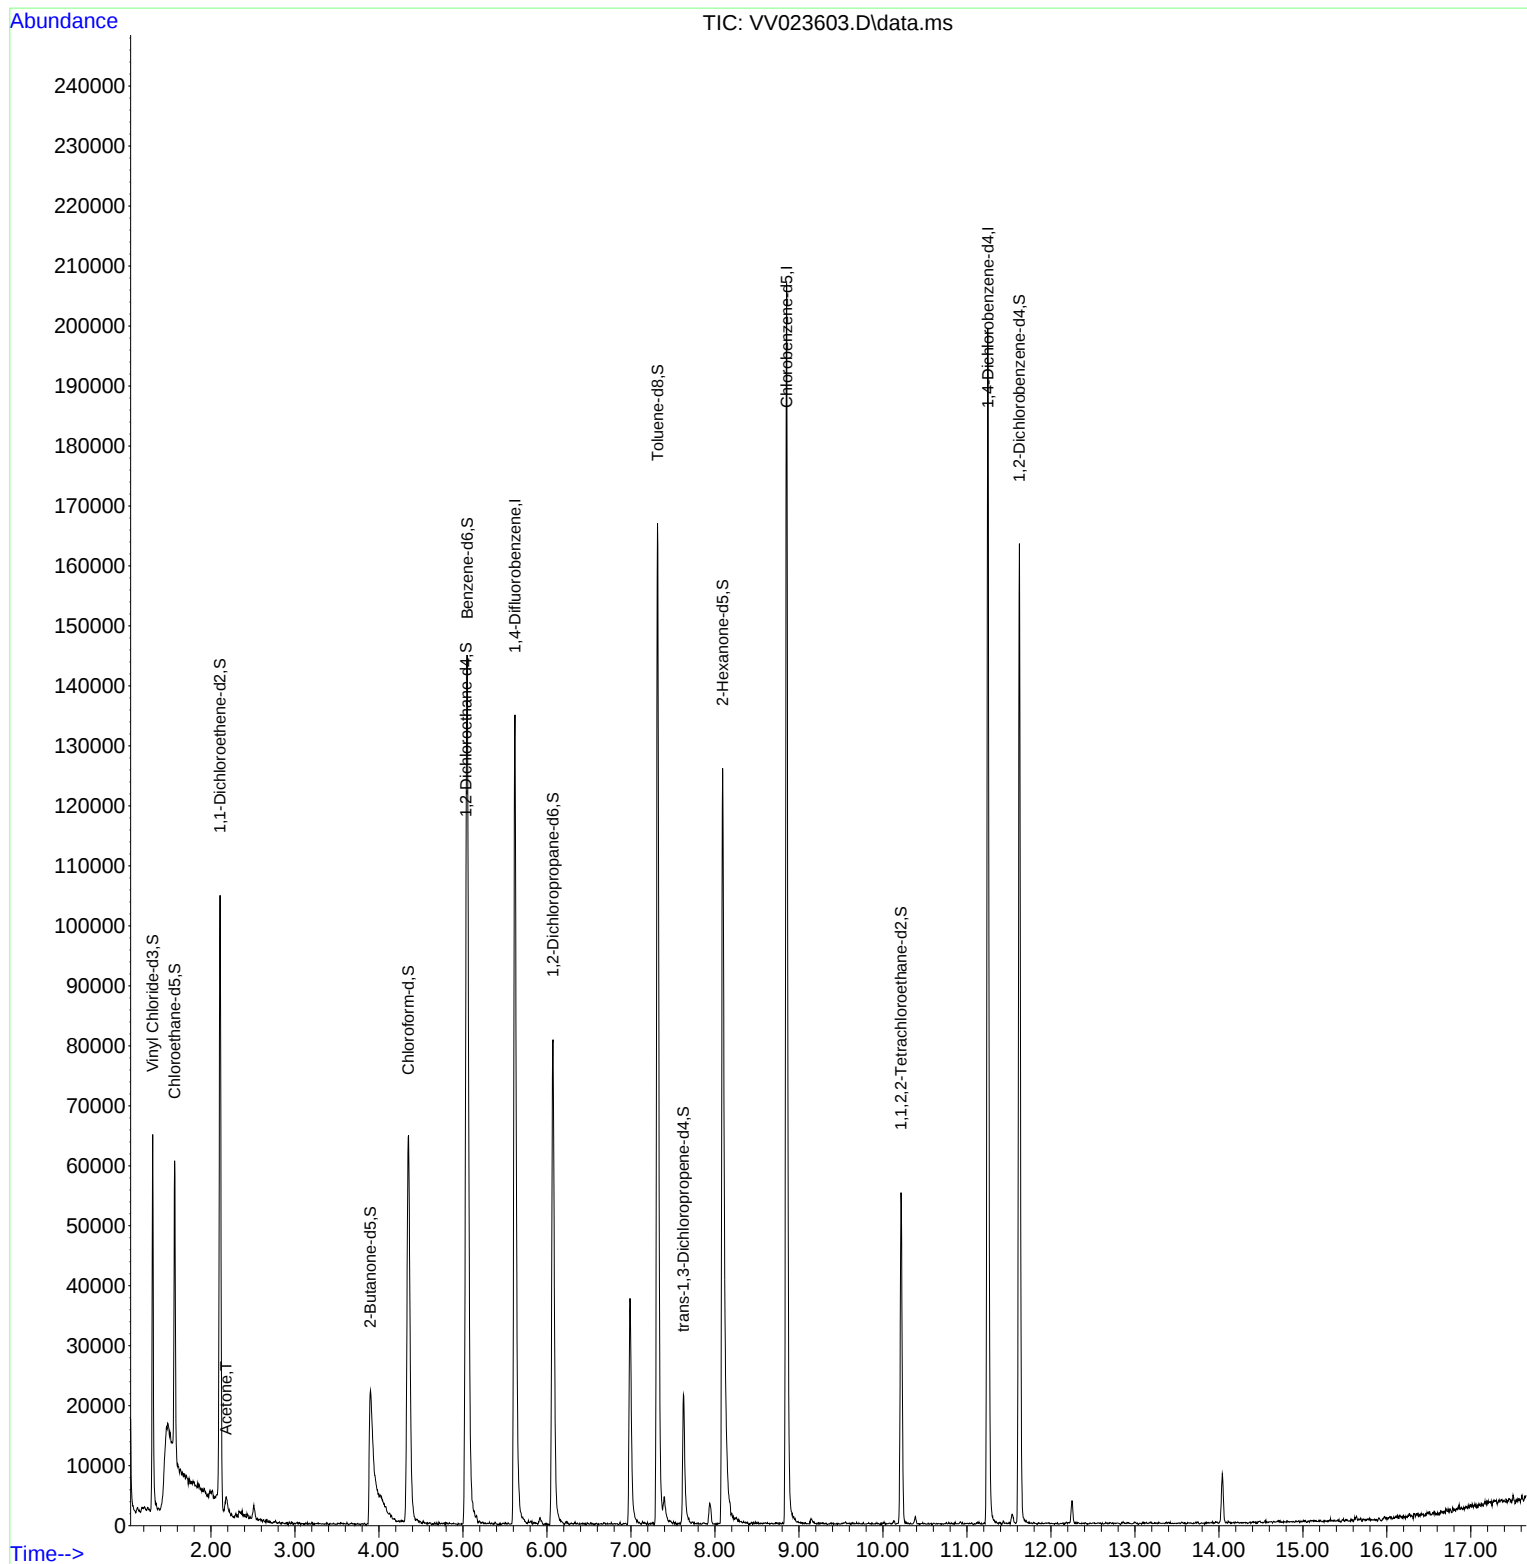

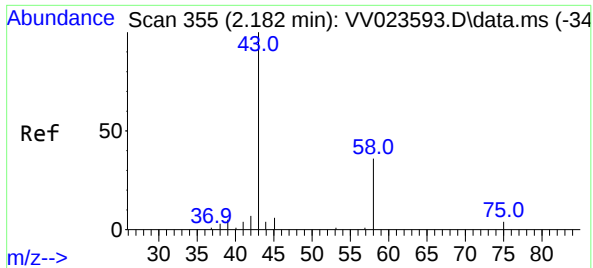

#13
Acetone
Concen: 8.092 ug/L
RT: 2.179 min Scan# 31
Delta R.T. -0.003 min
Lab File: VV023603.D
Acq: 18 Nov 2021 14:48

Instrument :
MSVOA_V
ClientSampleId :
H4634

Tgt Ion: 43 Resp: 6375
Ion Ratio Lower Upper
43 100
58 33.4 0.0 55.4

