

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
 Data File : VV023598.D
 Acq On : 18 Nov 2021 12:48
 Operator : SY/MD
 Sample : M4627-15DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4642DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023598.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.214	49	54	66	rVB	4592	4868	1.38%	0.152%
2	1.304	75	82	91	rBV	64716	66028	18.75%	2.058%
3	1.565	156	163	178	rBV	50451	57627	16.36%	1.796%
4	2.105	321	331	346	rVB	104409	154031	43.74%	4.801%
5	2.507	445	456	473	rBV	25486	43038	12.22%	1.341%
6	2.767	523	537	550	rBV4	11182	23372	6.64%	0.728%
7	3.912	879	893	912	rBV3	51526	149687	42.51%	4.666%
8	4.349	1014	1029	1055	rBV	61950	157172	44.63%	4.899%
9	5.050	1230	1247	1277	rBV3	138934	352153	100.00%	10.976%
10	5.619	1412	1424	1455	rBV	122245	251693	71.47%	7.845%
11	5.915	1499	1516	1540	rBV	97639	196581	55.82%	6.127%
12	6.069	1552	1564	1584	rBV	78953	163820	46.52%	5.106%
13	6.989	1838	1850	1870	rBV	36821	69754	19.81%	2.174%
14	7.317	1940	1952	1973	rBV	162920	289169	82.11%	9.013%
15	7.625	2039	2048	2062	rBV	20812	37844	10.75%	1.180%
16	7.979	2149	2158	2167	rVB3	4526	7349	2.09%	0.229%
17	8.092	2179	2193	2234	rBV	106443	263631	74.86%	8.217%
18	8.854	2419	2430	2460	rBV	190341	315368	89.55%	9.830%
19	10.217	2843	2854	2867	rBV	52909	84022	23.86%	2.619%
20	11.249	3161	3175	3197	rBV	177100	278308	79.03%	8.675%
21	11.625	3281	3292	3312	rBV	151710	242757	68.94%	7.567%




Sum of corrected areas: 3208272

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
Data File : VV023598.D
Acq On : 18 Nov 2021 12:48
Operator : SY/MD
Sample : M4627-15DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4642DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

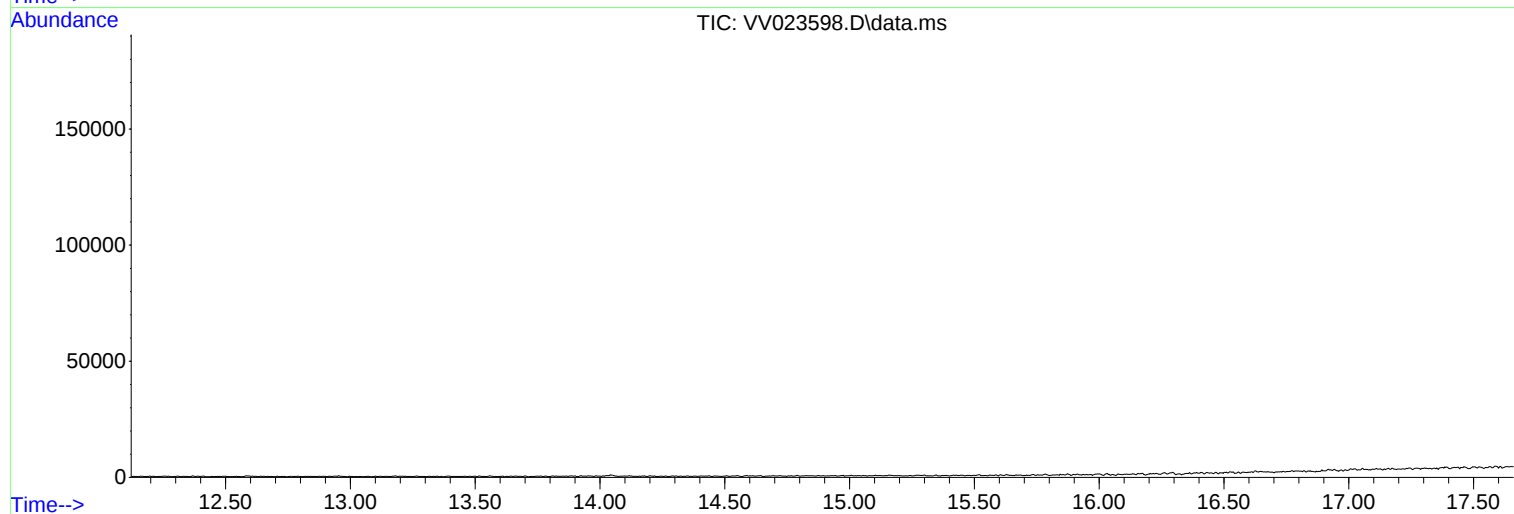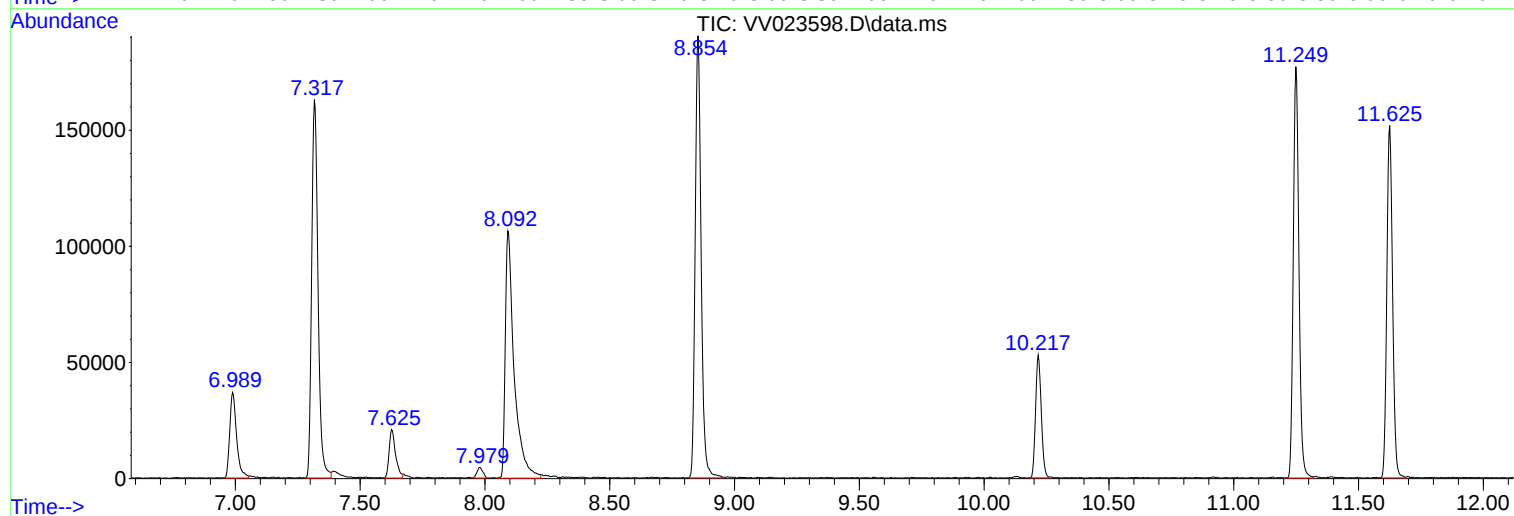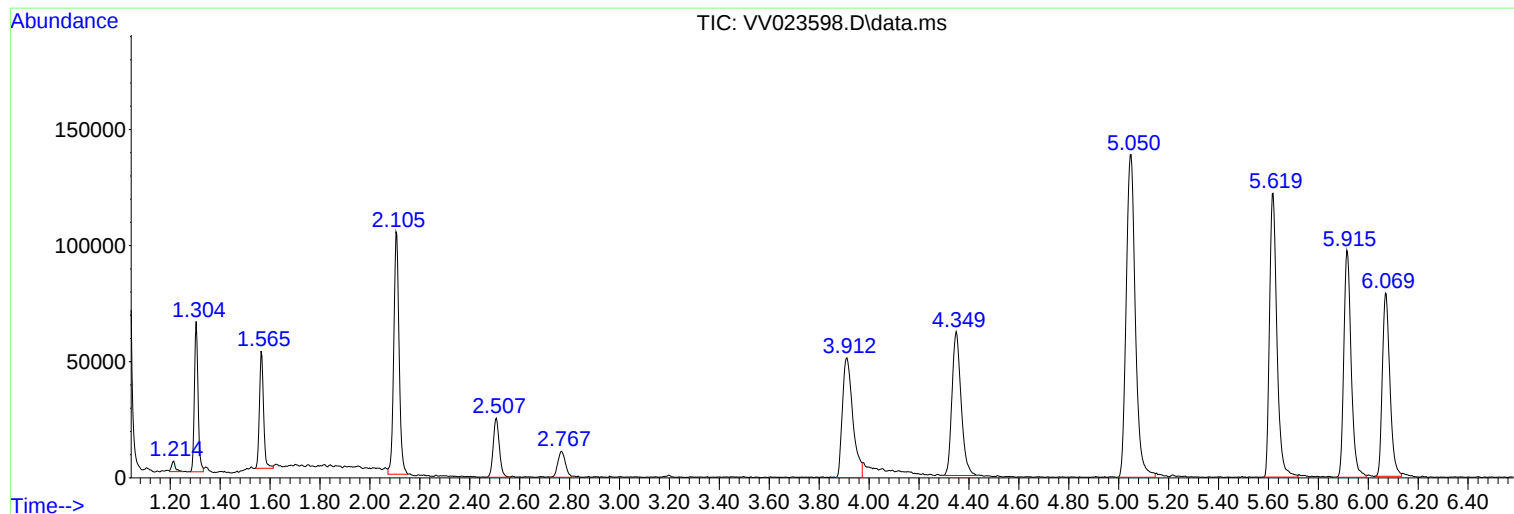

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
Data File : VV023598.D
Acq On : 18 Nov 2021 12:48
Operator : SY/MD
Sample : M4627-15DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4642DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
Data File : VV023598.D
Acq On : 18 Nov 2021 12:48
Operator : SY/MD
Sample : M4627-15DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4642DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc