

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
 Data File : VV023606.D
 Acq On : 18 Nov 2021 16:00
 Operator : SY/MD
 Sample : M4627-15DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4642DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023606.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	96	rBV	70412	72148	19.63%	2.148%
2	1.568	156	164	175	rBV	51650	59168	16.10%	1.762%
3	2.108	322	332	347	rVB	102659	149935	40.79%	4.464%
4	2.506	446	456	471	rBV2	25008	43107	11.73%	1.283%
5	2.767	528	537	555	rBV5	13443	27843	7.58%	0.829%
6	3.912	879	893	917	rBV2	118828	320506	87.20%	9.542%
7	4.352	1014	1030	1056	rBV	64622	166647	45.34%	4.961%
8	5.050	1231	1247	1275	rBV2	146631	367537	100.00%	10.942%
9	5.619	1410	1424	1445	rBV	130205	265308	72.19%	7.899%
10	5.921	1508	1518	1533	rBV5	15694	34350	9.35%	1.023%
11	6.072	1551	1565	1586	rBV2	81243	171998	46.80%	5.121%
12	6.989	1836	1850	1871	rBV3	38594	74560	20.29%	2.220%
13	7.317	1941	1952	1973	rBV	168455	297650	80.99%	8.861%
14	7.625	2039	2048	2069	rBV3	22425	42694	11.62%	1.271%
15	8.091	2182	2193	2227	rBV2	128124	286957	78.08%	8.543%
16	8.853	2419	2430	2451	rBV	204114	329693	89.70%	9.815%
17	10.217	2842	2854	2869	rBV	59498	93909	25.55%	2.796%
18	11.249	3165	3175	3195	rBV	198007	299551	81.50%	8.918%
19	11.625	3280	3292	3308	rBV	158855	255356	69.48%	7.602%




Sum of corrected areas: 3358917

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
Data File : VV023606.D
Acq On : 18 Nov 2021 16:00
Operator : SY/MD
Sample : M4627-15DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4642DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

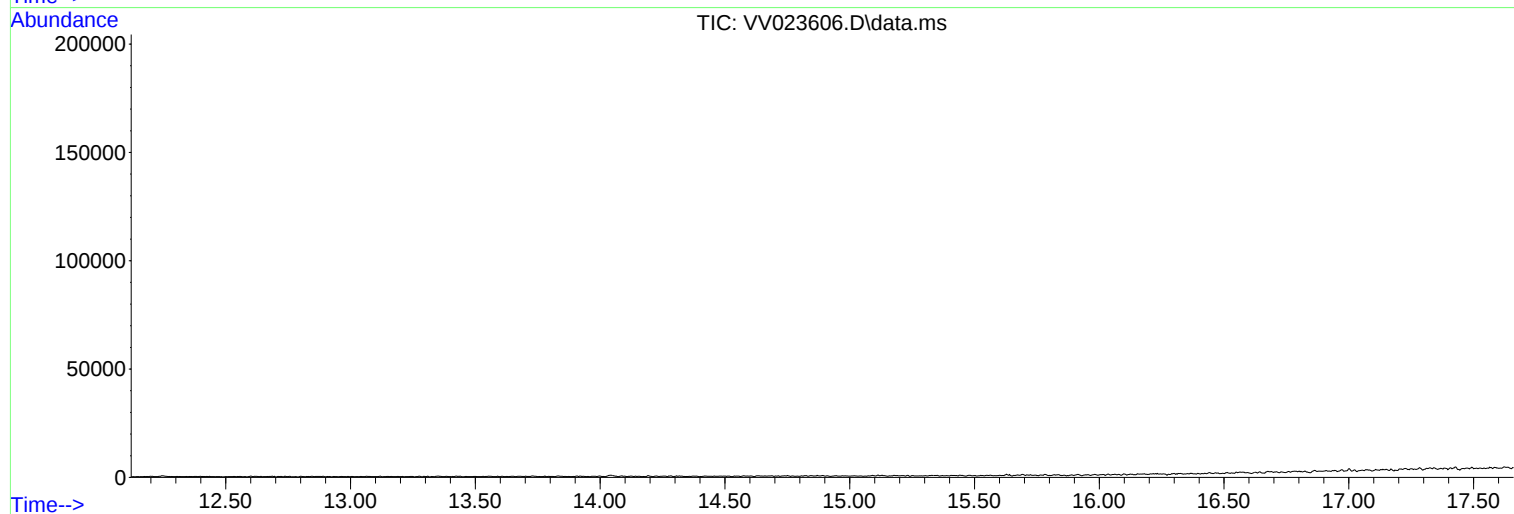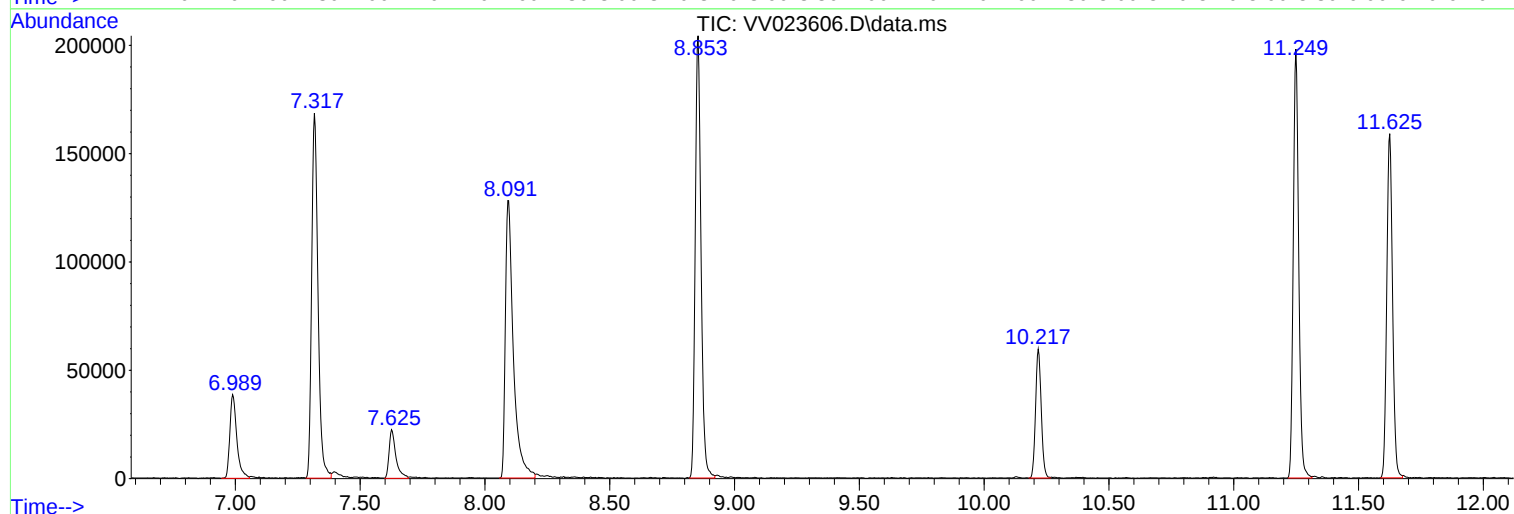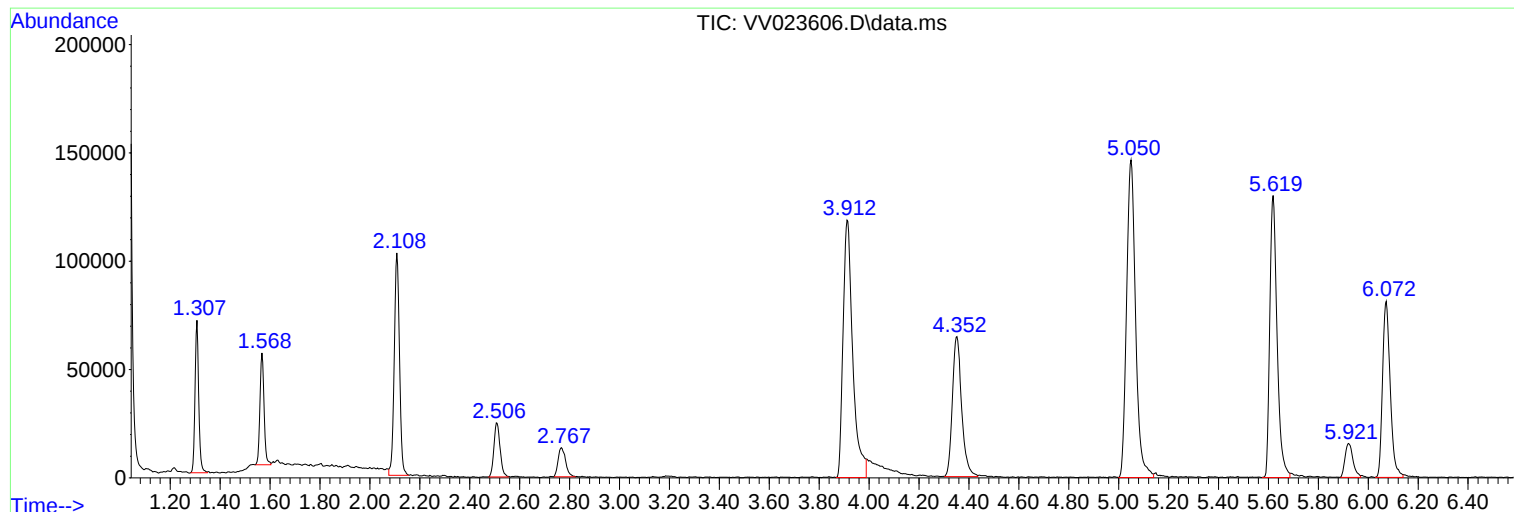

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
Data File : VV023606.D
Acq On : 18 Nov 2021 16:00
Operator : SY/MD
Sample : M4627-15DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4642DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111821\
Data File : VV023606.D
Acq On : 18 Nov 2021 16:00
Operator : SY/MD
Sample : M4627-15DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4642DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc